

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079872.D
 Acq On : 10 Jun 2015 18:45
 Operator : TP/IZ
 Sample : G2523-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LIP-16-6-3-15

Quant Time: Jun 11 02:13:31 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 00:53:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	54581	20.00	ng	0.00
21) Naphthalene-d8	8.71	136	216903	20.00	ng	0.00
38) Acenaphthene-d10	10.48	164	106876	20.00	ng	-0.01
63) Phenanthrene-d10	11.99	188	224221	20.00	ng	-0.01
75) Chrysene-d12	14.90	240	221364	20.00	ng	-0.17
86) Perylene-d12	16.78	264	203533	20.00	ng	-0.25
System Monitoring Compounds						
5) 2-Fluorophenol	6.03	112	182880	55.22	ng	0.00
7) Phenol-d6	7.02	99	144959	33.83	ng	0.00
23) Nitrobenzene-d5	7.98	82	295141	78.61	ng	0.00
41) 2,4,6-Tribromophenol	11.28	330	127763	138.13	ng	0.00
44) 2-Fluorobiphenyl	9.78	172	743023	97.78	ng	0.00
78) Terphenyl-d14	13.66	244	913167	93.00	ng	-0.08


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079872.D
Acq On : 10 Jun 2015 18:45
Operator : TP/IZ
Sample : G2523-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LIP-16-6-3-15

Quant Time: Jun 11 02:13:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

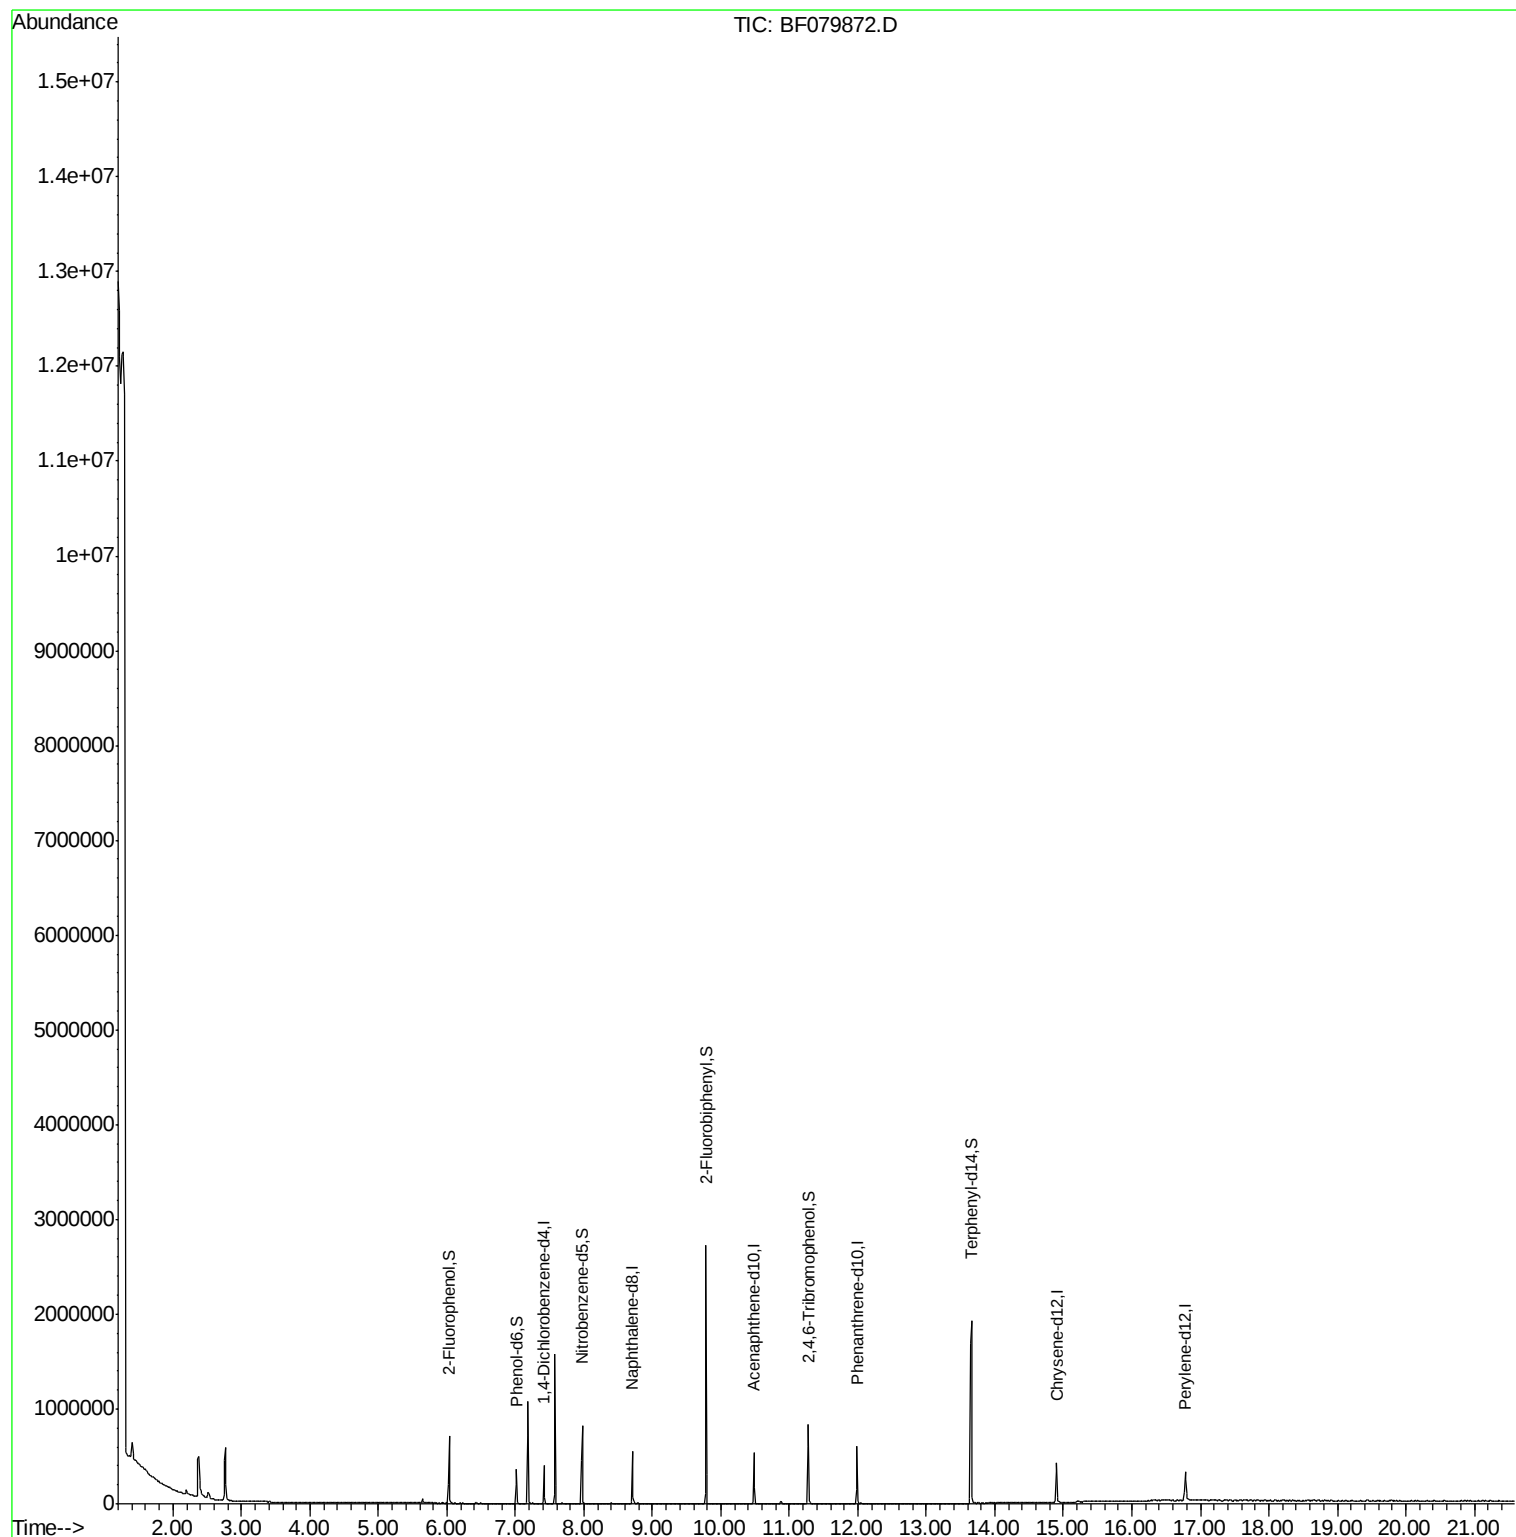




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.42 min Scan# 545
Delta R.T. 0.00 min
Lab File: BF079872.D
Acq: 10 Jun 2015 18:45

Instrument :
BNA_F
ClientSampleId :
LIP-16-6-3-15

Tgt Ion:152 Resp: 54581
Ion Ratio Lower Upper
152 100
150 157.6 131.4 197.2
115 60.0 56.5 84.7

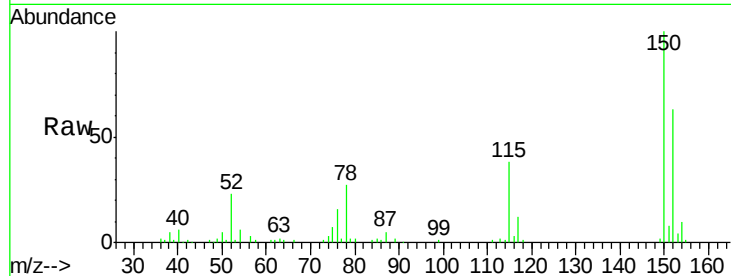


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

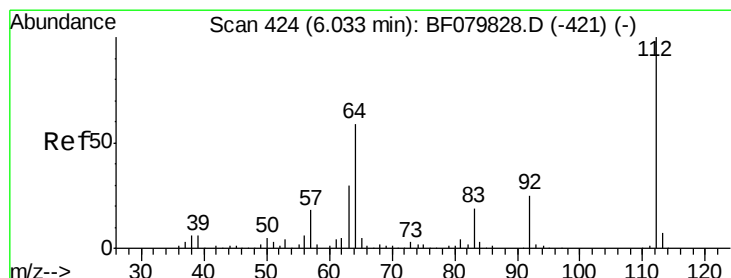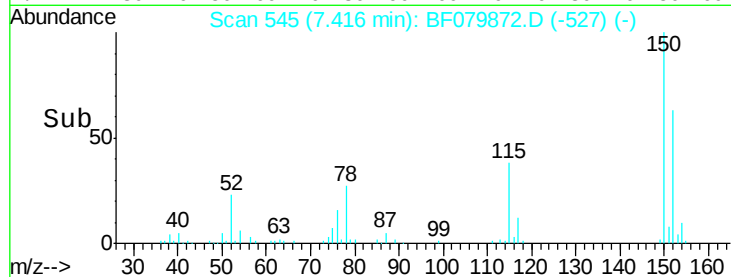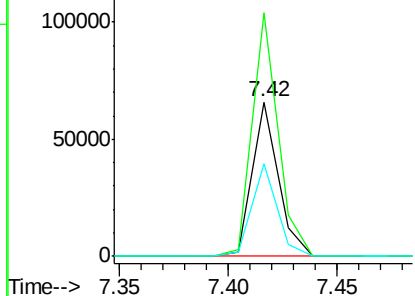



#5


2-Fluorophenol
Concen: 55.22 ng
RT: 6.03 min Scan# 424
Delta R.T. 0.00 min
Lab File: BF079872.D
Acq: 10 Jun 2015 18:45

Tgt Ion:112 Resp: 182880
Ion Ratio Lower Upper
112 100
64 56.3 44.2 66.4
63 28.5 22.8 34.2

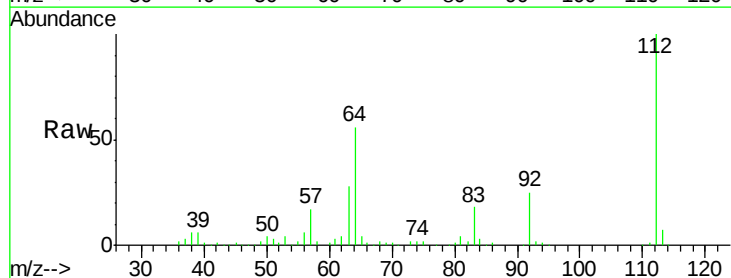

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

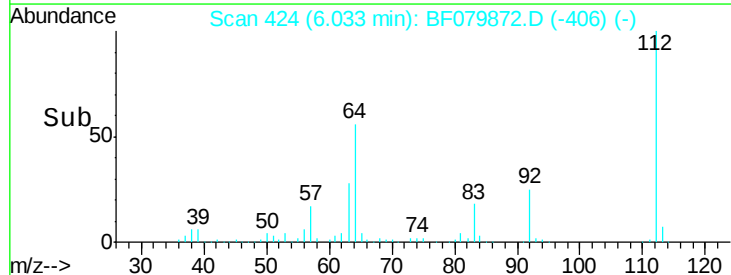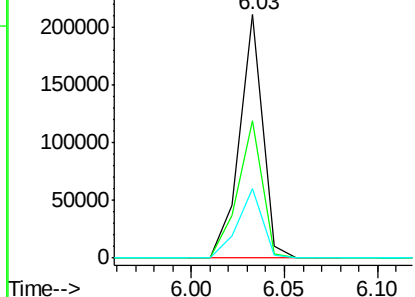

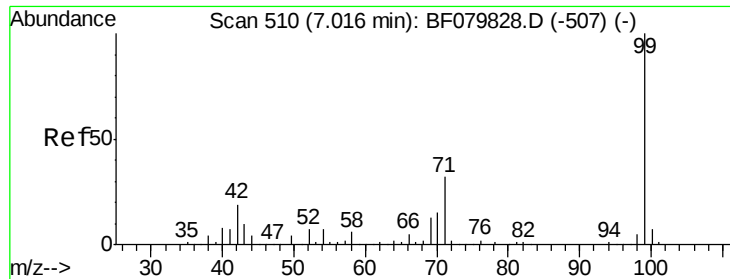

#7

Phenol-d6

Concen: 33.83 ng

RT: 7.02 min Scan# 510

Delta R.T. 0.00 min

Lab File: BF079872.D

Acq: 10 Jun 2015 18:45

Instrument :

BNA_F

ClientSampleId :

LIP-16-6-3-15


Tgt Ion: 99 Resp: 144959

Ion Ratio Lower Upper




99 100

42 15.8 13.7 20.5

71 28.6 25.1 37.7

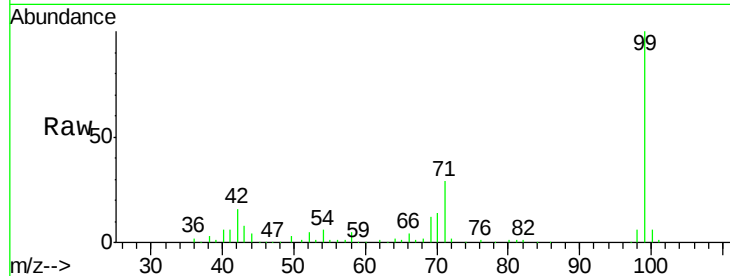

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

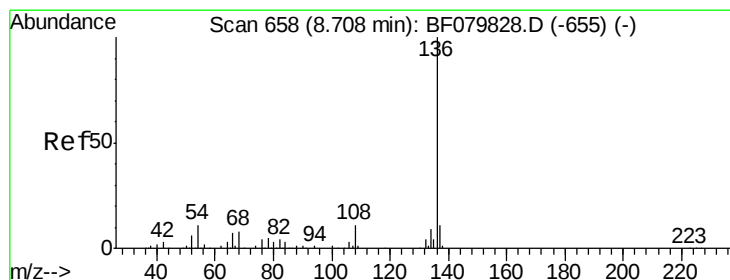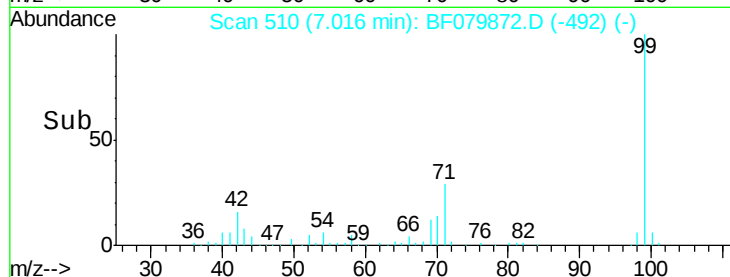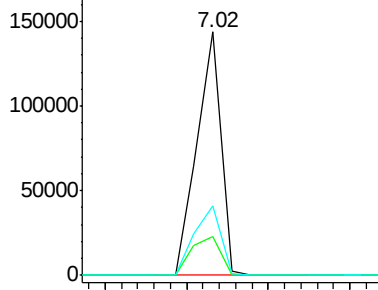

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.71 min Scan# 658

Delta R.T. 0.00 min

Lab File: BF079872.D

Acq: 10 Jun 2015 18:45

Tgt Ion: 136 Resp: 216903


Ion Ratio Lower Upper

136 100



137 10.7 9.3 13.9

54 8.7 8.1 12.1

68 6.6 4.8 7.2

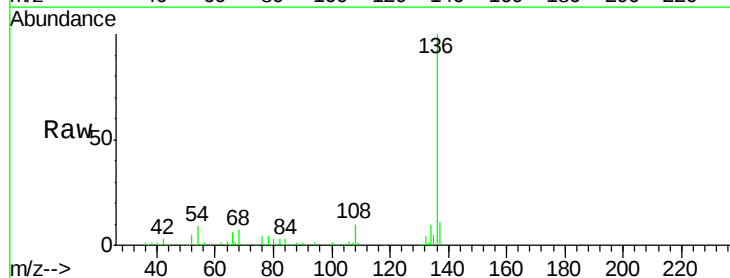

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

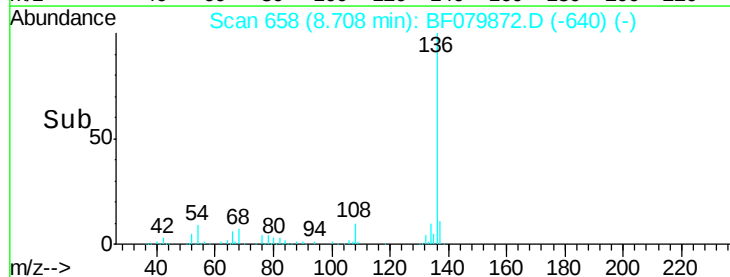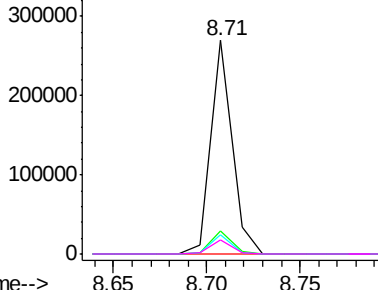







#23
 Nitrobenzene-d5
 Concen: 78.61 ng
 RT: 7.98 min Scan# 594
 Delta R.T. 0.00 min
 Lab File: BF079872.D
 Acq: 10 Jun 2015 18:45

Instrument :
 BNA_F
 ClientSampleId :
 LIP-16-6-3-15

Tgt Ion: 82 Resp: 295141
 Ion Ratio Lower Upper
 82 100
 128 50.7 35.2 52.8
 54 46.6 39.2 58.8

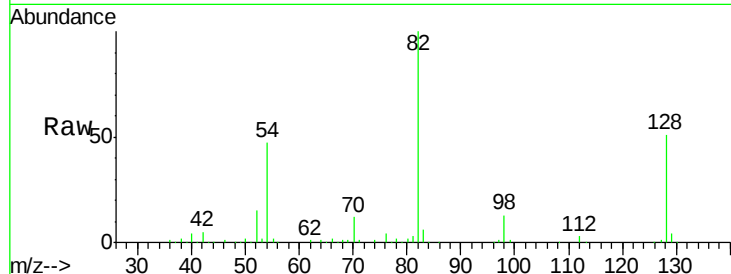


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

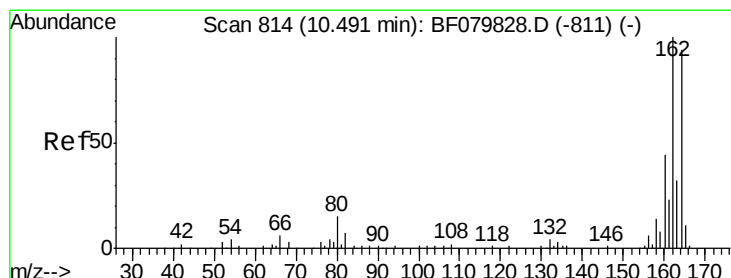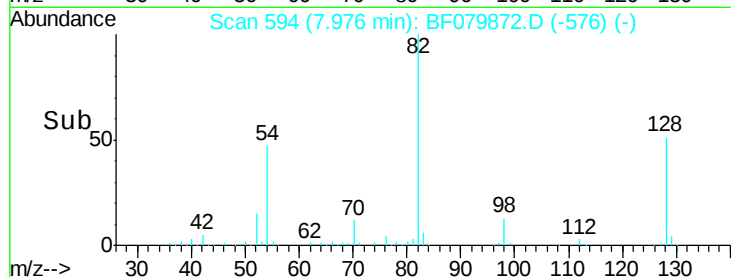
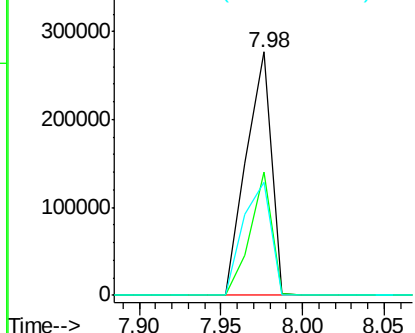



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.48 min Scan# 813
 Delta R.T. -0.01 min
 Lab File: BF079872.D
 Acq: 10 Jun 2015 18:45

Tgt Ion: 164 Resp: 106876
 Ion Ratio Lower Upper
 164 100
 162 103.4 89.8 134.8
 160 46.0 39.6 59.4

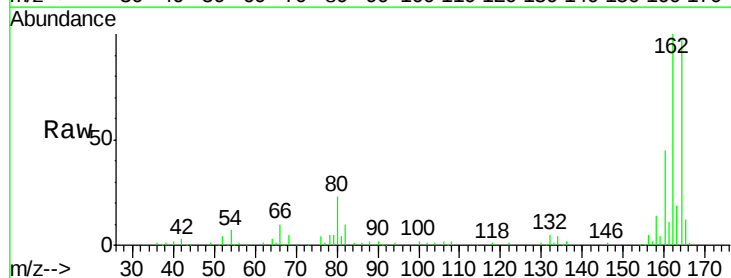

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

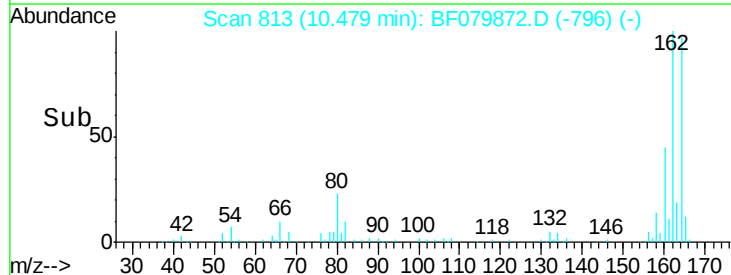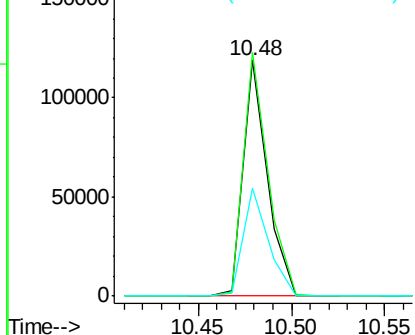


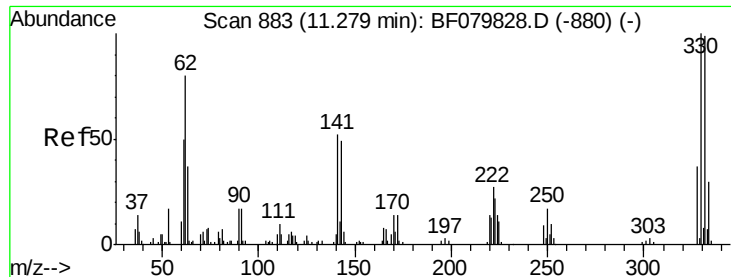




#41
 2,4,6-Tribromophenol
 Concen: 138.13 ng
 RT: 11.28 min Scan# 883
 Delta R.T. 0.00 min
 Lab File: BF079872.D
 Acq: 10 Jun 2015 18:45

Instrument :
 BNA_F
 ClientSampleId :
 LIP-16-6-3-15

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.8	115.2
141	33.2	29.1	43.7

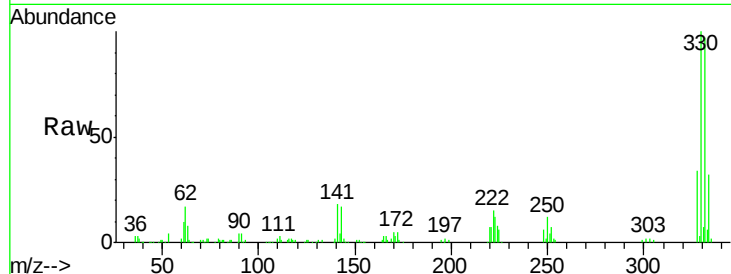


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

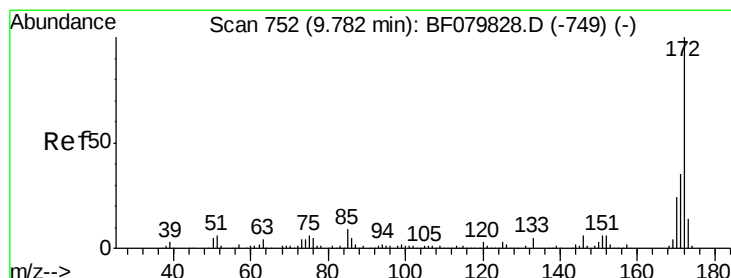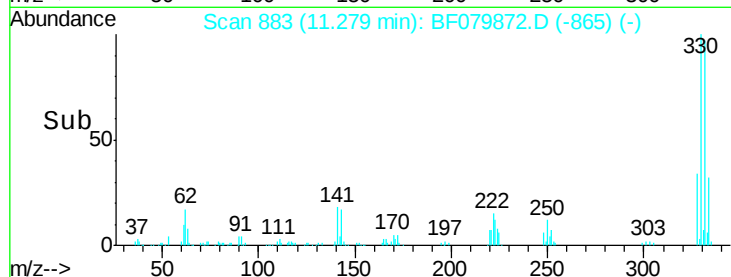
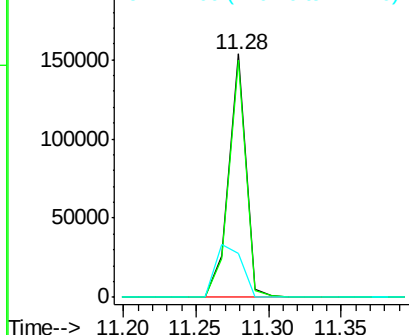



#44
 2-Fluorobiphenyl
 Concen: 97.78 ng
 RT: 9.78 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: BF079872.D
 Acq: 10 Jun 2015 18:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	28.5	42.7
170	23.8	18.8	28.2

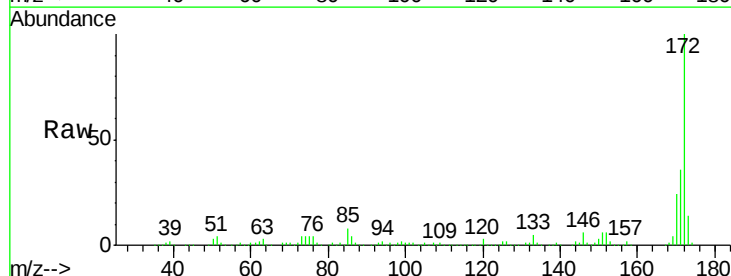

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



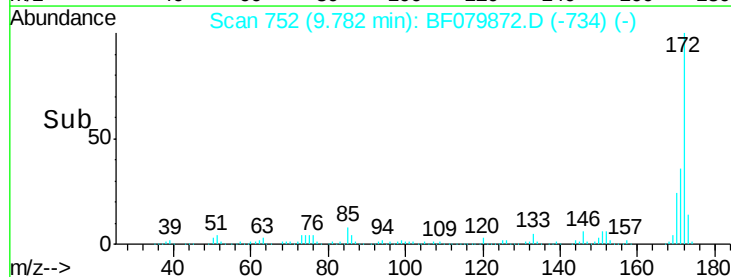
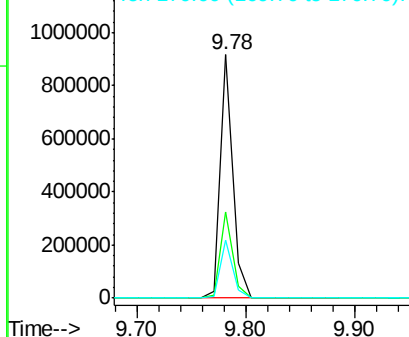


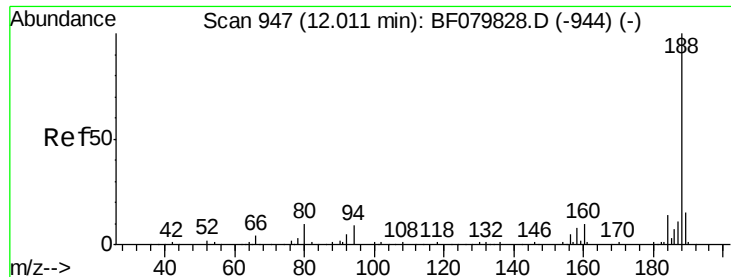

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.99 min Scan# 945
Delta R.T. -0.01 min
Lab File: BF079872.D
Acq: 10 Jun 2015 18:45




Instrument :
BNA_F
ClientSampleId :
LIP-16-6-3-15


Tgt Ion:188 Resp: 224221
Ion Ratio Lower Upper
188 100
94 8.2 7.4 11.0
80 8.3 8.0 12.0

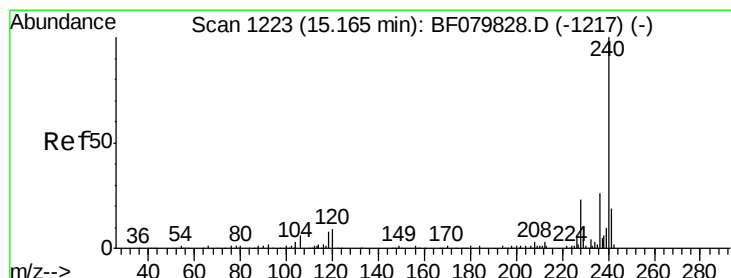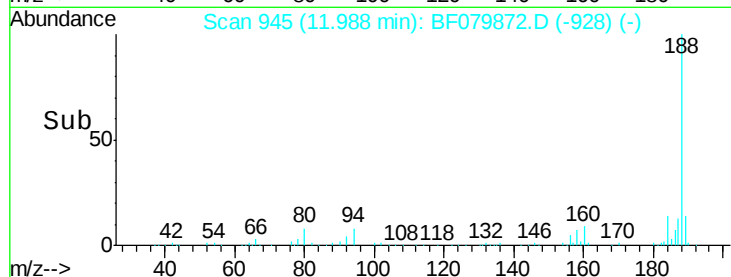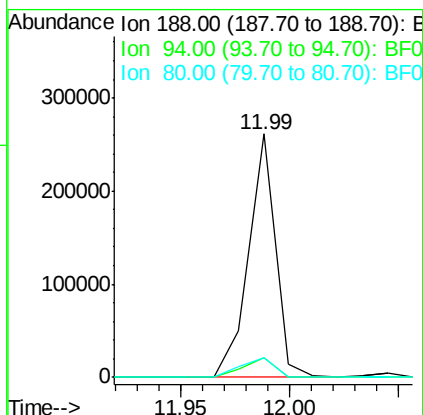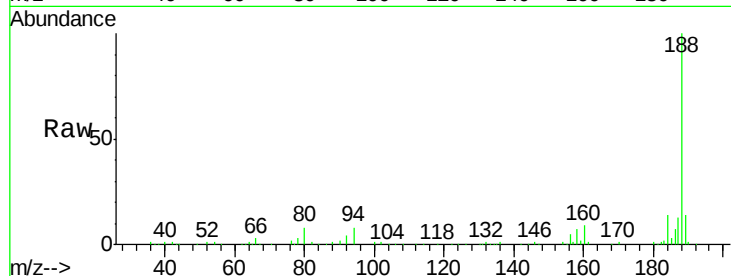

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.90 min Scan# 1200
Delta R.T. -0.17 min
Lab File: BF079872.D
Acq: 10 Jun 2015 18:45

Tgt Ion:240 Resp: 221364
Ion Ratio Lower Upper
240 100
120 7.4 6.6 9.8
236 25.7 20.2 30.4

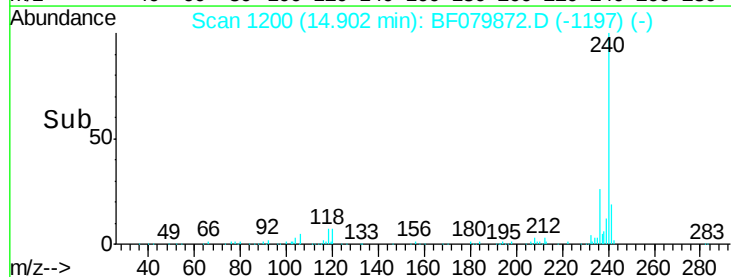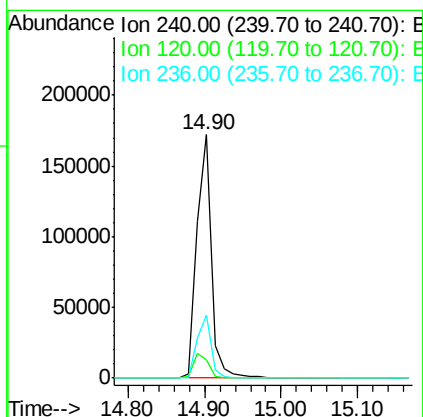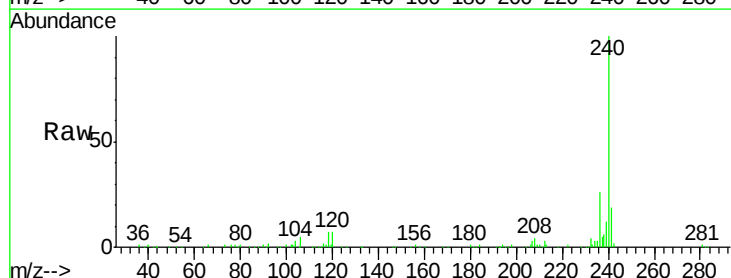

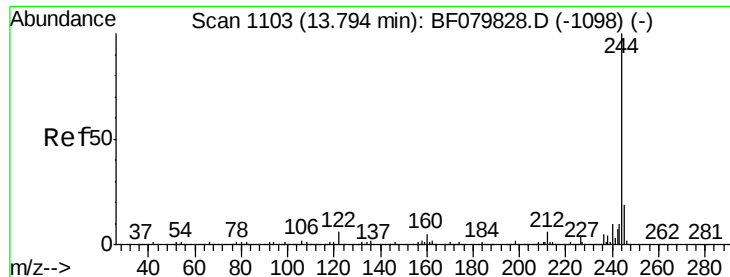

#78

Terphenyl-d14

Concen: 93.00 ng

RT: 13.66 min Scan# 1091

Delta R.T. -0.08 min

Lab File: BF079872.D

Acq: 10 Jun 2015 18:45

Instrument :

BNA_F

ClientSampleId :

LIP-16-6-3-15


Tgt Ion:244 Resp: 913167

Ion Ratio Lower Upper

244 100

212 6.3 5.6 8.4




122 6.6 8.2 12.2#

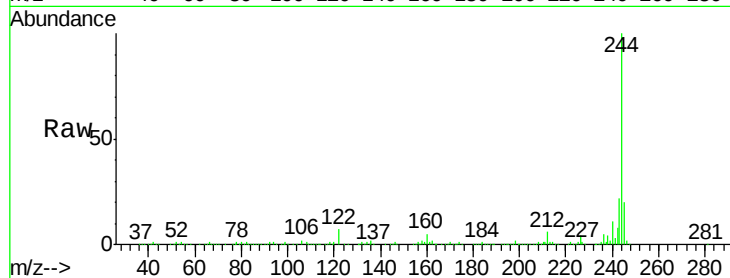

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

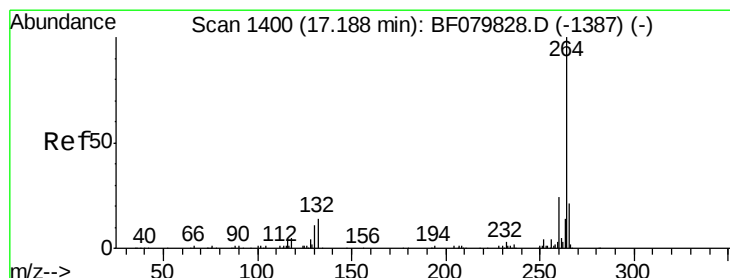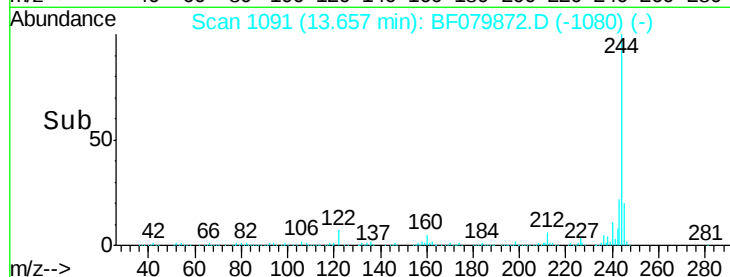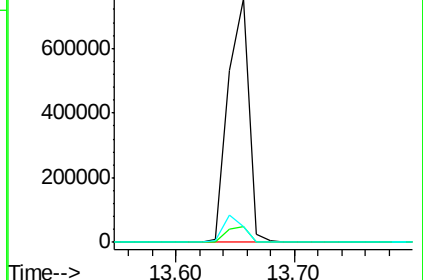

#86

Perylene-d12

Concen: 20.00 ng

RT: 16.78 min Scan# 1364

Delta R.T. -0.25 min

Lab File: BF079872.D

Acq: 10 Jun 2015 18:45


Tgt Ion:264 Resp: 203533

Ion Ratio Lower Upper

264 100

260 23.5 19.5 29.3

265 22.1 18.0 27.0

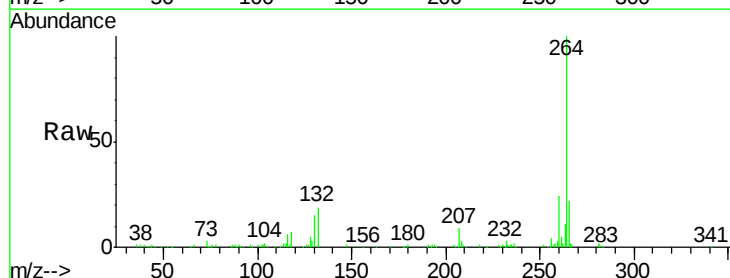

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

