

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079858.D
Acq On : 10 Jun 2015 11:56
Operator : TP/IZ
Sample : G2580-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.404	17	19	21	rVB	204093	193254	11.08%	4.589%
2	2.376	101	104	115	rVB	866403	1744340	100.00%	41.417%
3	7.416	543	545	548	rBV	317518	255476	14.65%	6.066%
4	8.708	656	658	660	rBV	436118	348586	19.98%	8.277%
5	10.479	811	813	816	rBV	413714	387776	22.23%	9.207%
6	11.999	944	946	949	rBV	502842	428729	24.58%	10.180%
7	15.074	1212	1215	1218	rBV	399496	437387	25.07%	10.385%
8	17.029	1383	1386	1397	rBV	249744	416114	23.86%	9.880%


Sum of corrected areas: 4211662

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079858.D
Acq On : 10 Jun 2015 11:56
Operator : TP/IZ
Sample : G2580-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

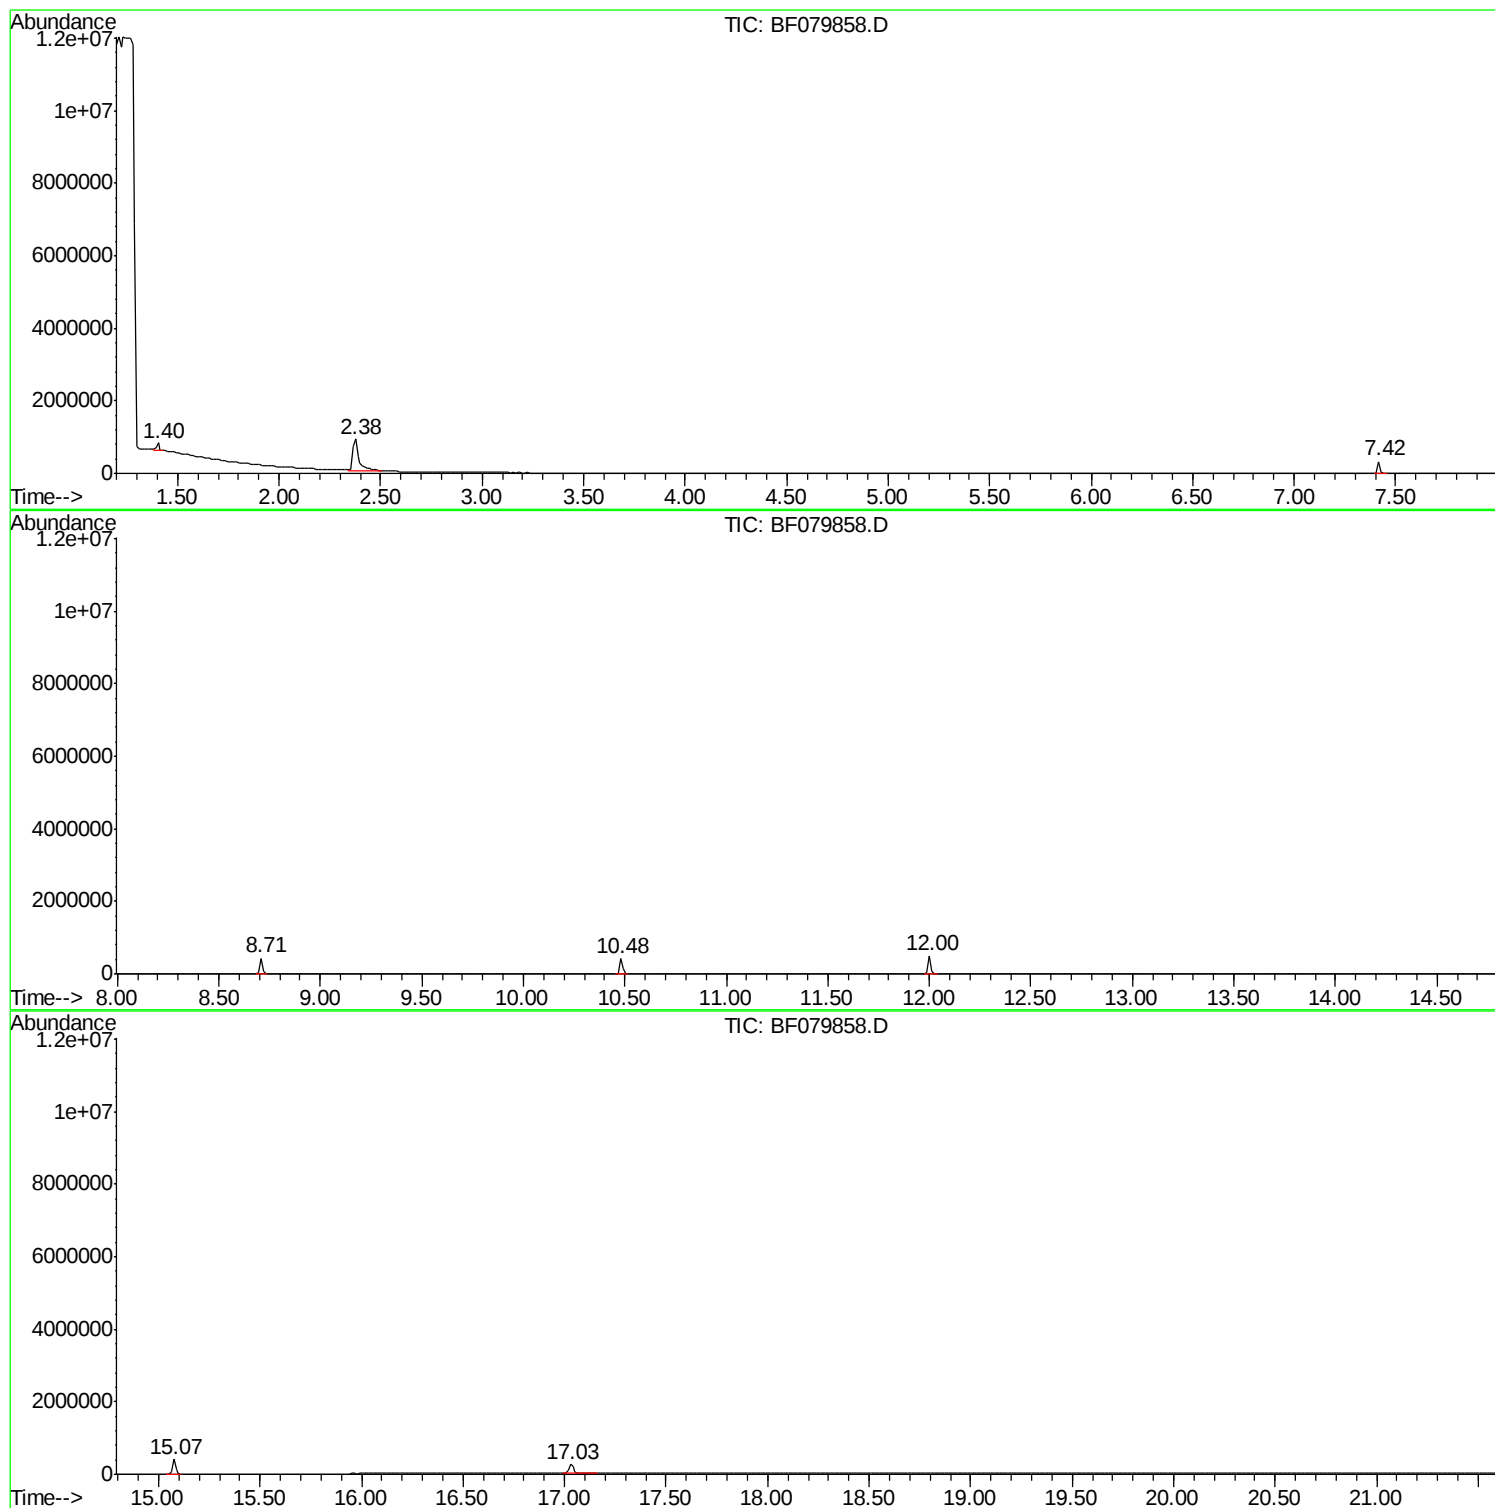

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079858.D
Acq On : 10 Jun 2015 11:56
Operator : TP/IZ
Sample : G2580-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, 1,2-dichloro-, (E)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.40	15.13 ng	193254	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethene, 1,2-dichloro-, (E)-	96	C2H2Cl2	000156-60-5	91
2		Ethene, 1,1-dichloro-	96	C2H2Cl2	000075-35-4	91
3		Ethene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	91
4		1,2-Dichloroethylene	96	C2H2Cl2	000540-59-0	90
5		Chloromethylmethyl sulfide	96	C2H5ClS	002373-51-5	46

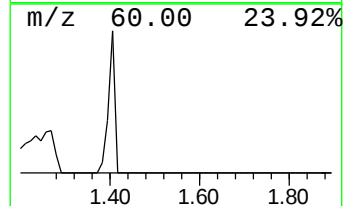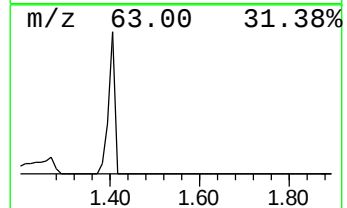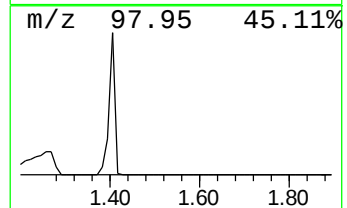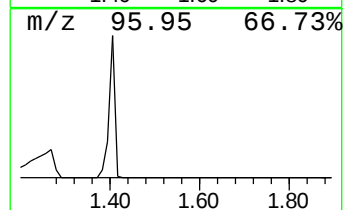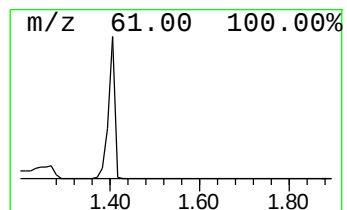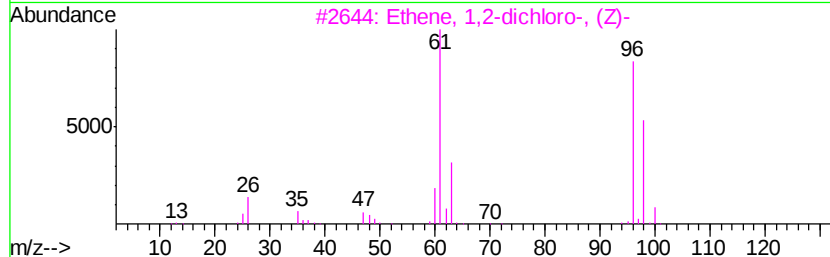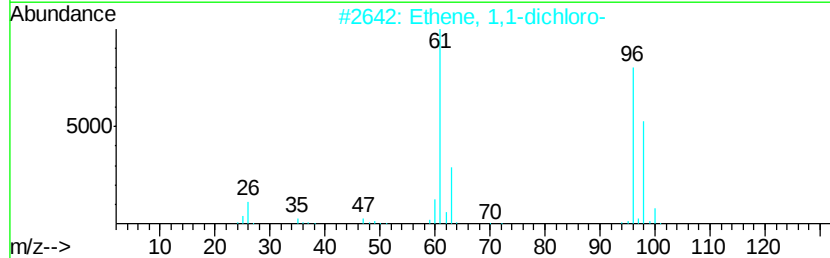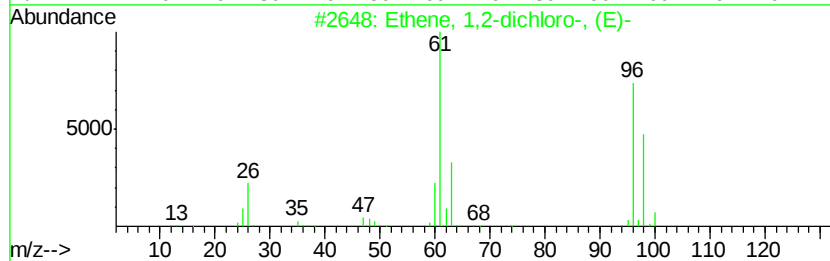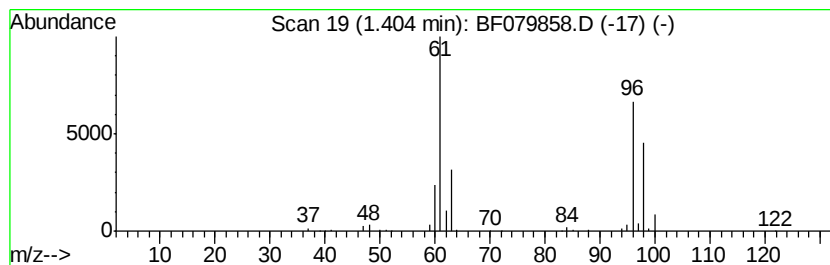

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079858.D
Acq On : 10 Jun 2015 11:56
Operator : TP/IZ
Sample : G2580-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, 1,2-dichl...	1.40	15.1	ng	193254	1	7.42	255476	20.0