

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079859.D
 Acq On : 10 Jun 2015 12:25
 Operator : TP/IZ
 Sample : PB83898BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83898BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	8	10	12	rVB2	12277317	16289986	100.00%	49.488%
2	2.181	86	87	98	rVB	317971	545459	3.35%	1.657%
3	2.341	98	101	102	rVV	1566469	2000679	12.28%	6.078%
4	2.364	102	103	132	rVB	496955	1124095	6.90%	3.415%
5	6.033	422	424	426	rBV	1595486	1319023	8.10%	4.007%
6	7.016	508	510	512	rBV	1649455	1404697	8.62%	4.267%
7	7.188	522	525	527	rBV	1259432	1335250	8.20%	4.056%
8	7.416	543	545	547	rVB	334259	280925	1.72%	0.853%
9	7.576	557	559	562	rBV	1320907	1085688	6.66%	3.298%
10	7.976	591	594	596	rBV	629549	684109	4.20%	2.078%
11	8.708	656	658	660	rBV	484129	387306	2.38%	1.177%
12	9.782	750	752	755	rBV	2111703	1718786	10.55%	5.222%
13	10.479	811	813	816	rVB	430089	436325	2.68%	1.326%
14	11.279	880	883	885	rBV	894503	815463	5.01%	2.477%
15	12.011	944	947	949	rBV	419037	467759	2.87%	1.421%
16	13.782	1099	1102	1104	rBV	2063893	2117416	13.00%	6.433%
17	15.143	1219	1221	1224	rBV	401178	476765	2.93%	1.448%
18	17.154	1394	1397	1406	rVB	263573	427541	2.62%	1.299%


Sum of corrected areas: 32917272

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079859.D
Acq On : 10 Jun 2015 12:25
Operator : TP/IZ
Sample : PB83898BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83898BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

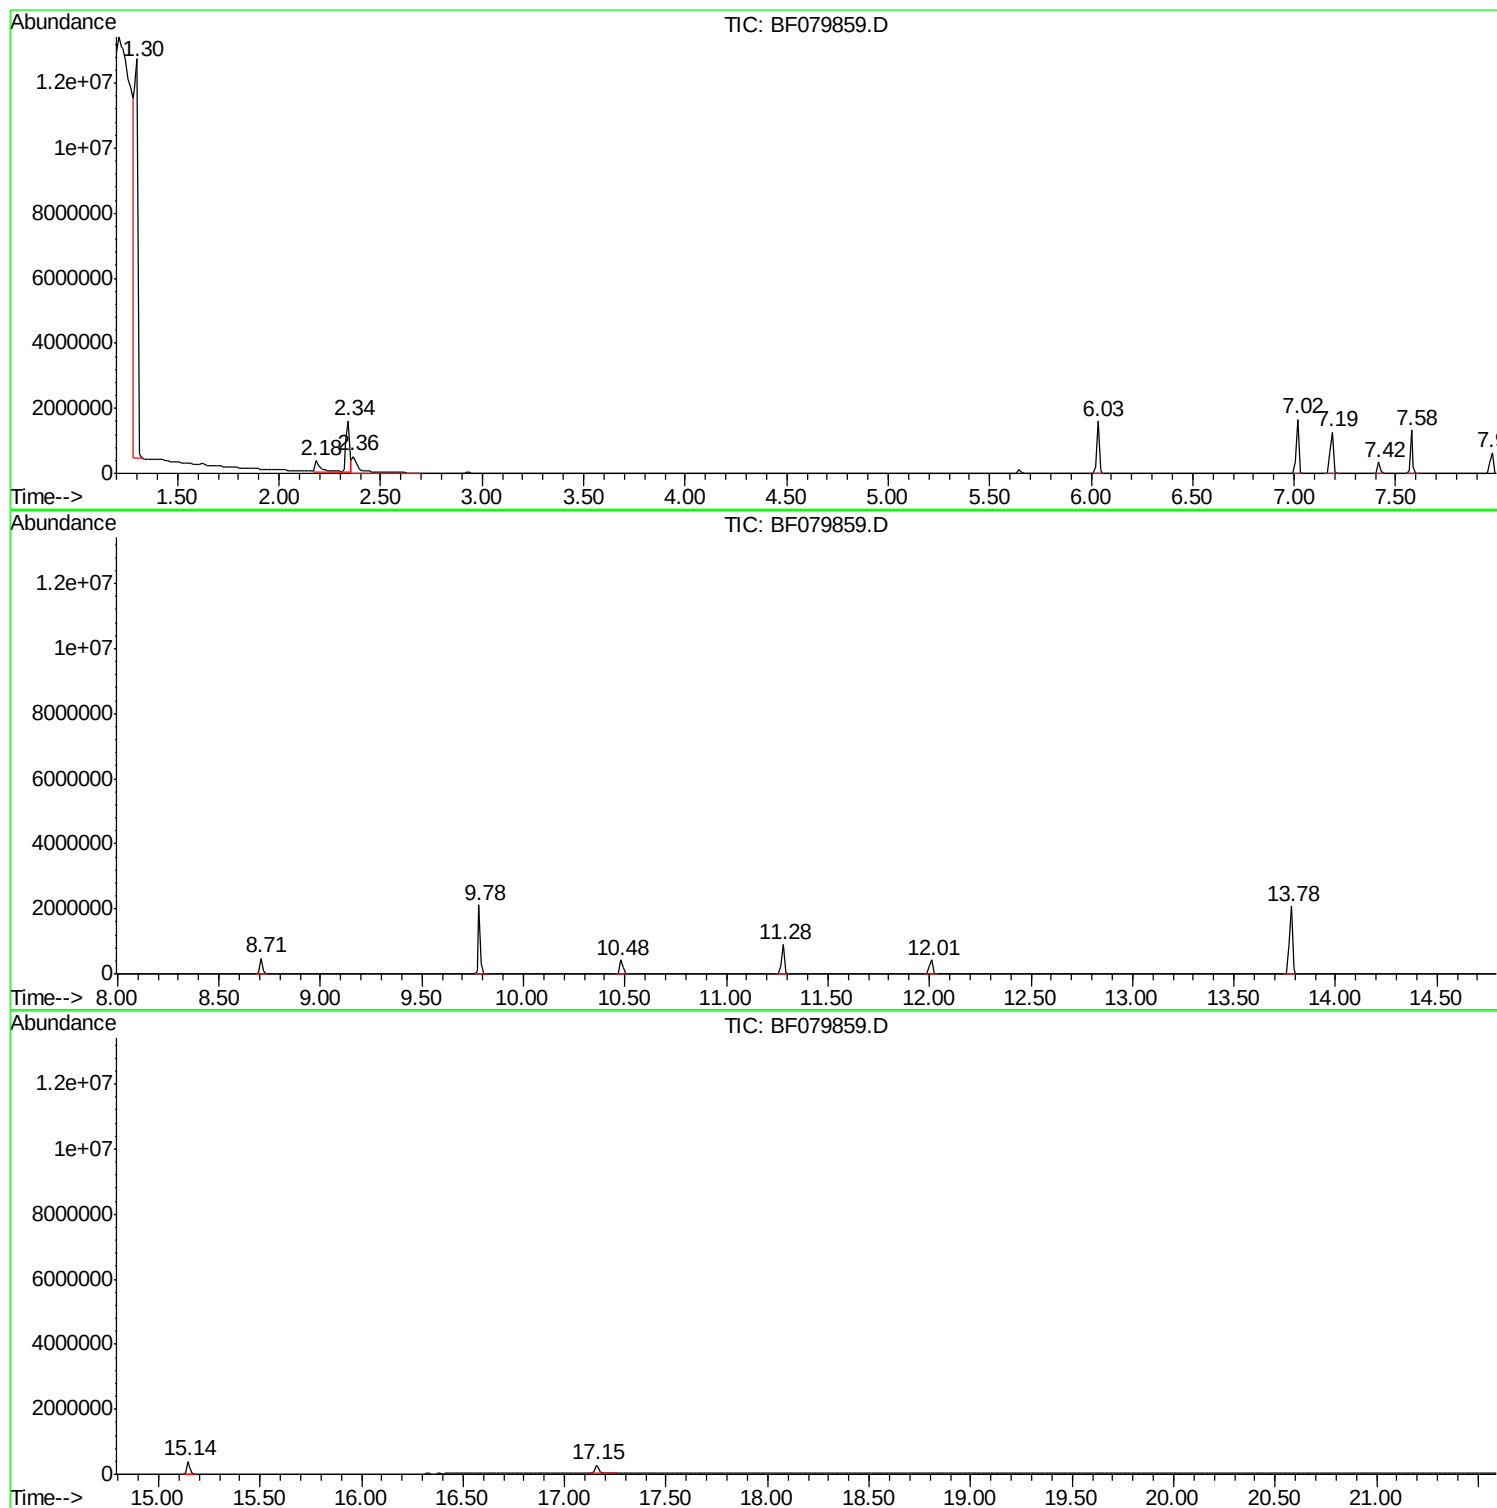

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079859.D
Acq On : 10 Jun 2015 12:25
Operator : TP/IZ
Sample : PB83898BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83898BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Propane, 2,2-dimethoxy- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.34	142.44 ng	2000680	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	72
2		Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
3		1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9
4		2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
5		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

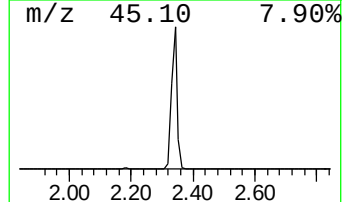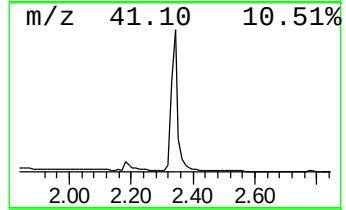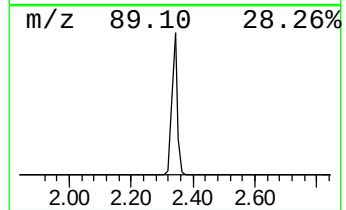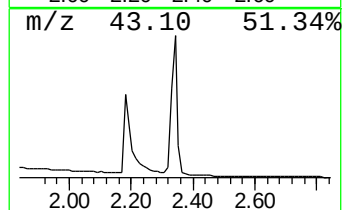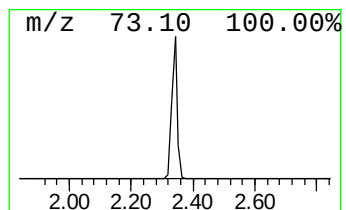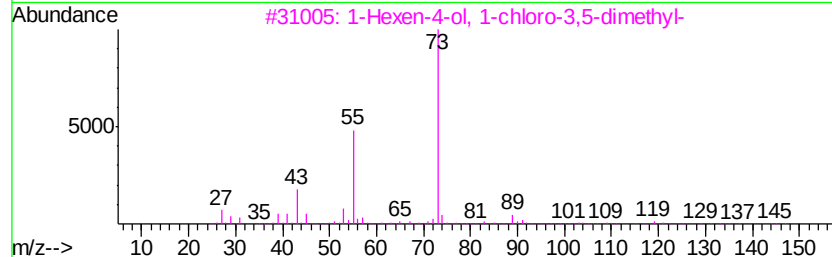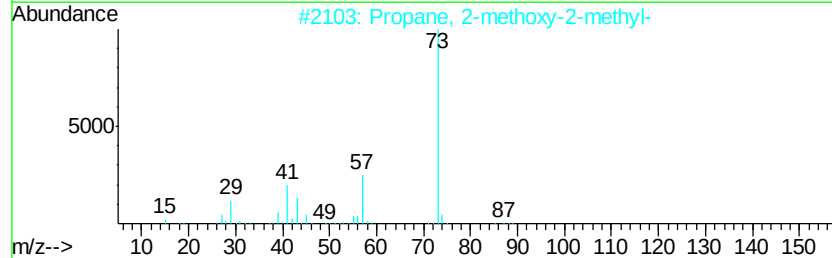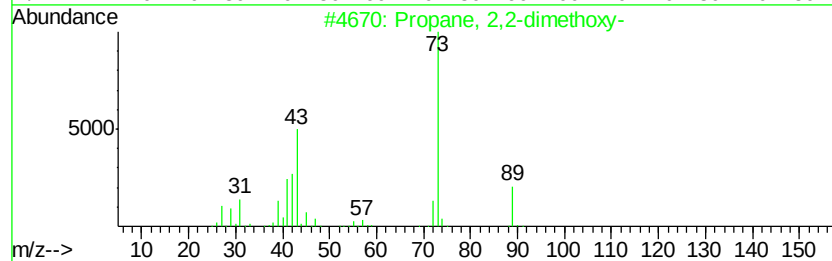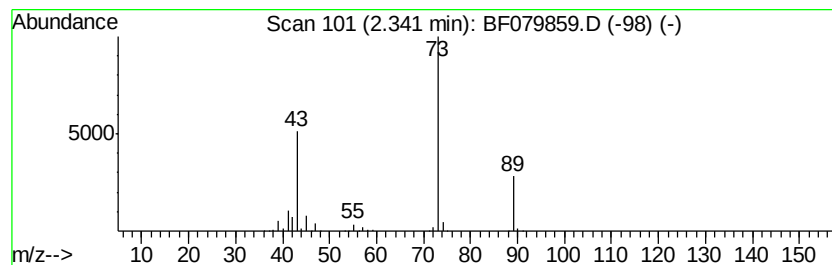

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079859.D
Acq On : 10 Jun 2015 12:25
Operator : TP/IZ
Sample : PB83898BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83898BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown7.19 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	95.06 ng	1335250	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Xenon	132	Xe	007440-63-3	9

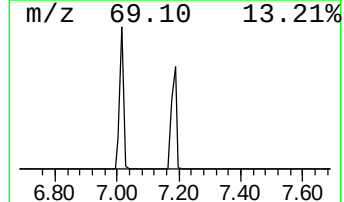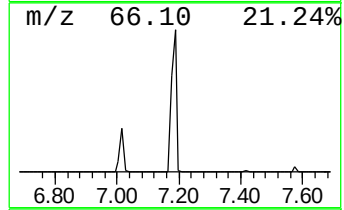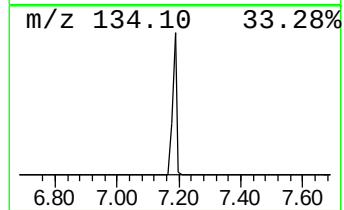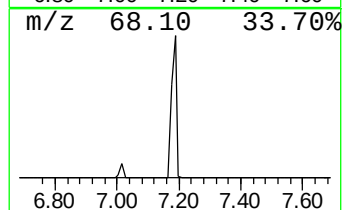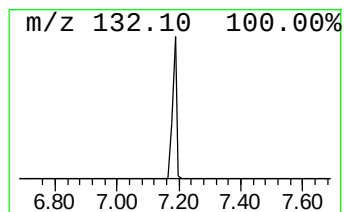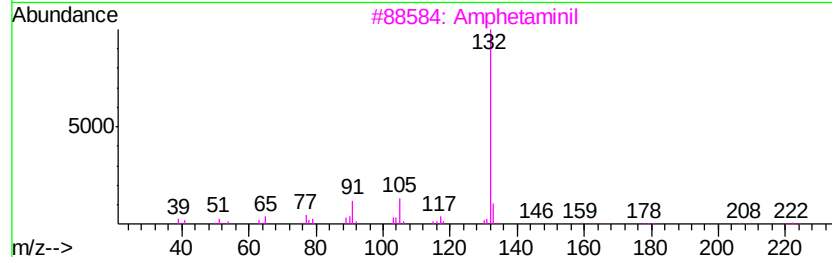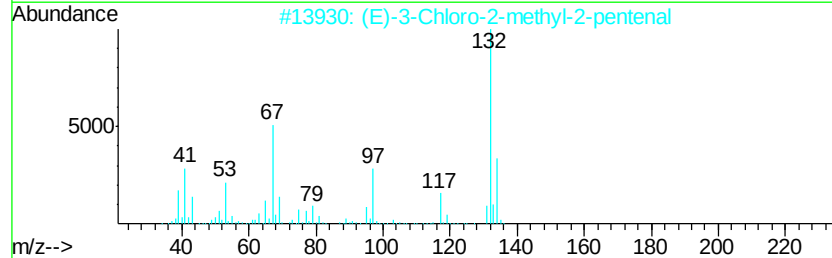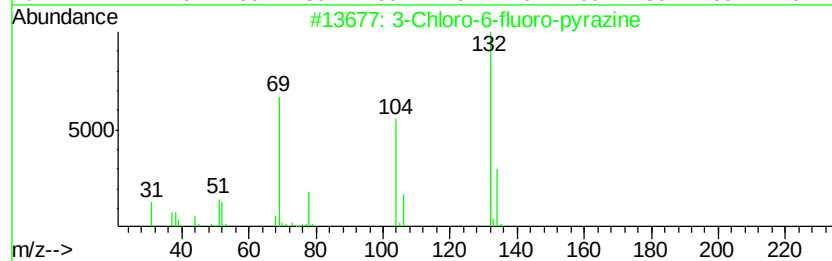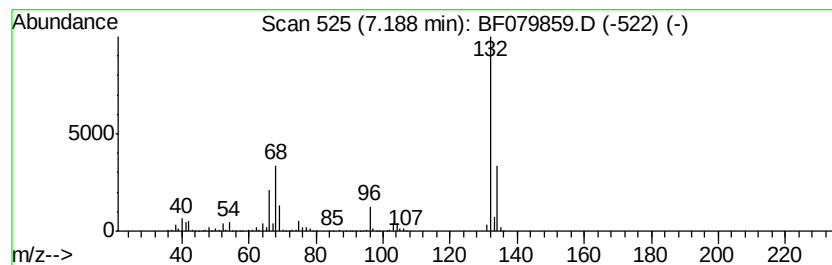

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079859.D
Acq On : 10 Jun 2015 12:25
Operator : TP/IZ
Sample : PB83898BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83898BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-dime...	2.34	142.4	ng	2000680	1	7.42	280925	20.0
unknown7.19	7.19	95.1	ng	1335250	1	7.42	280925	20.0