


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079854.D
 Acq On : 10 Jun 2015 8:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 15:11:40 2015

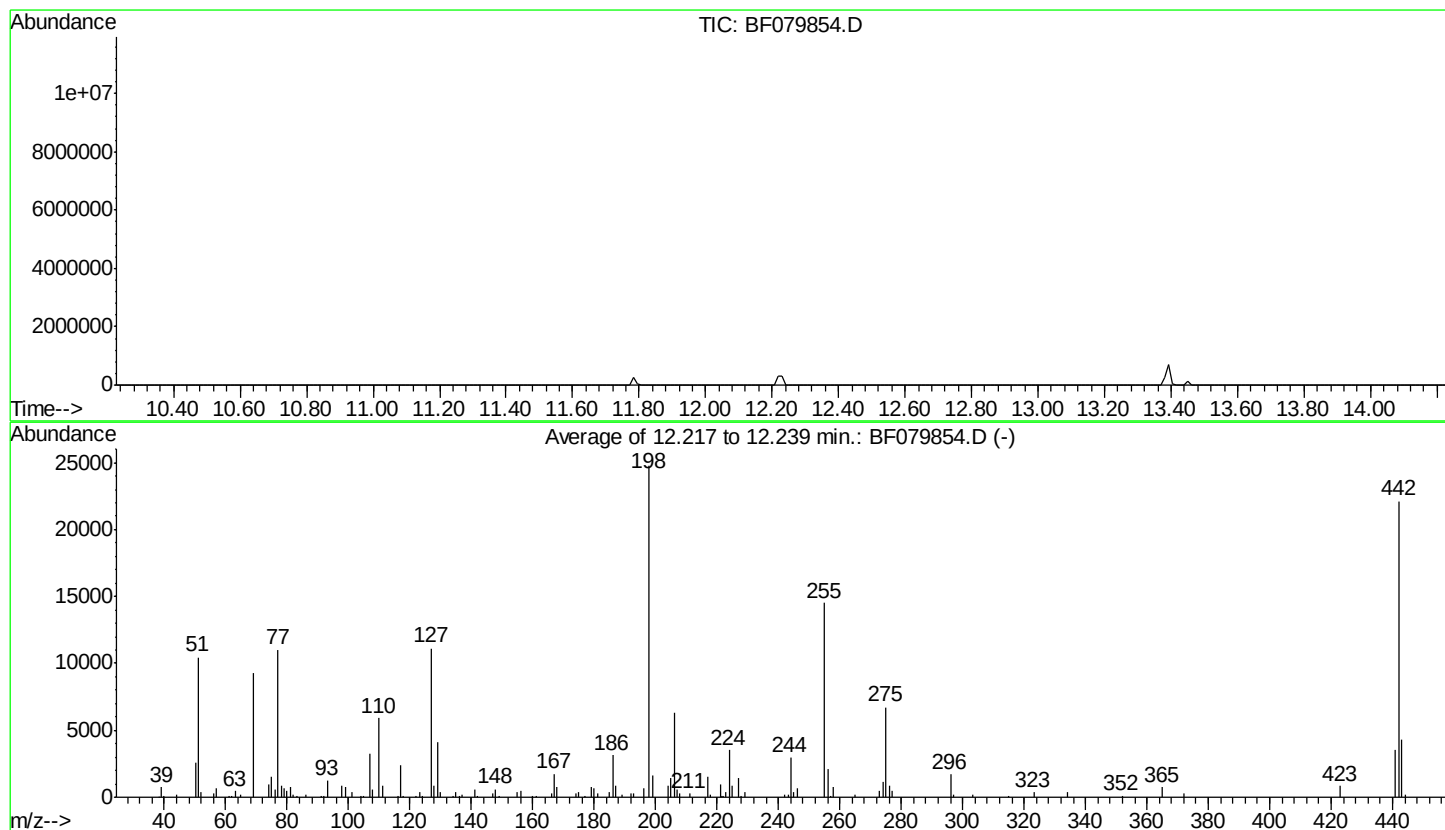

AutoFind: Scans 965, 966, 967; Background Corrected with Scan 962

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	10434	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	9320	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	11125	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24774	PASS
199	198	5	9	6.4	1582	PASS
275	198	10	60	27.1	6711	PASS
365	198	1	100	3.0	746	PASS
441	442	0.01	24	16.0	3528	PASS
442	198	50	100	89.2	22105	PASS
443	442	15	24	19.4	4281	PASS