


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079878.D
 Acq On : 10 Jun 2015 23:08
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 15:11:40 2015

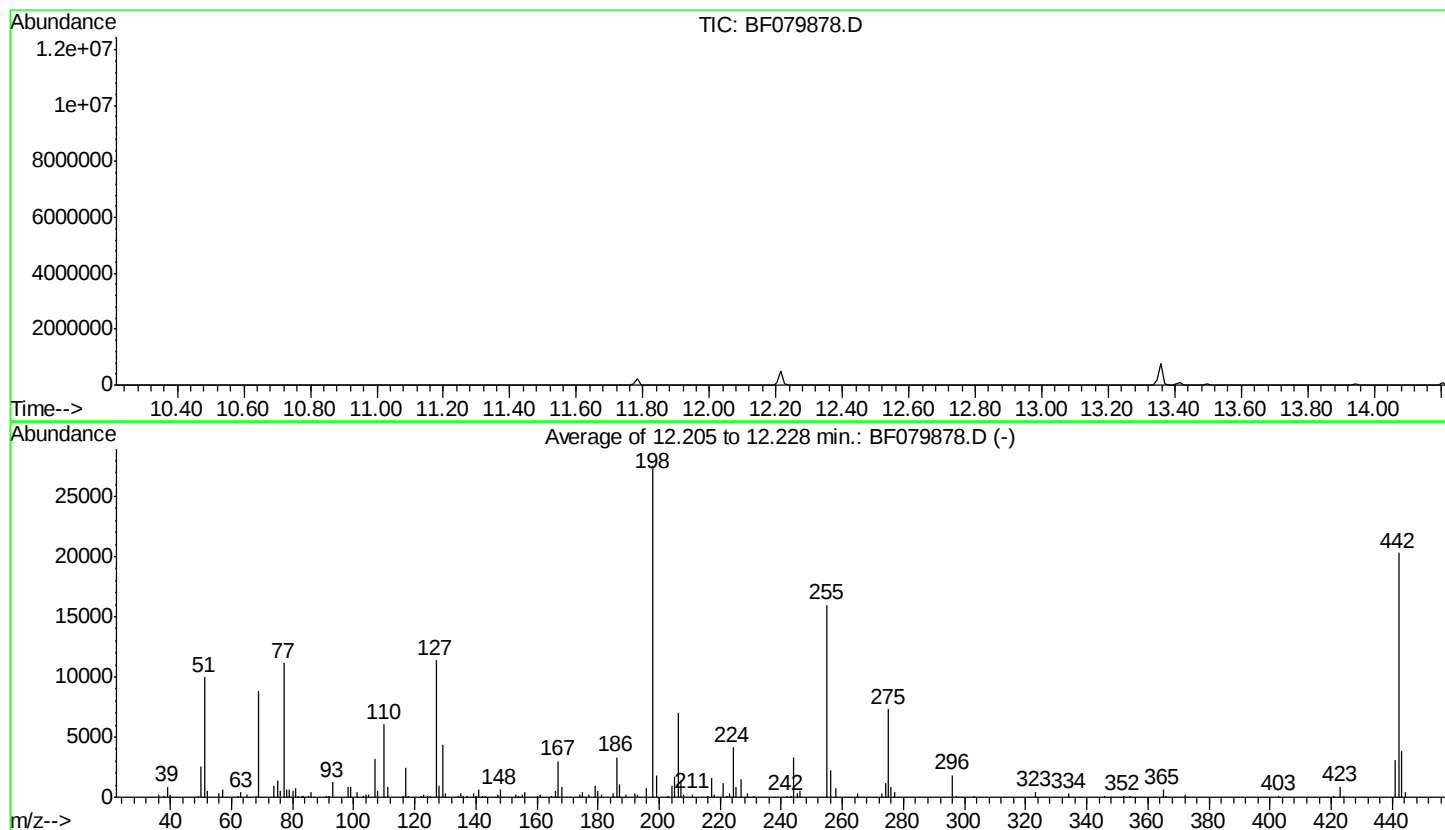

AutoFind: Scans 964, 965, 966; Background Corrected with Scan 961

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	9994	PASS
68	69	0.00	2	1.4	120	PASS
69	198	0.00	100	32.0	8818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	11363	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27553	PASS
199	198	5	9	6.4	1777	PASS
275	198	10	60	26.5	7293	PASS
365	198	1	100	2.2	608	PASS
441	442	0.01	24	15.2	3088	PASS
442	198	50	100	73.7	20312	PASS
443	442	15	24	19.1	3882	PASS