
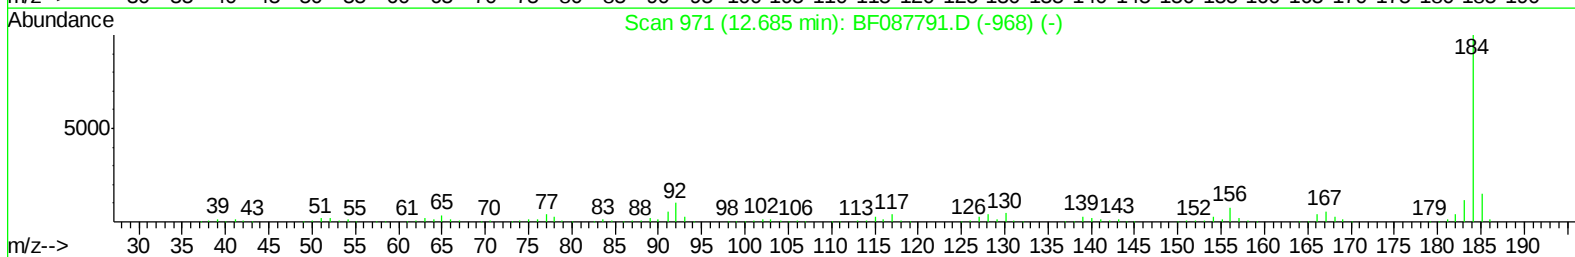
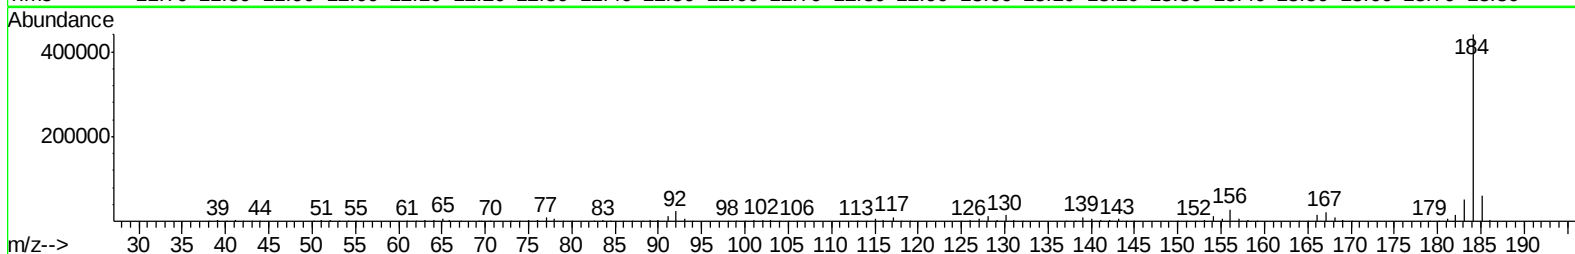


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF061016\  
Data File : BF087868.D  
Acq On : 10 Jun 2016 12:09  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 06:43:15 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 07 18:51:55 2016  
Response via : Initial Calibration

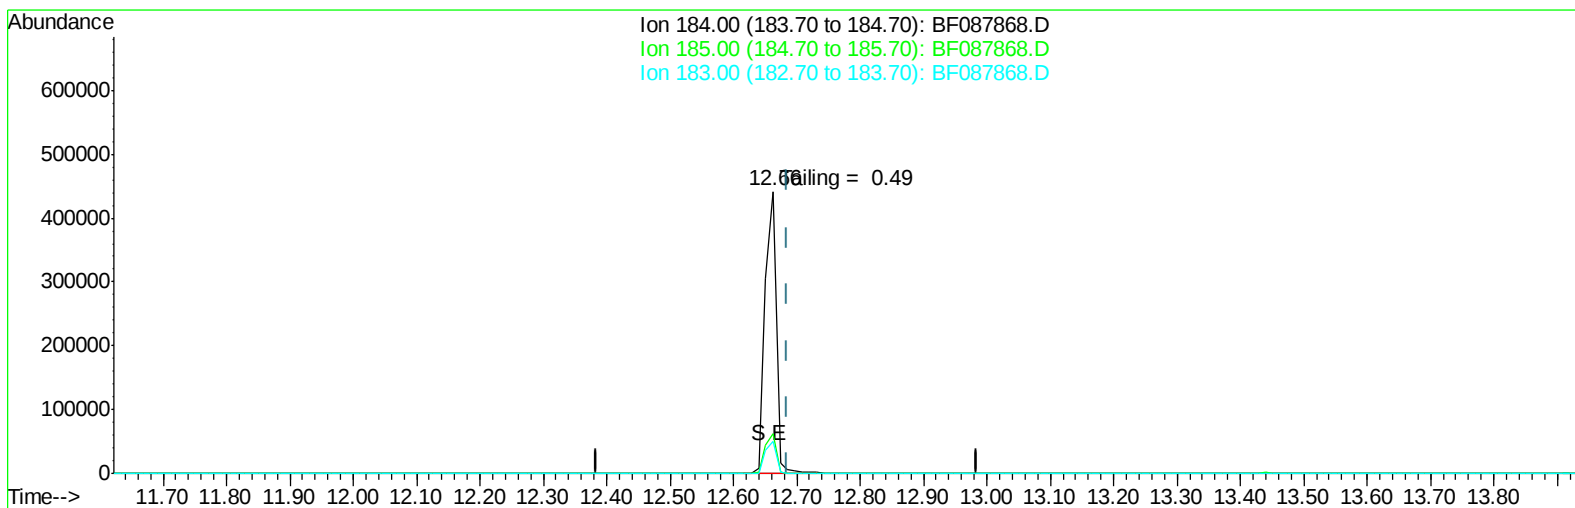

TIC: BF087868.D

(76) Benzidine




12.662min (-0.023) 0.00ng

response 542807

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 13.94 |
| 183.00 | 11.60 | 11.39 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF061016\  
Data File : BF087868.D  
Acq On : 10 Jun 2016 12:09  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 06:43:15 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 07 18:51:55 2016  
Response via : Initial Calibration

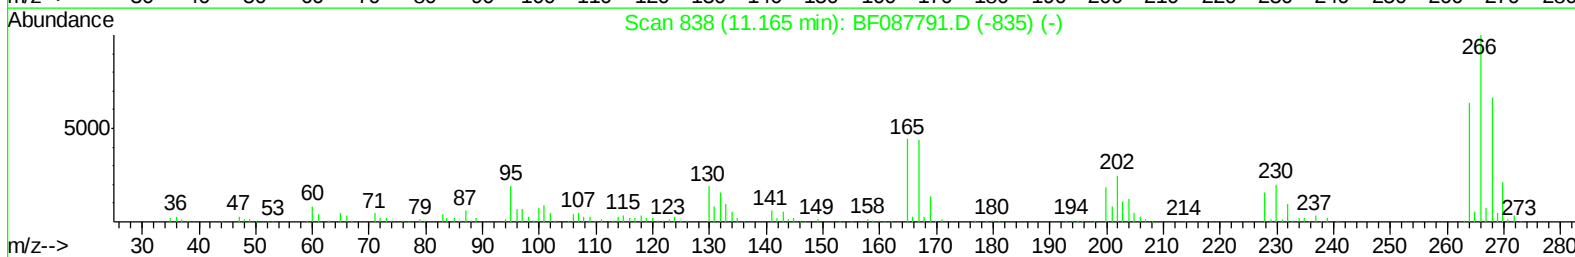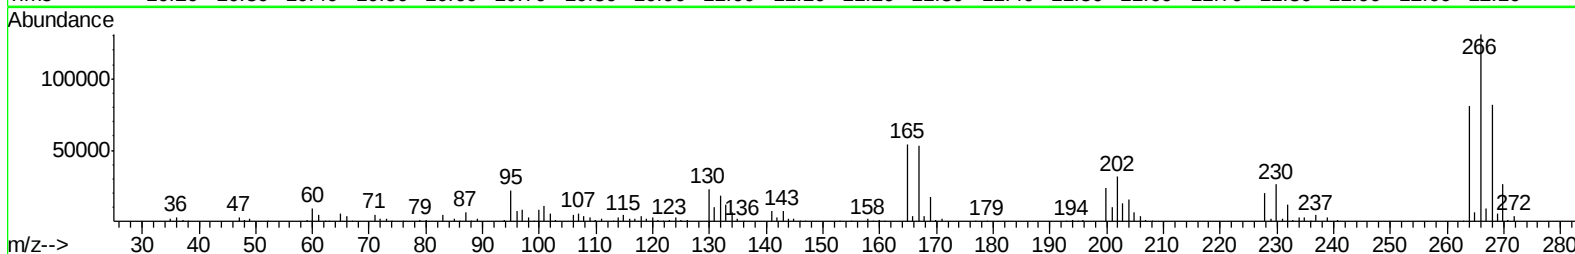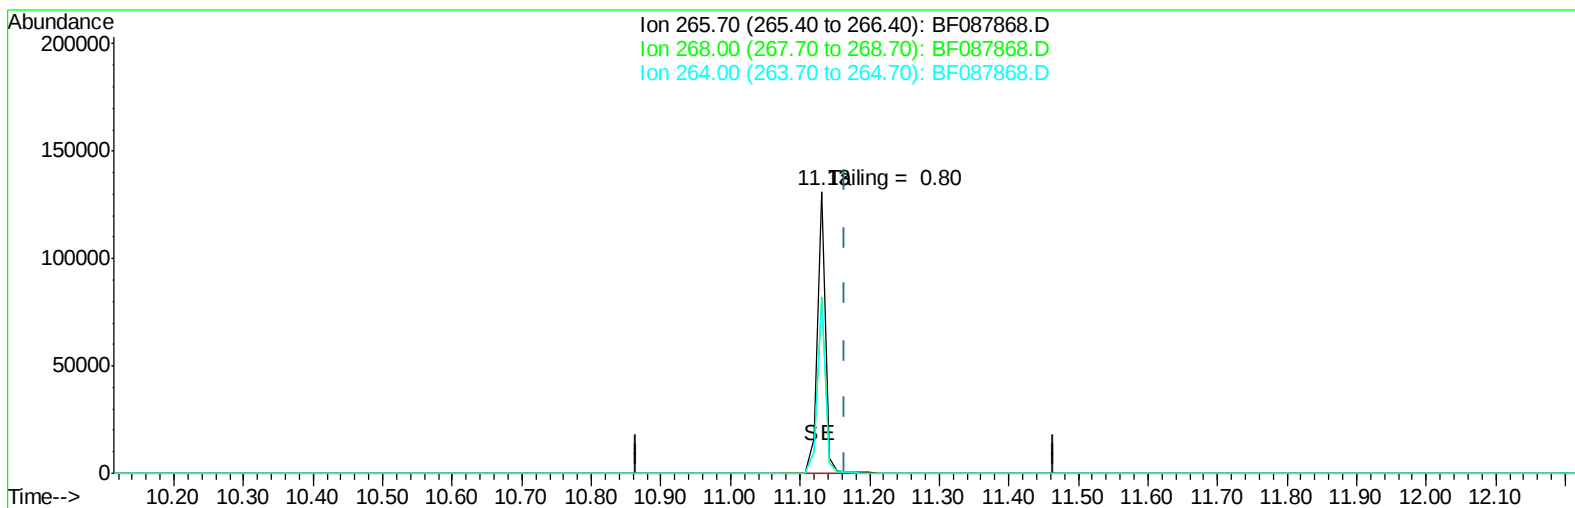

TIC: BF087868.D

(69) Pentachlorophenol (C)

11.131min (-0.034) 66248.22ng

response 108604

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.00 | 62.65 |
| 264.00 | 62.00 | 61.93 |
| 0.00   | 0.00  | 0.00  |