
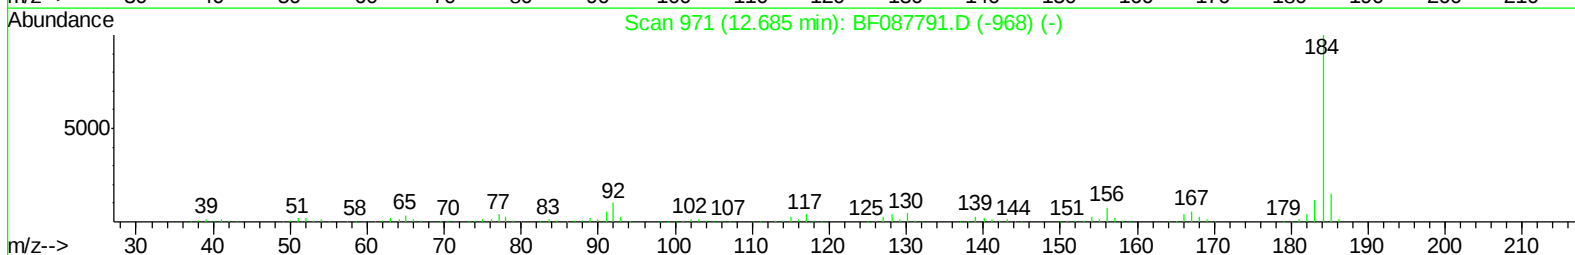
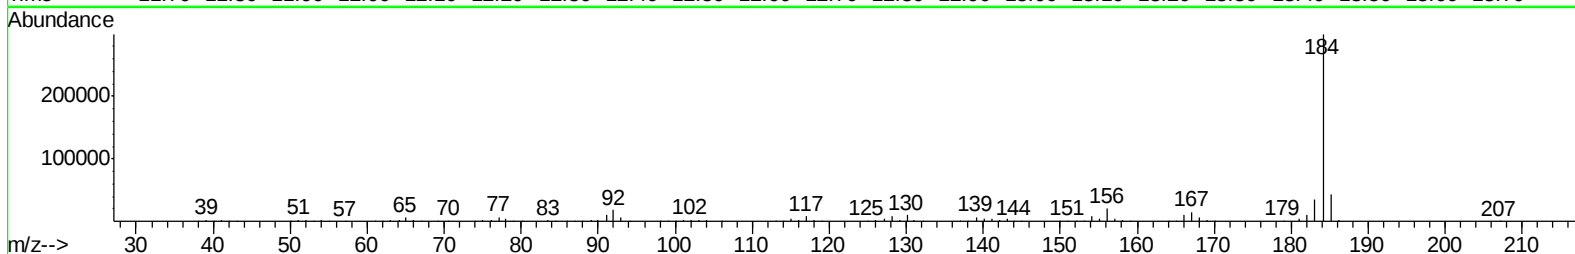


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061016\
Data File : BF087892.D
Acq On : 11 Jun 2016 00:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 06:44:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

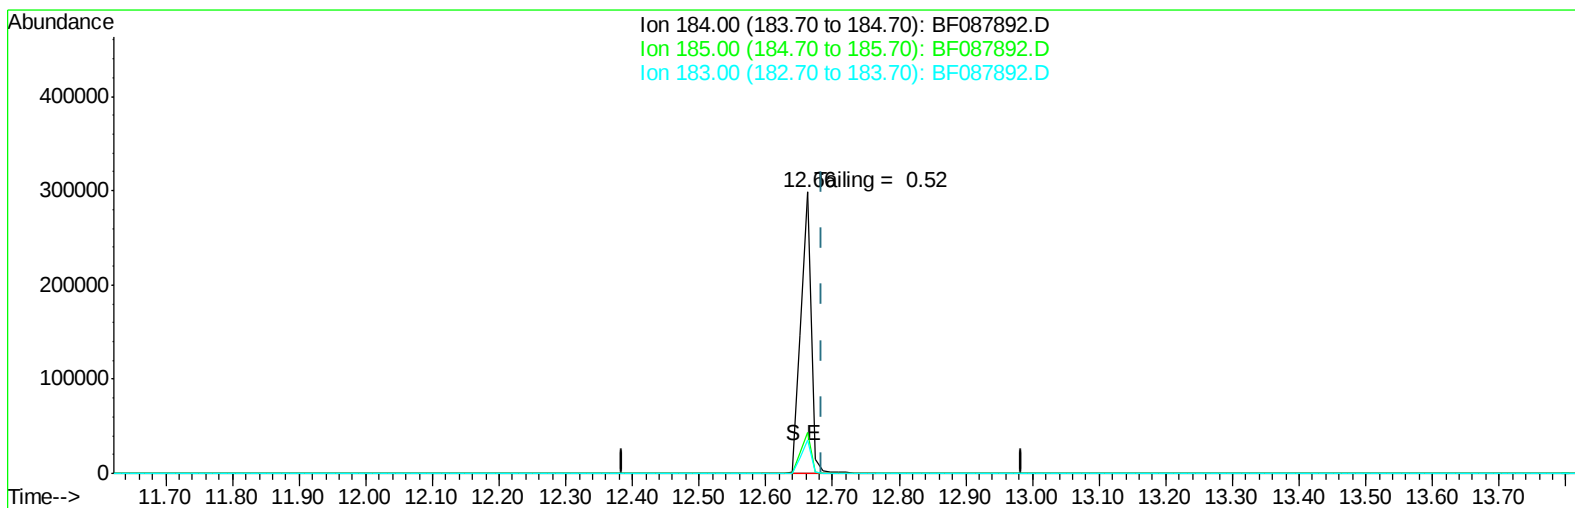

TIC: BF087892.D

(76) Benzidine




12.662min (-0.023) 0.00ng

response 323540

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.58
183.00	11.60	11.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF061016\
Data File : BF087892.D
Acq On : 11 Jun 2016 00:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 06:44:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

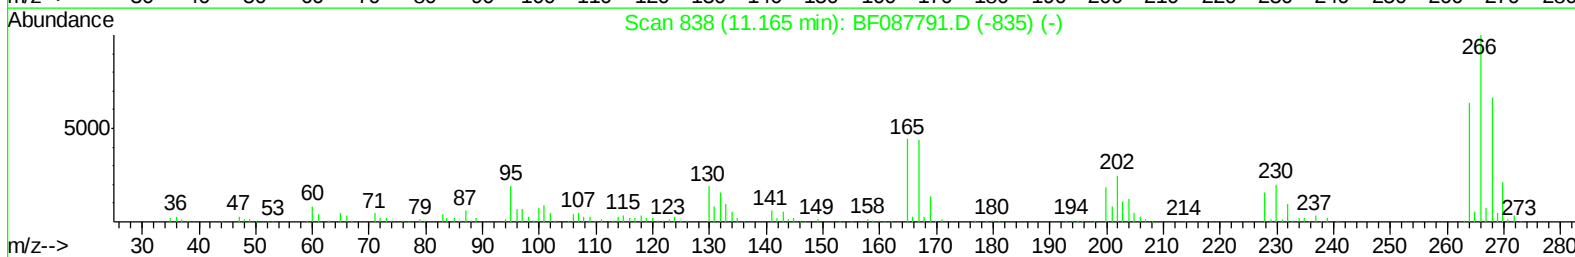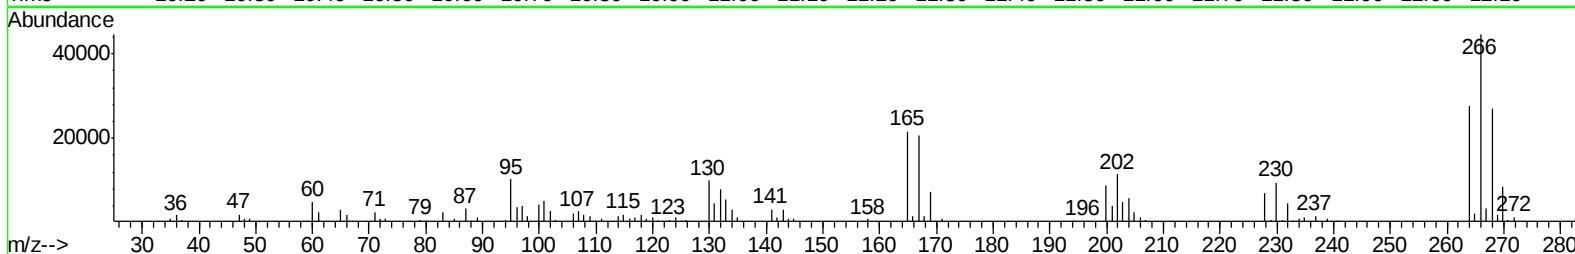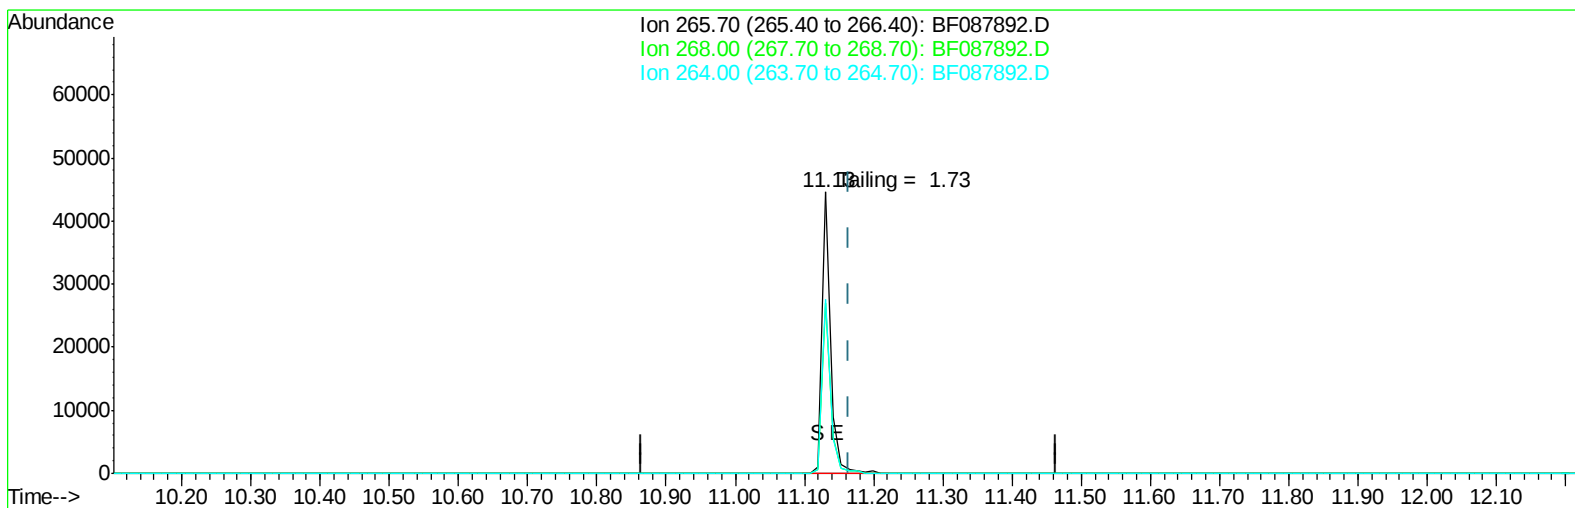

TIC: BF087892.D

(69) Pentachlorophenol (C)

11.131min (-0.034) 0.00ng

response 39670

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	60.66
264.00	62.00	61.70
0.00	0.00	0.00