


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061016\
 Data File : BF087868.D
 Acq On : 10 Jun 2016 12:09
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 14:10:49 2016

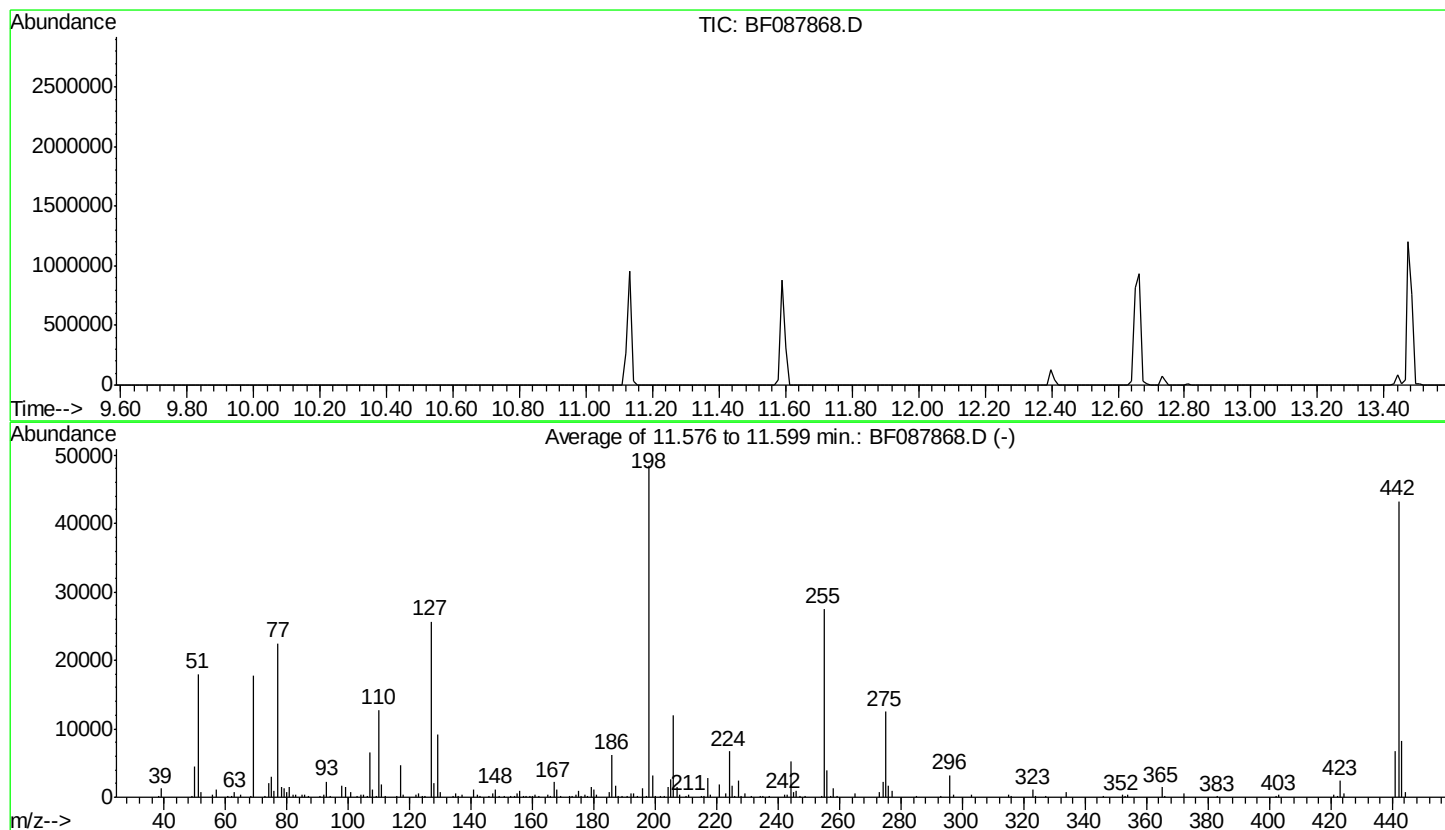

AutoFind: Scans 874, 875, 876; Background Corrected with Scan 871

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	18026	PASS
68	69	0.00	2	1.6	280	PASS
69	198	0.00	100	36.8	17836	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	25682	PASS
197	198	0.00	2	0.5	259	PASS
198	198	100	100	100.0	48456	PASS
199	198	5	9	6.7	3225	PASS
275	198	10	60	25.8	12492	PASS
365	198	1	100	3.1	1485	PASS
441	442	0.01	24	15.5	6715	PASS
442	198	50	100	89.4	43296	PASS
443	442	15	24	19.1	8253	PASS