

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061017\
 Data File : BF095851.D
 Acq On : 10 Jun 2017 16:58
 Operator : SJ/MA
 Sample : I3591-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-R10-BASE

Quant Time: Jun 12 04:30:15 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	55453	20.00	ng	-0.03
21) Naphthalene-d8	9.40	136	231683	20.00	ng	-0.04
38) Acenaphthene-d10	12.22	164	106019	20.00	ng	-0.04
63) Phenanthrene-d10	14.62	188	206115	20.00	ng	-0.03
75) Chrysene-d12	18.33	240	183488	20.00	ng	-0.02
86) Perylene-d12	20.00	264	122779	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	442096	127.04	ng	-0.03
7) Phenol-d6	6.93	99	543980	130.57	ng	-0.03
23) Nitrobenzene-d5	8.28	82	308164	82.61	ng	-0.04
41) 2,4,6-Tribromophenol	13.52	330	103550	110.39	ng	-0.04
44) 2-Fluorobiphenyl	11.18	172	521628	68.47	ng	-0.04
78) Terphenyl-d14	16.99	244	455609	61.62	ng	-0.02
Target Compounds						
49) Dimethylphthalate	11.87	163	79730	9.90	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061017\
Data File : BF095851.D
Acq On : 10 Jun 2017 16:58
Operator : SJ/MA
Sample : I3591-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-R10-BASE

Quant Time: Jun 12 04:30:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

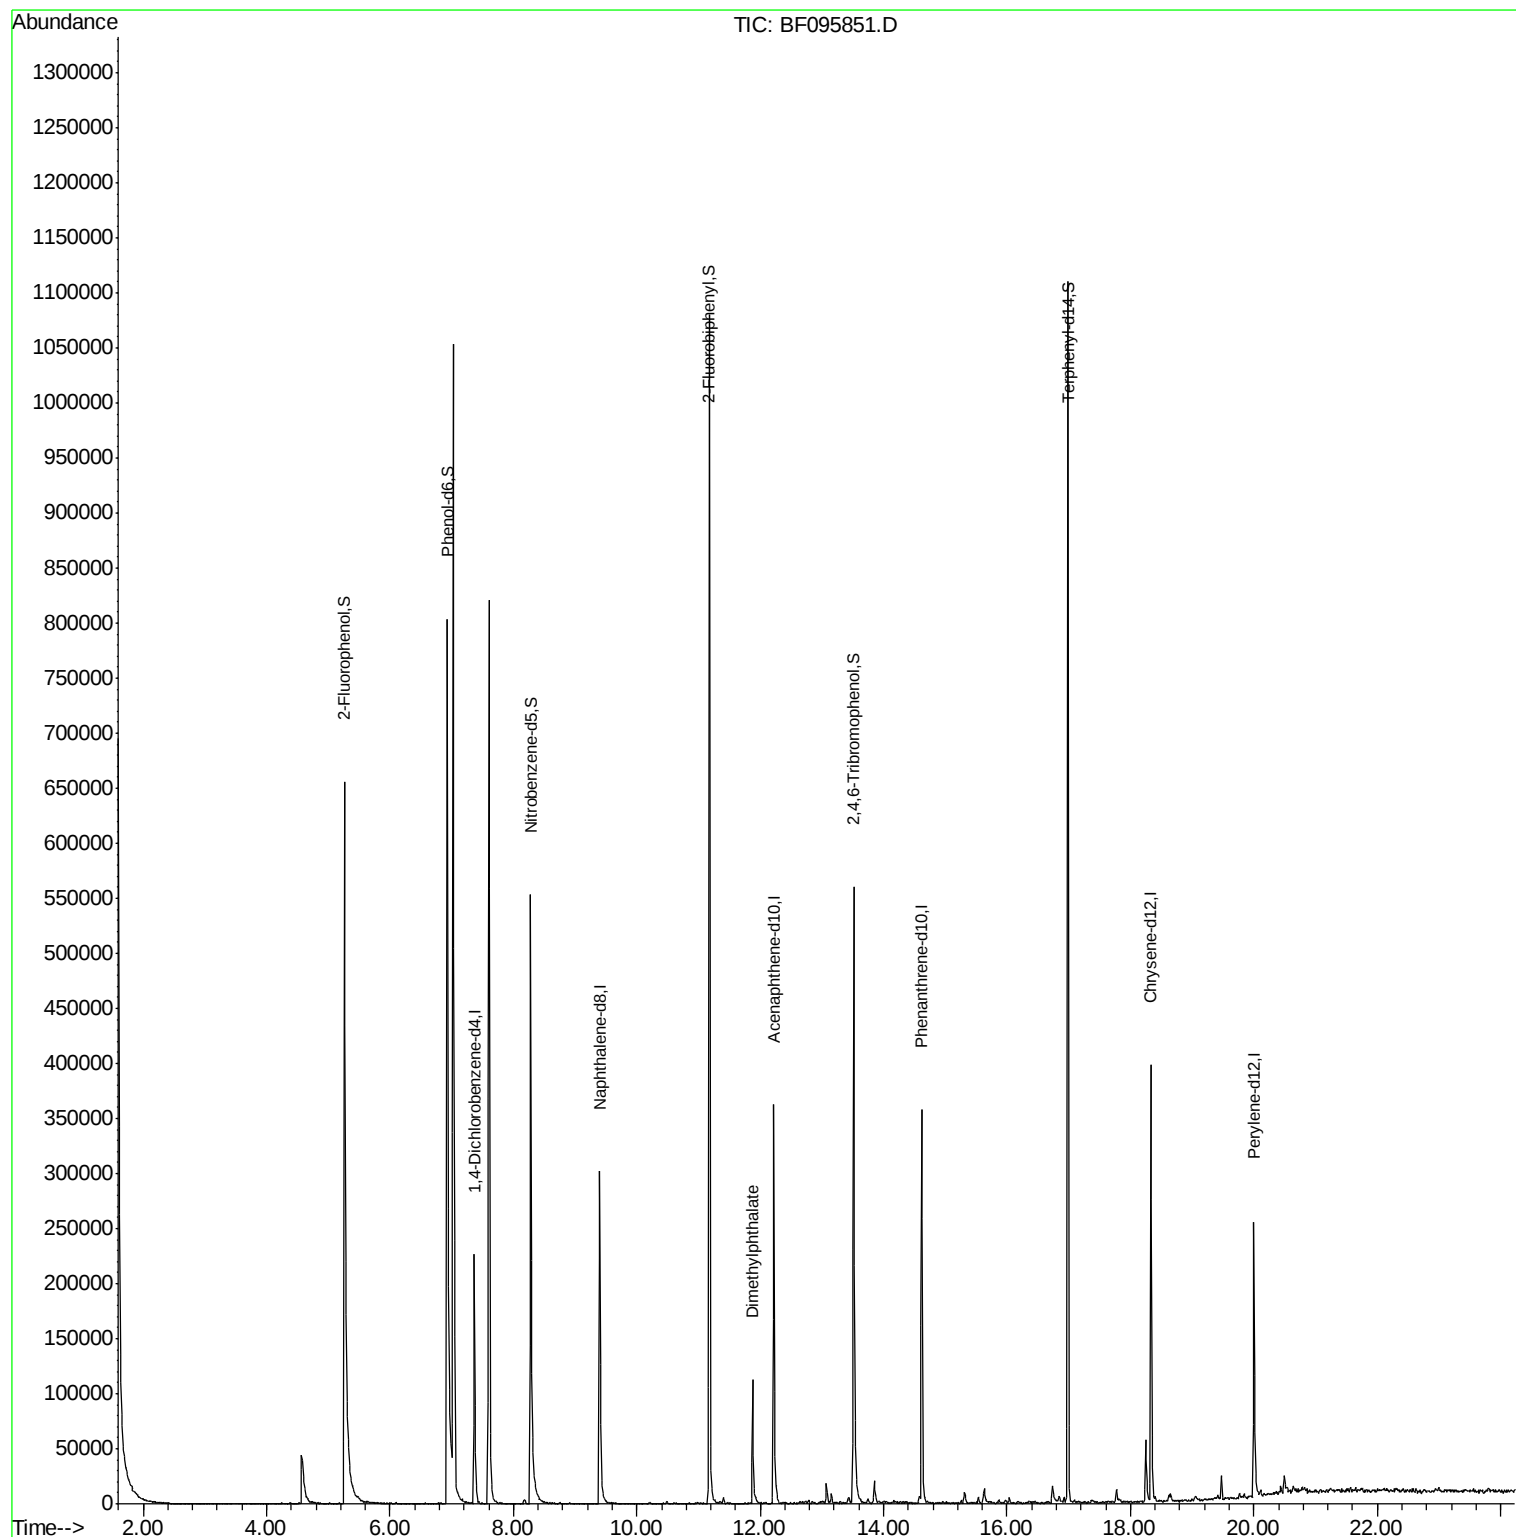




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.37 min Scan# 983
Delta R.T. -0.03 min
Lab File: BF095851.D
Acq: 10 Jun 2017 16:58

Instrument :
BNA_F
ClientSampleId :
E2-R10-BASE

Tot Ion:152 Resp: 55453
Ion Ratio Lower Upper
152 100
150 158.9 126.2 189.2
115 57.9 52.2 78.2

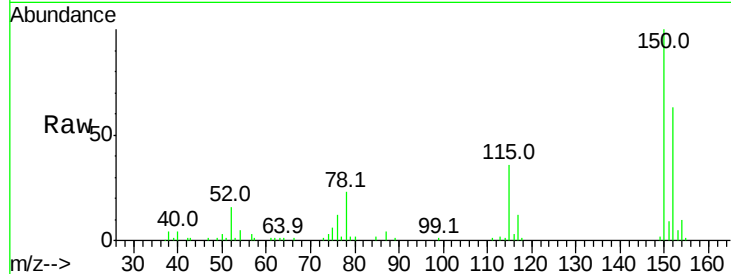


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

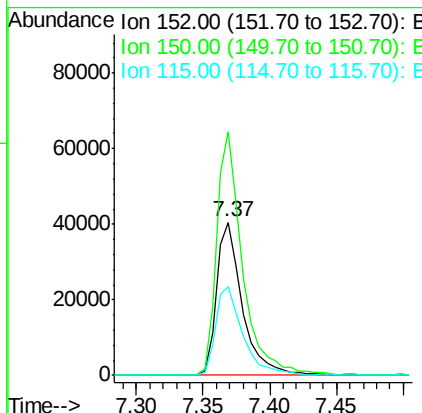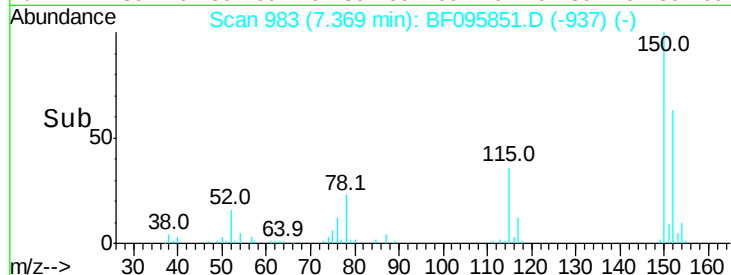



#5

2-Fluorophenol
Concen: 127.04 ng
RT: 5.26 min Scan# 624
Delta R.T. -0.03 min
Lab File: BF095851.D
Acq: 10 Jun 2017 16:58

Tgt Ion:112 Resp: 442096
Ion Ratio Lower Upper
112 100
64 56.3 46.0 69.0
63 28.5 23.4 35.0

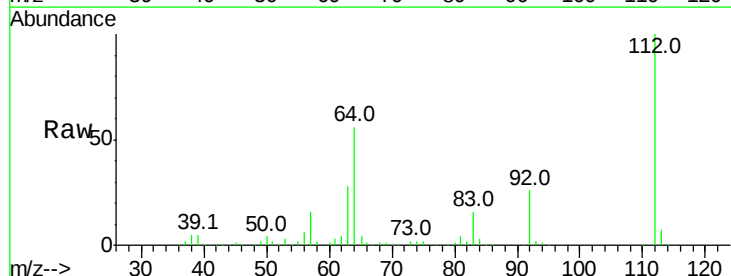

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

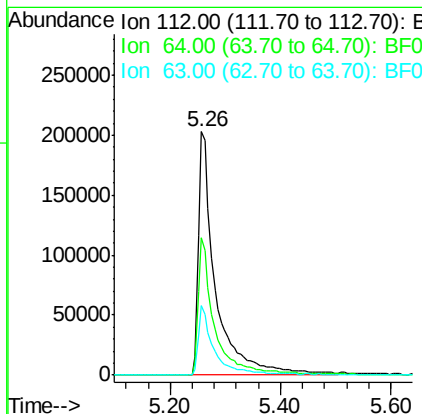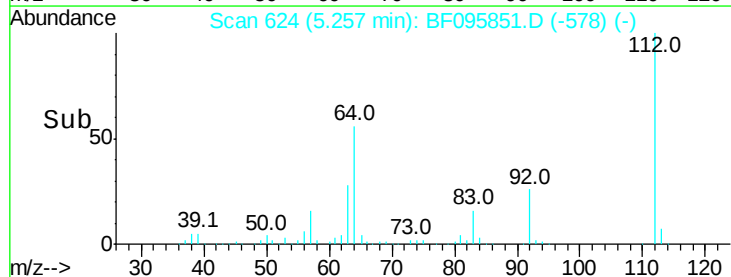



#7

Phenol-d6

Concen: 130.57 ng

RT: 6.93 min Scan# 908

Delta R.T. -0.03 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58

Instrument :

BNA_F

ClientSampleId :

E2-R10-BASE


Tot Ion: 99 Resp: 543980

Ion Ratio Lower Upper

99 100

42 16.0 13.5 20.3




71 31.3 24.5 36.7

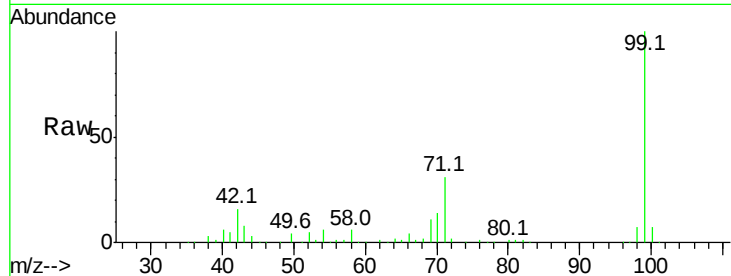

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

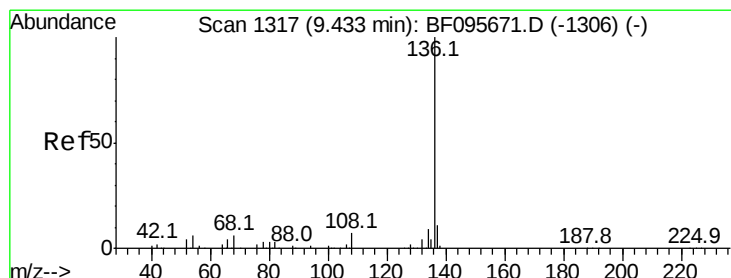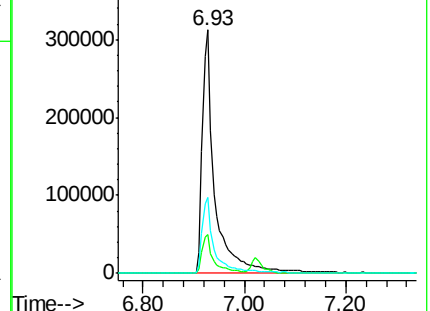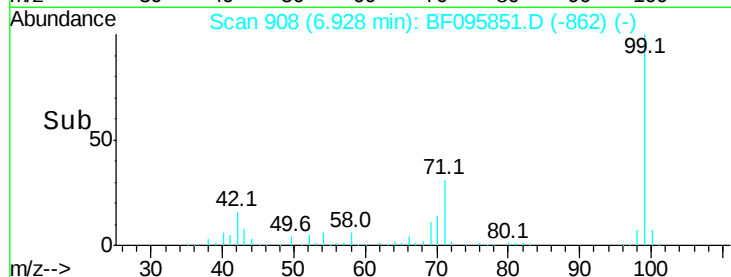

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.40 min Scan# 1328

Delta R.T. -0.04 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58

Tgt Ion: 136 Resp: 231683


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 6.4 4.9 7.3

68 5.4 4.1 6.1


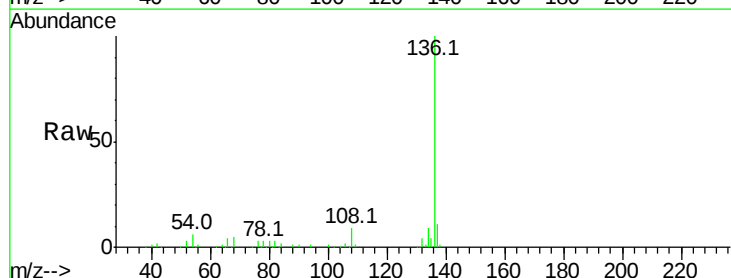


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

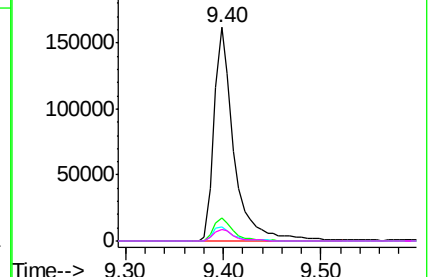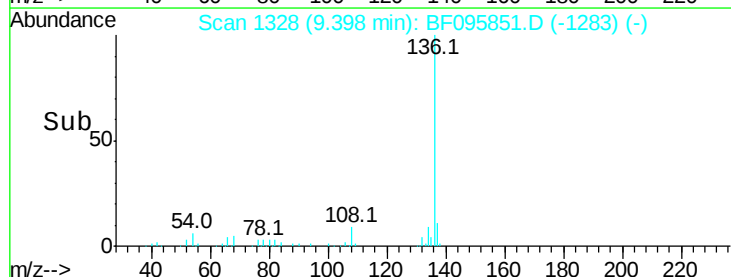







#23
Nitrobenzene-d5
Concen: 82.61 ng
RT: 8.28 min Scan# 1138
Delta R.T. -0.04 min
Lab File: BF095851.D
Acq: 10 Jun 2017 16:58

Instrument :
BNA_F
ClientSampleId :
E2-R10-BASE

Tot Ion: 82 Resp: 308164
Ion Ratio Lower Upper
82 100
128 45.9 34.0 51.0
54 46.6 42.2 63.2

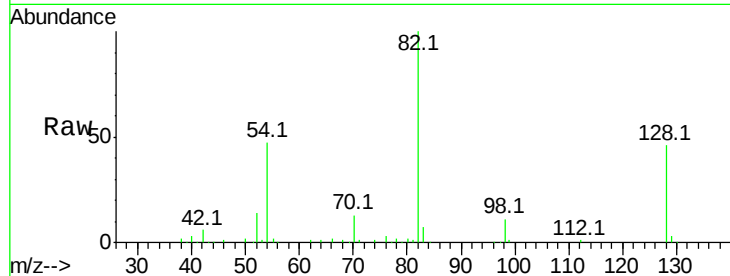


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

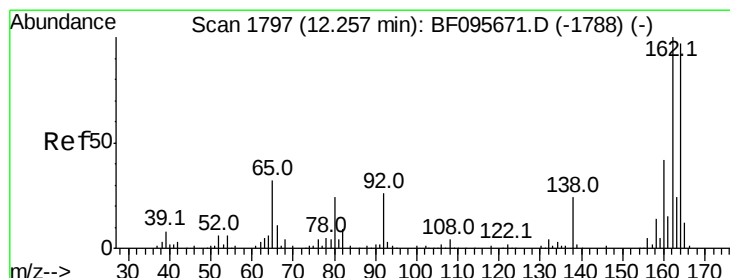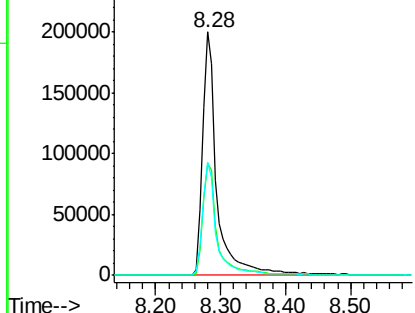
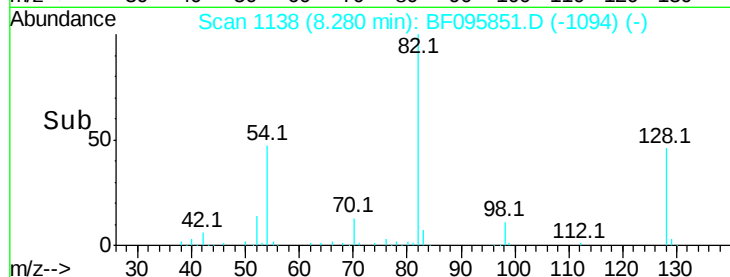



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.22 min Scan# 1808
Delta R.T. -0.04 min
Lab File: BF095851.D
Acq: 10 Jun 2017 16:58

Tgt Ion:164 Resp: 106019
Ion Ratio Lower Upper
164 100
162 104.2 82.6 123.8
160 47.4 36.2 54.2

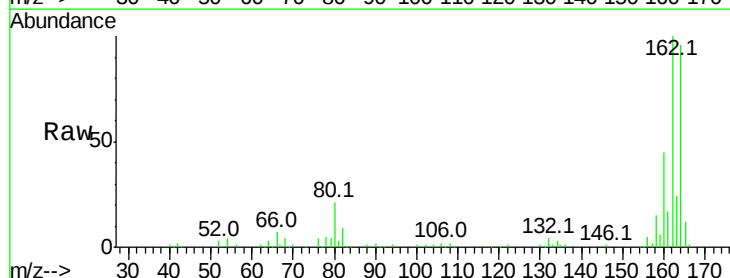

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



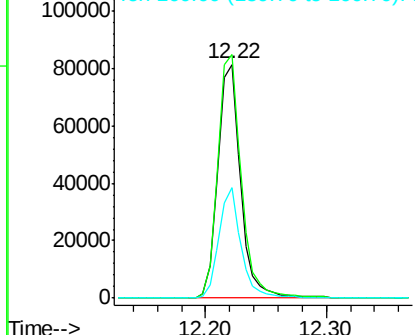
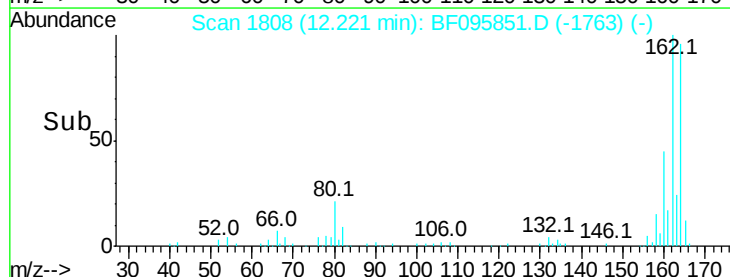


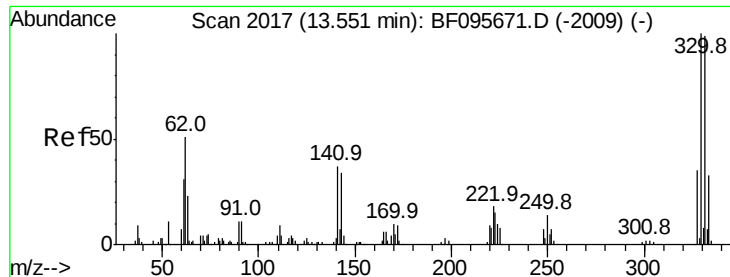

#41
 2,4,6-Tribromophenol
 Concen: 110.39 ng
 RT: 13.52 min Scan# 2028
 Delta R.T. -0.04 min
 Lab File: BF095851.D
 Acq: 10 Jun 2017 16:58




Instrument :
 BNA_F
 ClientSampleId :
 E2-R10-BASE

Tot Ion:330 Resp: 103550
 Ion Ratio Lower Upper
 330 100
 332 97.6 76.6 115.0
 141 38.0 31.4 47.2

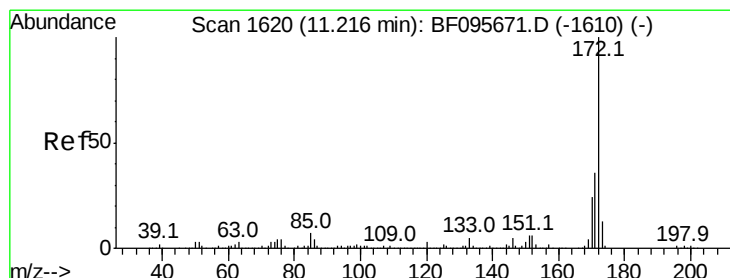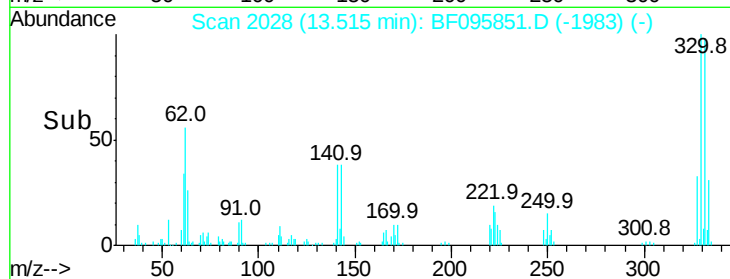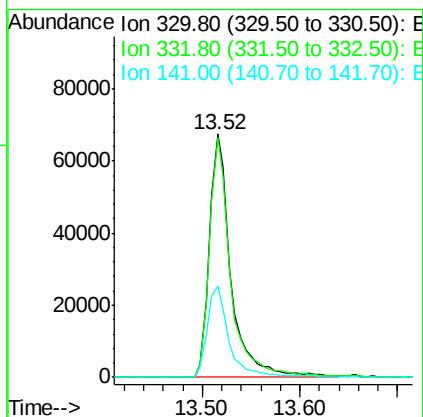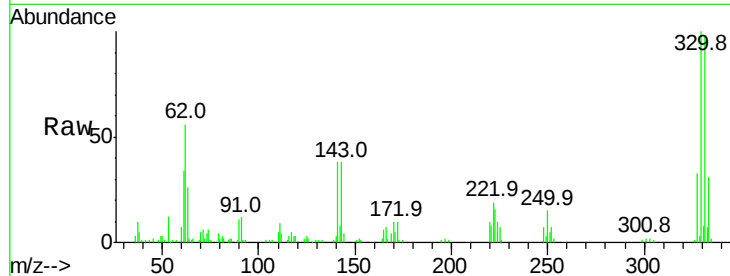

#44
 2-Fluorobiphenyl
 Concen: 68.47 ng
 RT: 11.18 min Scan# 1631
 Delta R.T. -0.04 min
 Lab File: BF095851.D
 Acq: 10 Jun 2017 16:58

Tgt Ion:172 Resp: 521628
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.6 44.4
 170 22.0 19.8 29.8

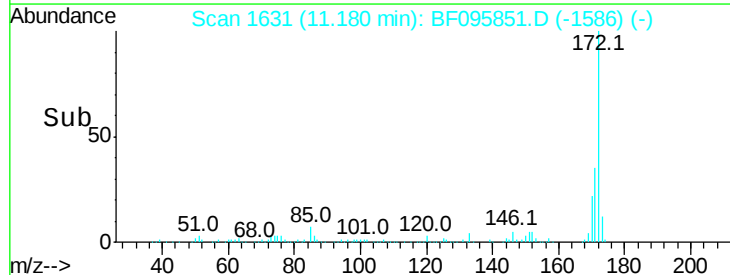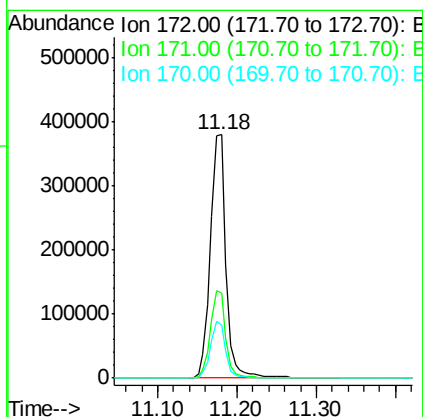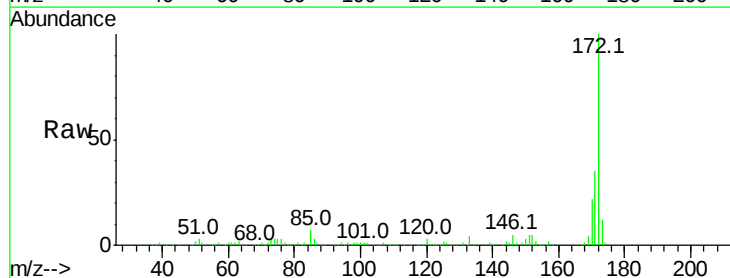



#49

Dimethylphthalate

Concen: 9.90 ng

RT: 11.87 min Scan# 1749

Delta R.T. -0.04 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58

Instrument :

BNA_F

ClientSampleId :

E2-R10-BASE


Tot Ion:163 Resp: 79730

Ion Ratio Lower Upper

163 100

194 3.7 2.6 4.0




164 10.3 8.4 12.6

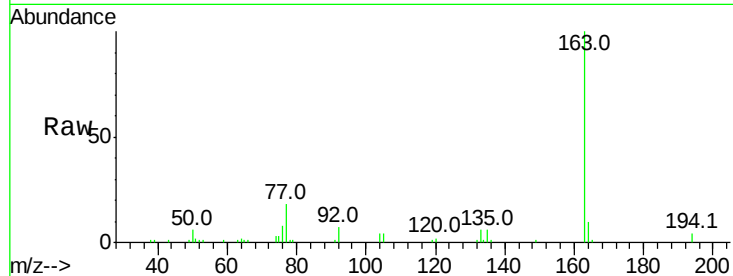

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

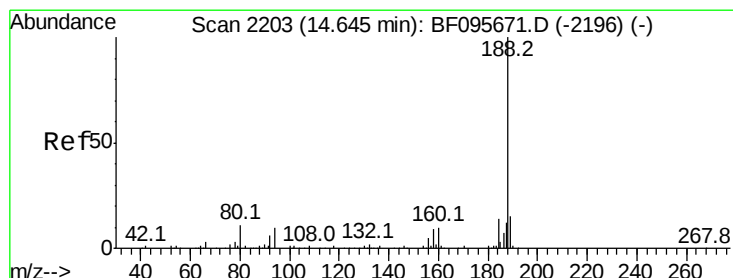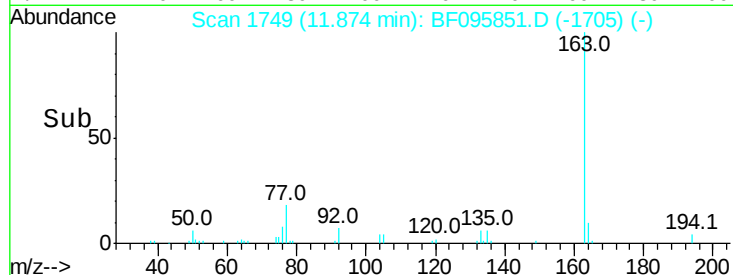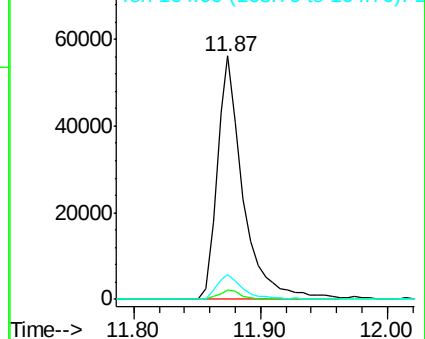

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.62 min Scan# 2215

Delta R.T. -0.03 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58


Tgt Ion:188 Resp: 206115

Ion Ratio Lower Upper

188 100

94 10.0 9.4 14.2



80 10.6 10.2 15.2

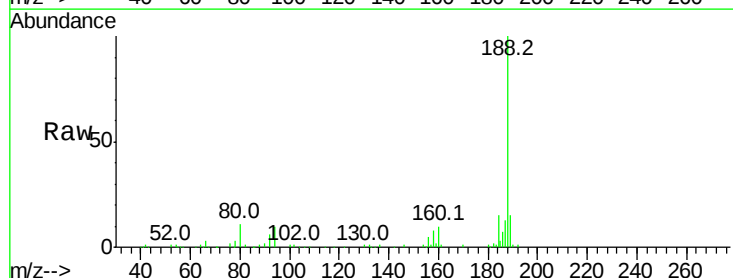

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

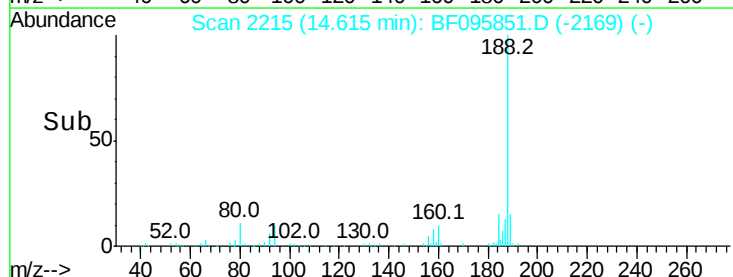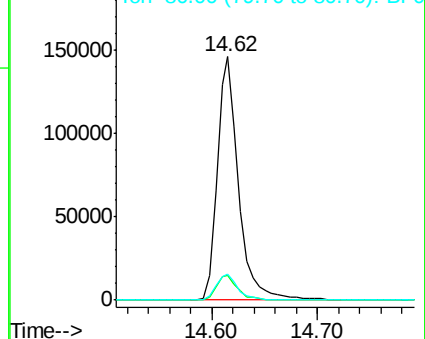



#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.33 min Scan# 2847

Delta R.T. -0.02 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58

Instrument :

BNA_F

ClientSampleId :

E2-R10-BASE


Tot Ion:240 Resp: 183488

Ion Ratio Lower Upper

240 100

120 13.3 5.8 8.8#




236 24.4 20.5 30.7

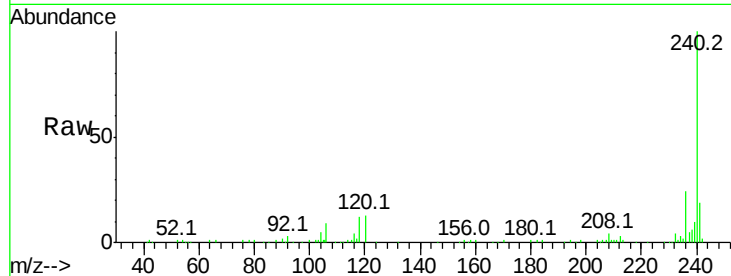

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

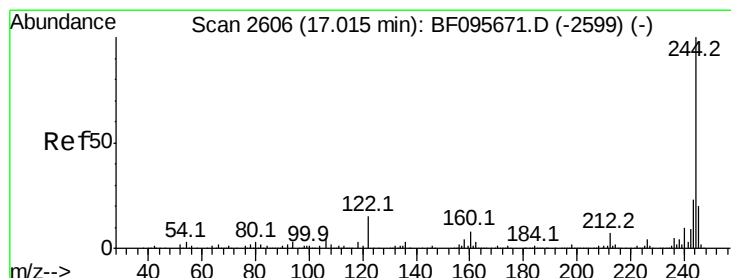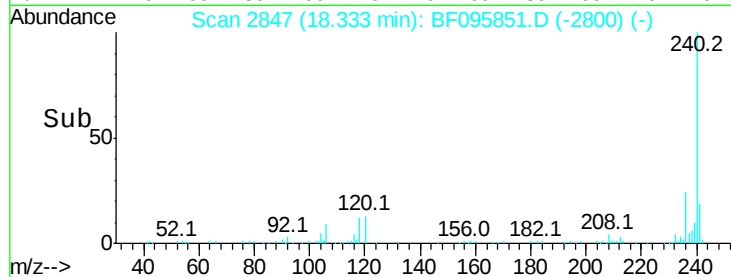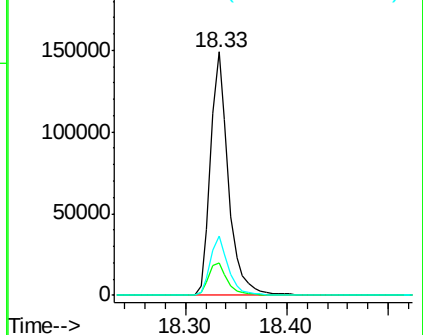

#78

Terphenyl-d14

Concen: 61.62 ng

RT: 16.99 min Scan# 2619

Delta R.T. -0.02 min

Lab File: BF095851.D

Acq: 10 Jun 2017 16:58


Tgt Ion:244 Resp: 455609

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0



122 13.2 10.3 15.5

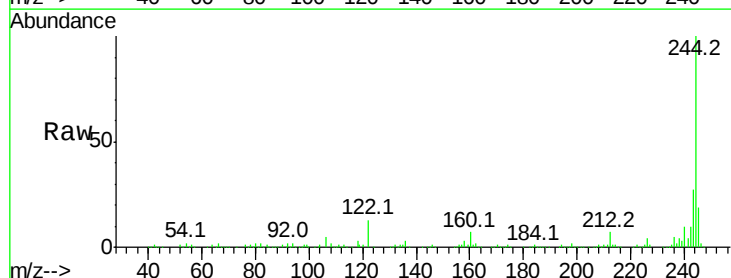


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

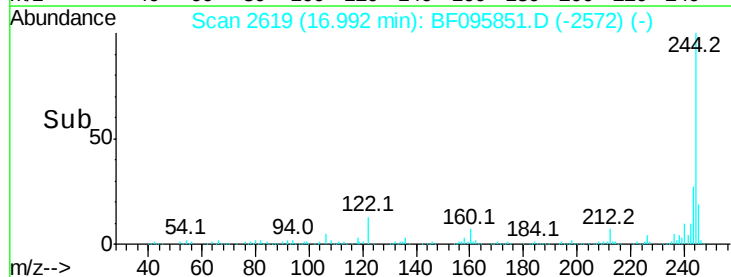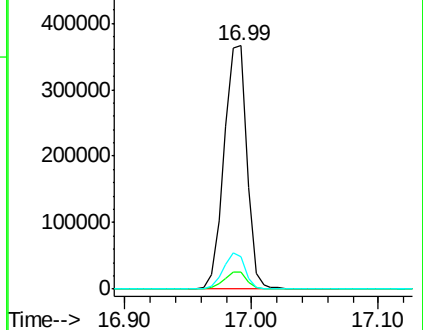


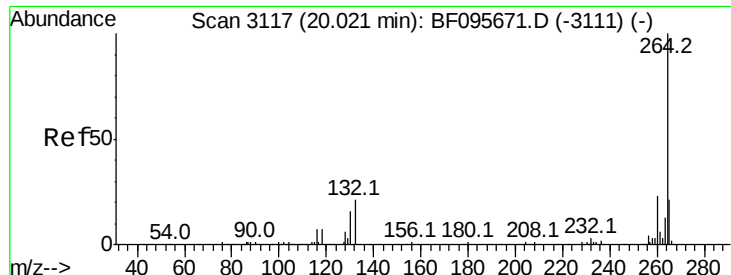

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 20.00 min Scan# 3131
 Delta R.T. -0.02 min
 Lab File: BF095851.D
 Acq: 10 Jun 2017 16:58

Instrument :
 BNA_F
 ClientSampleId :
 E2-R10-BASE

Tot Ion:264 Resp: 122779
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.5 29.3
 265 21.7 17.2 25.8

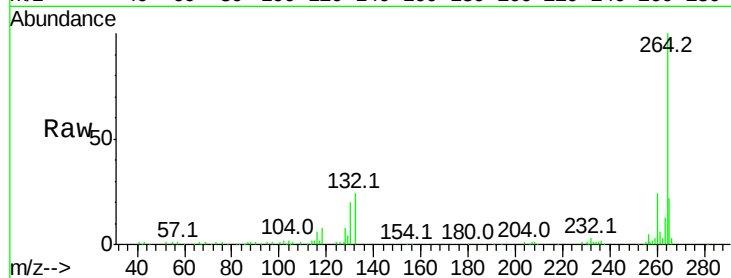

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

