


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061017\
 Data File : BF095846.D
 Acq On : 10 Jun 2017 13:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

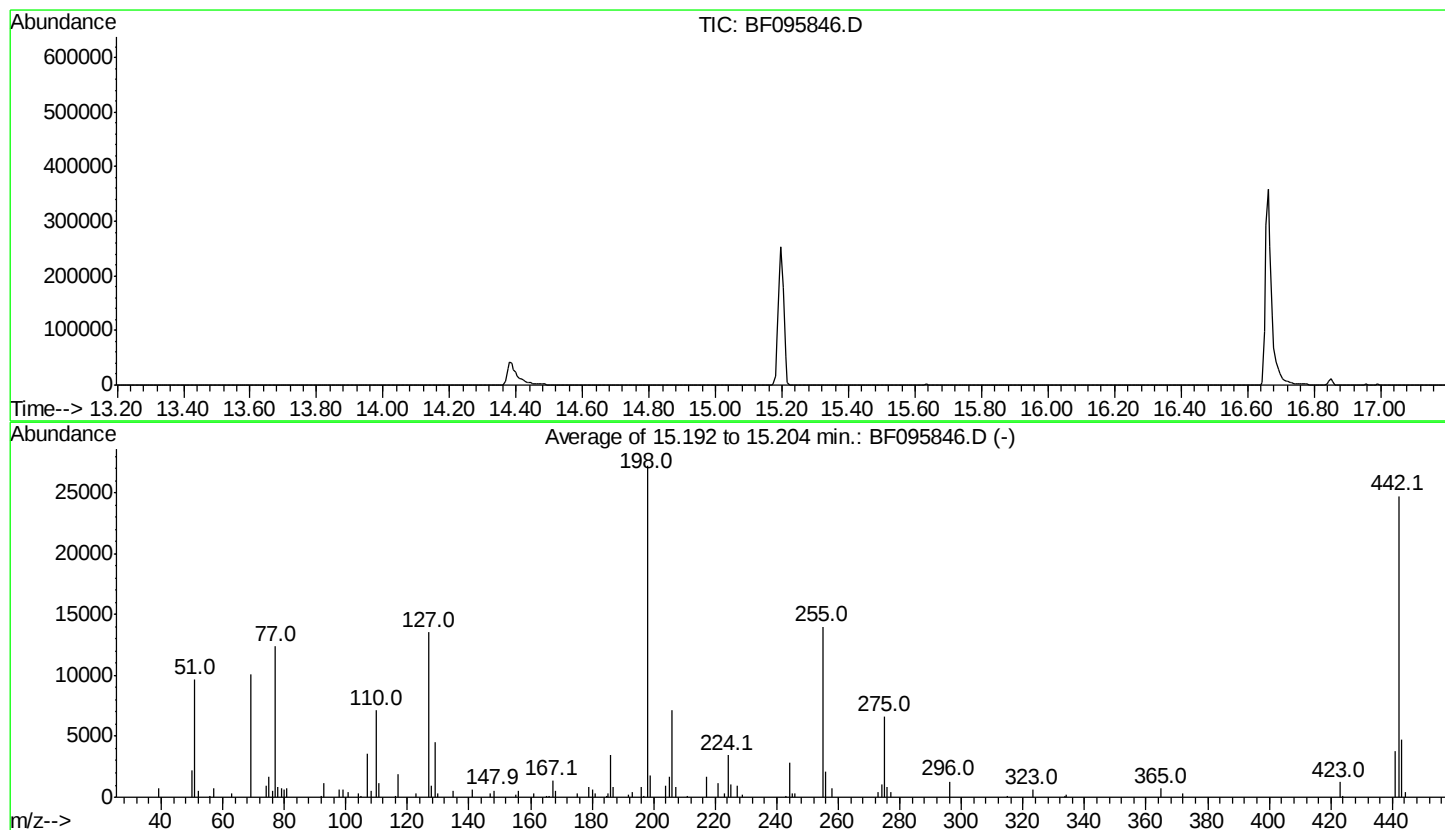

AutoFind: Scans 2313, 2314, 2315; Background Corrected with Scan 2307

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	9638	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.1	10102	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	13522	PASS
197	198	0.00	2	0.5	126	PASS
198	198	100	100	100.0	27237	PASS
199	198	5	9	6.4	1741	PASS
275	198	10	60	24.3	6622	PASS
365	198	1	100	2.6	703	PASS
441	442	0.01	24	15.4	3817	PASS
442	198	50	100	90.7	24717	PASS
443	442	15	24	19.2	4741	PASS