
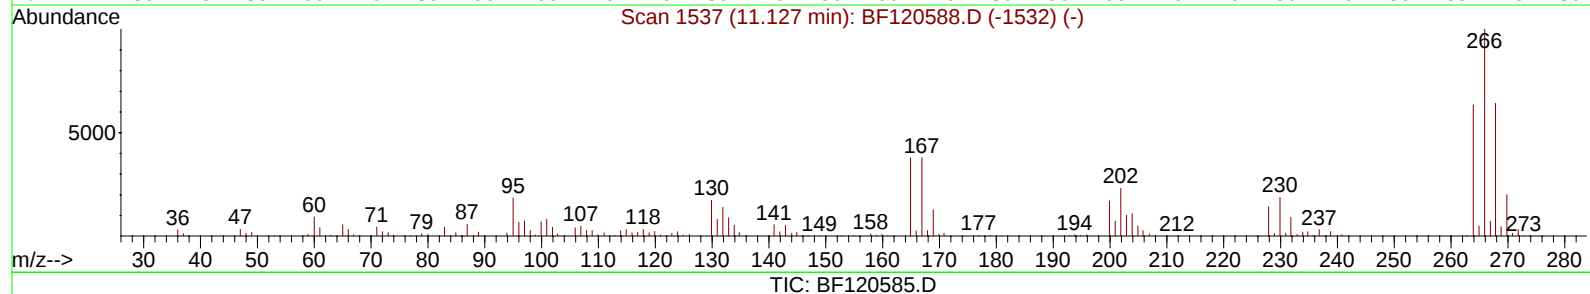
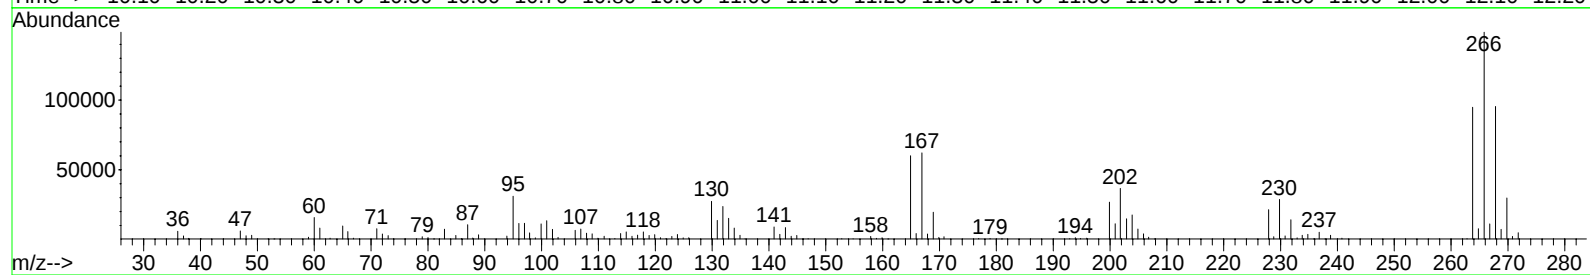


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061020\
Data File : BF120585.D
Acq On : 10 Jun 2020 10:22
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 18:58:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 10 18:10:18 2020
Response via : Initial Calibration

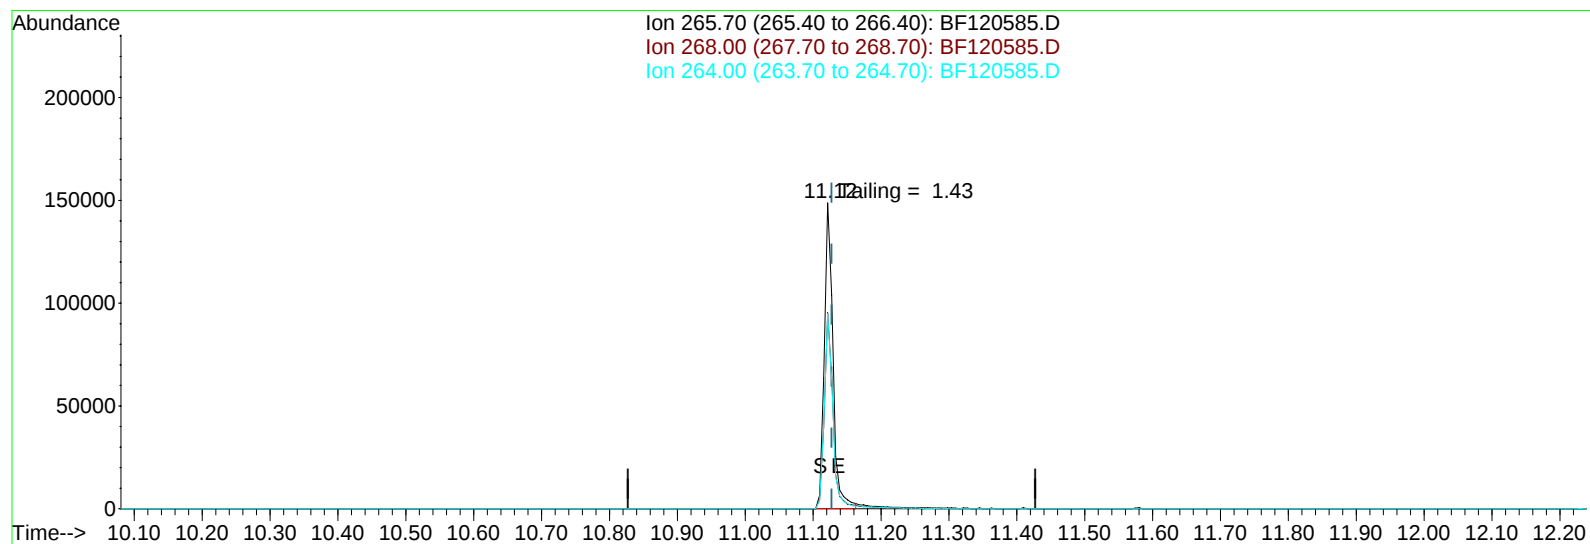

(70) Pentachlorophenol (C)




11.121min (-0.006) 32430.09ng

response 136402

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	64.13
264.00	63.50	63.76
0.00	0.00	0.00

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061020\  
Data File   : BF120585.D  
Acq On      : 10 Jun 2020   10:22  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 10 18:58:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 10 18:10:18 2020
Response via : Initial Calibration

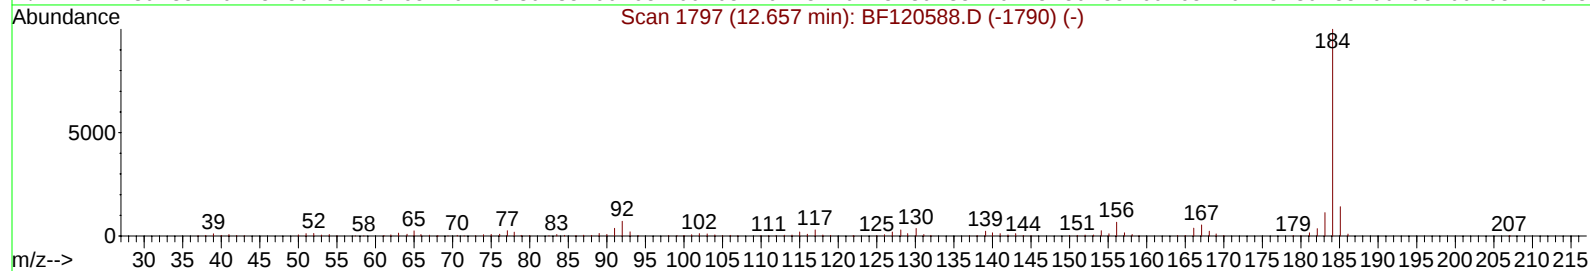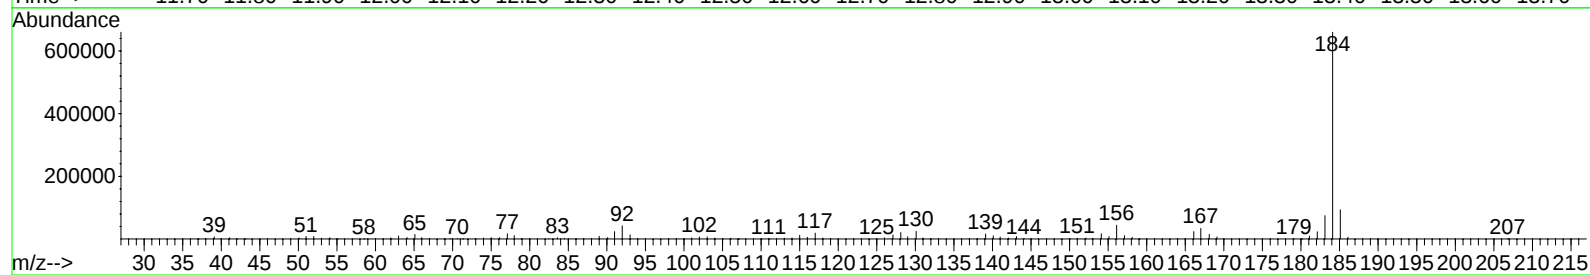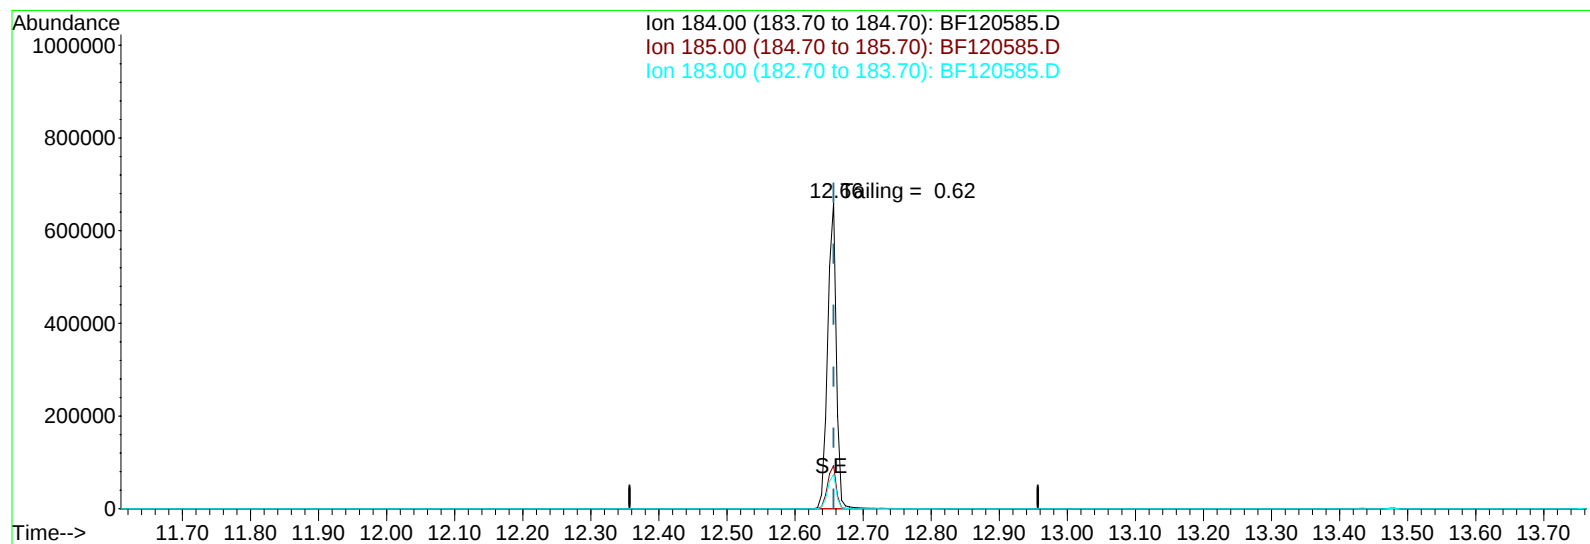

TIC: BF120585.D

(77) Benzidine

12.657min (-0.000) 0.00ng

response 584117

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.16
183.00	11.30	11.31
0.00	0.00	0.00