


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061020\
 Data File : BF120585.D
 Acq On : 10 Jun 2020 10:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 10 18:10:18 2020

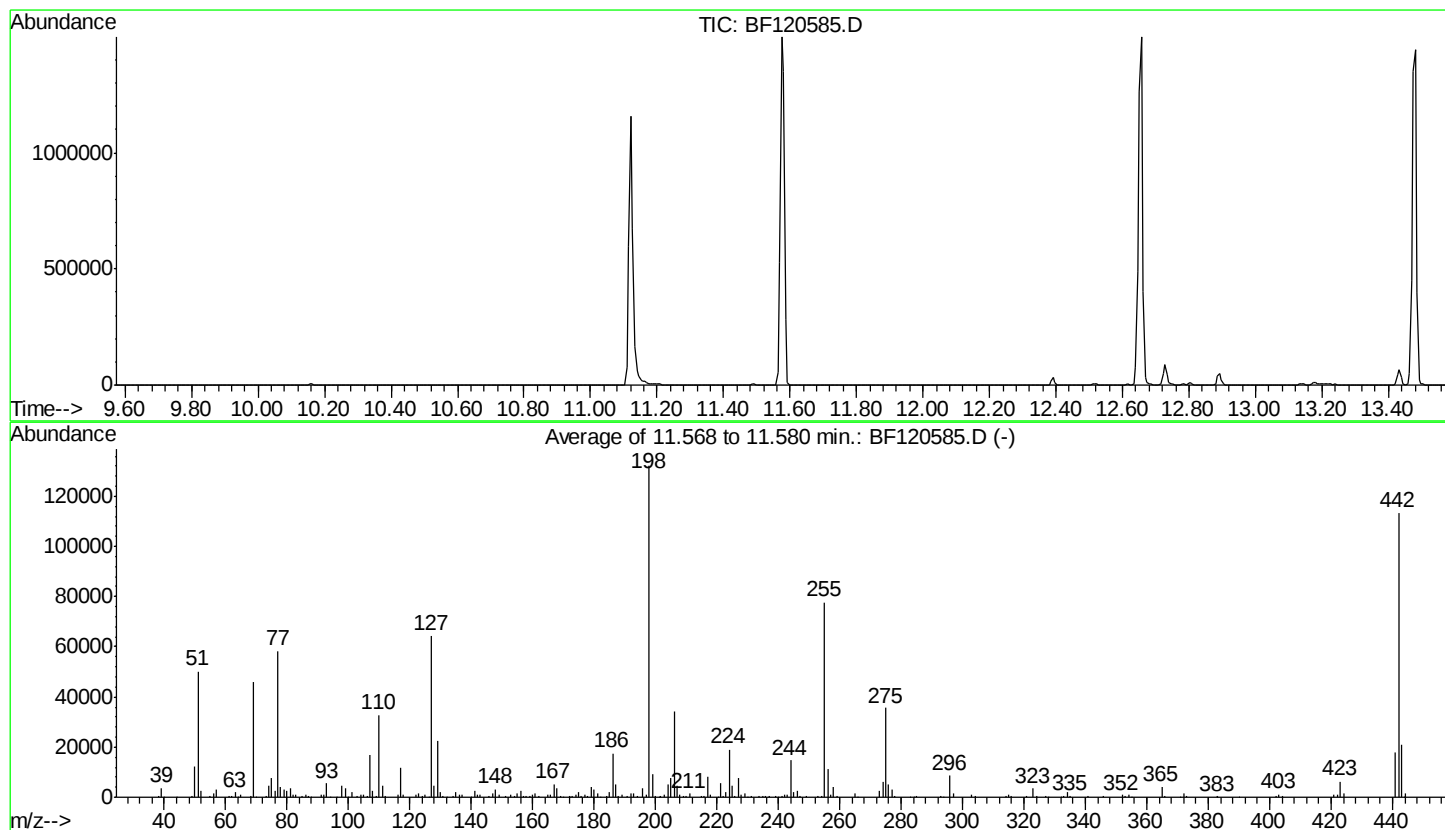

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	50141	PASS
68	69	0.00	2	1.6	731	PASS
69	198	0.00	100	34.7	45938	PASS
70	69	0.00	2	0.2	112	PASS
127	198	10	80	48.7	64392	PASS
197	198	0.00	2	0.8	1015	PASS
198	198	100	100	100.0	132234	PASS
199	198	5	9	6.8	8954	PASS
275	198	10	60	27.0	35703	PASS
365	198	1	100	3.2	4274	PASS
441	198	0.01	100	13.5	17829	PASS
442	198	50	100	85.7	113365	PASS
443	442	15	24	18.6	21051	PASS