
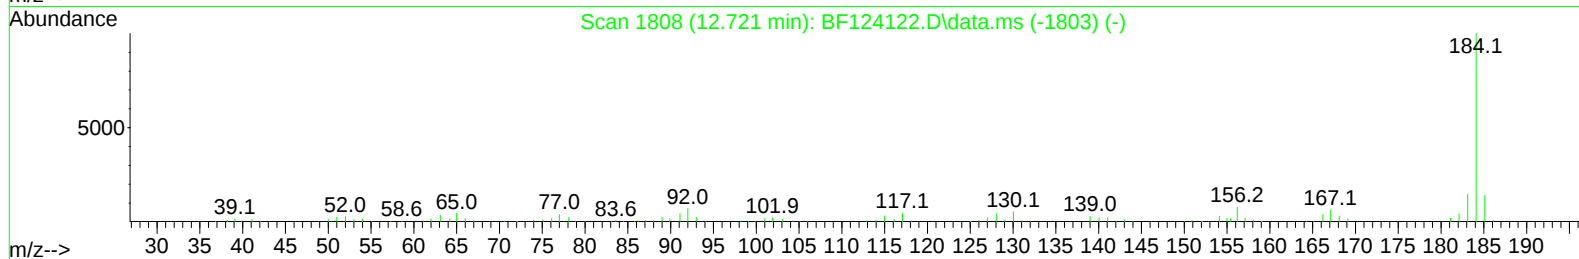
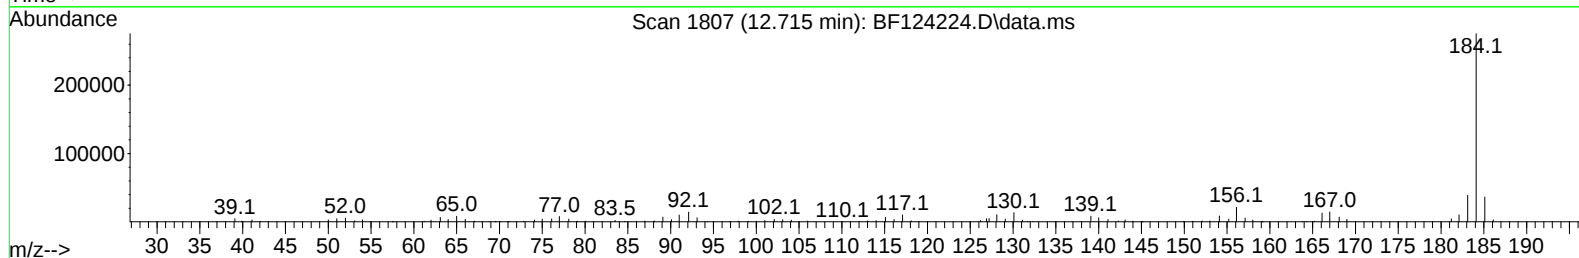


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\  
Data File : BF124224.D  
Acq On    : 10 Jun 2021    9:16  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 10 11:28:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

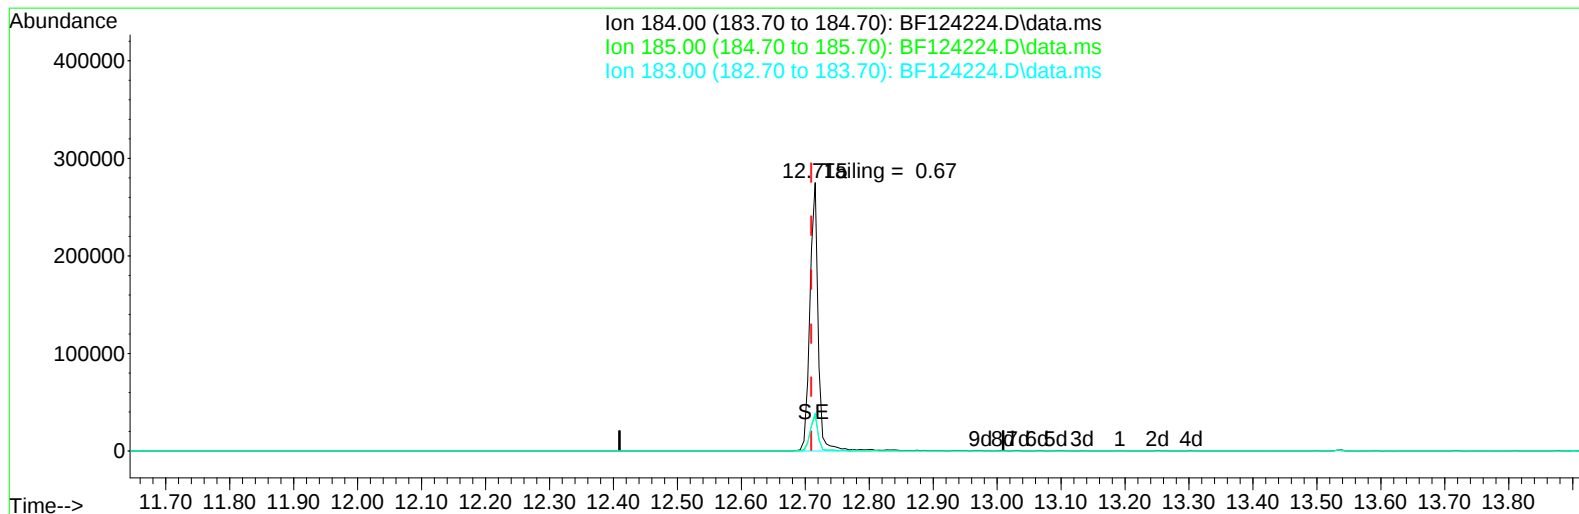

TIC: BF124224.D\data.ms

(77) Benzidine

12.715min (+ 0.006) 87525.96 ng m

response **251796**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------




185.00	15.10	13.24
--------	-------	-------

183.00 9.80 14.13#

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124224.D
Acq On : 10 Jun 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:28:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

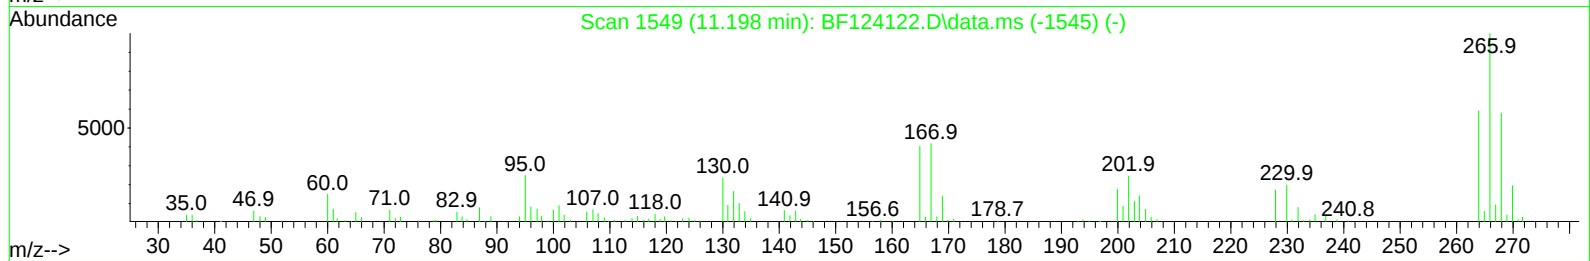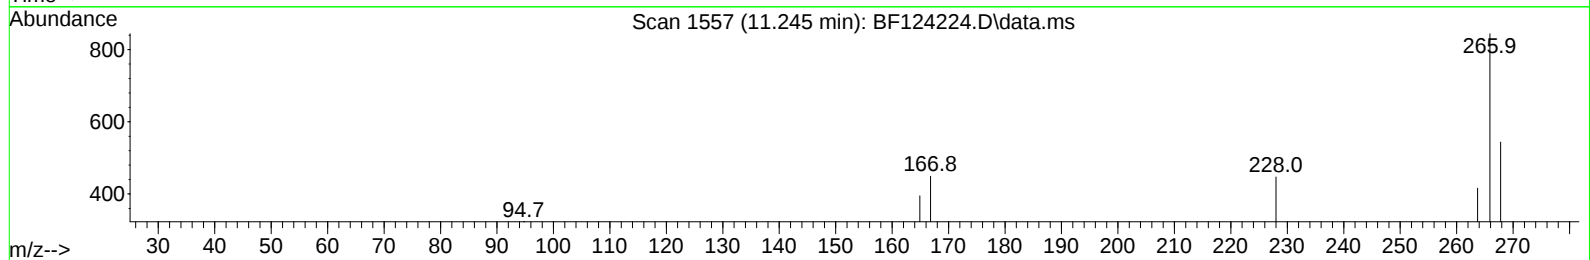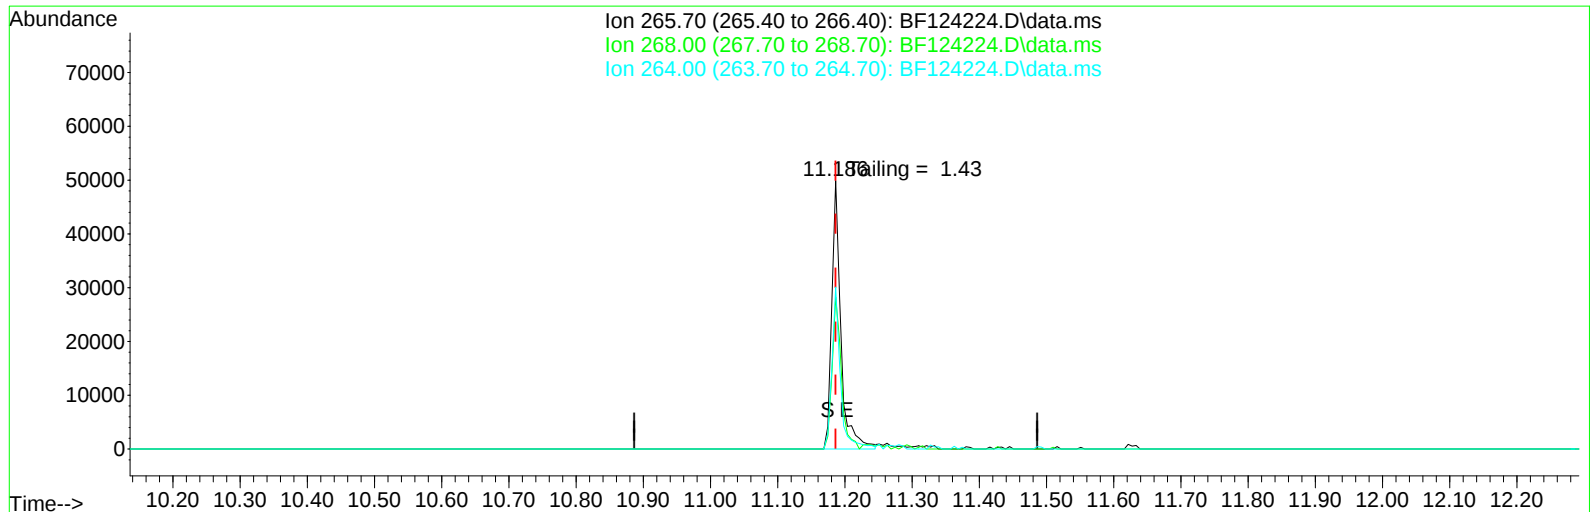

TIC: BF124224.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 9965.84 ng

response 48962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	56.59
264.00	65.70	60.37
0.00	0.00	0.00