
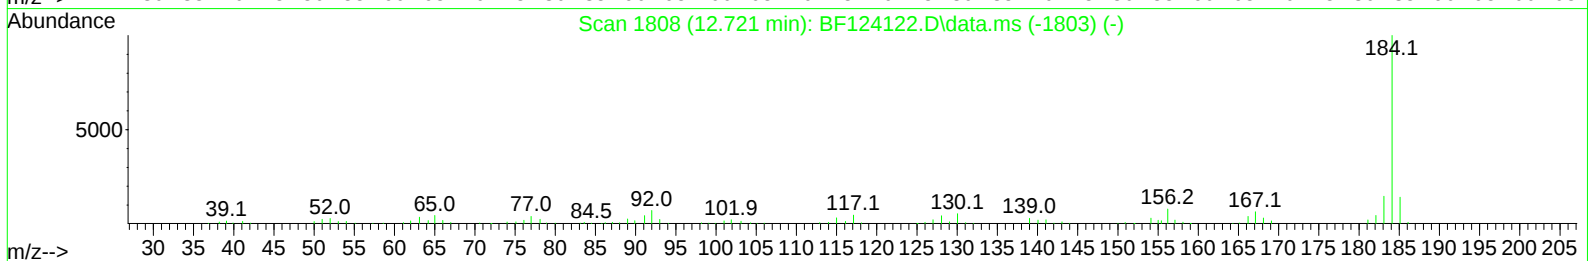
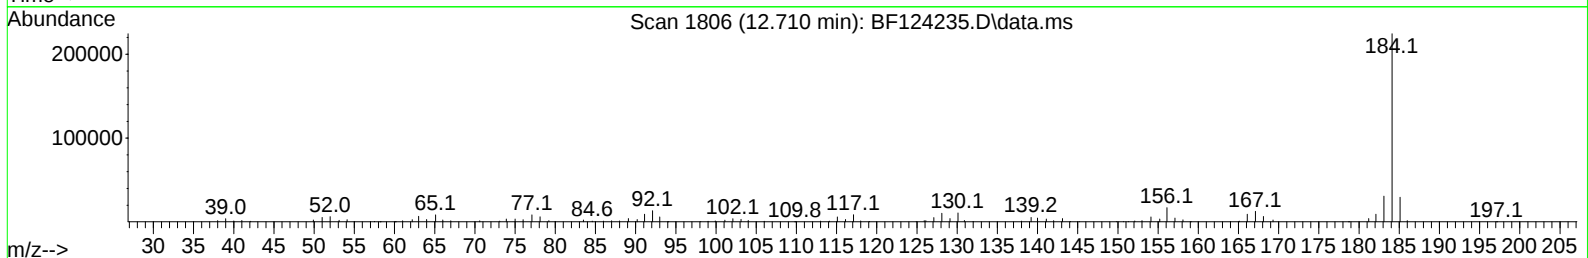


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124235.D
 Acq On : 10 Jun 2021 16:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 17:14:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

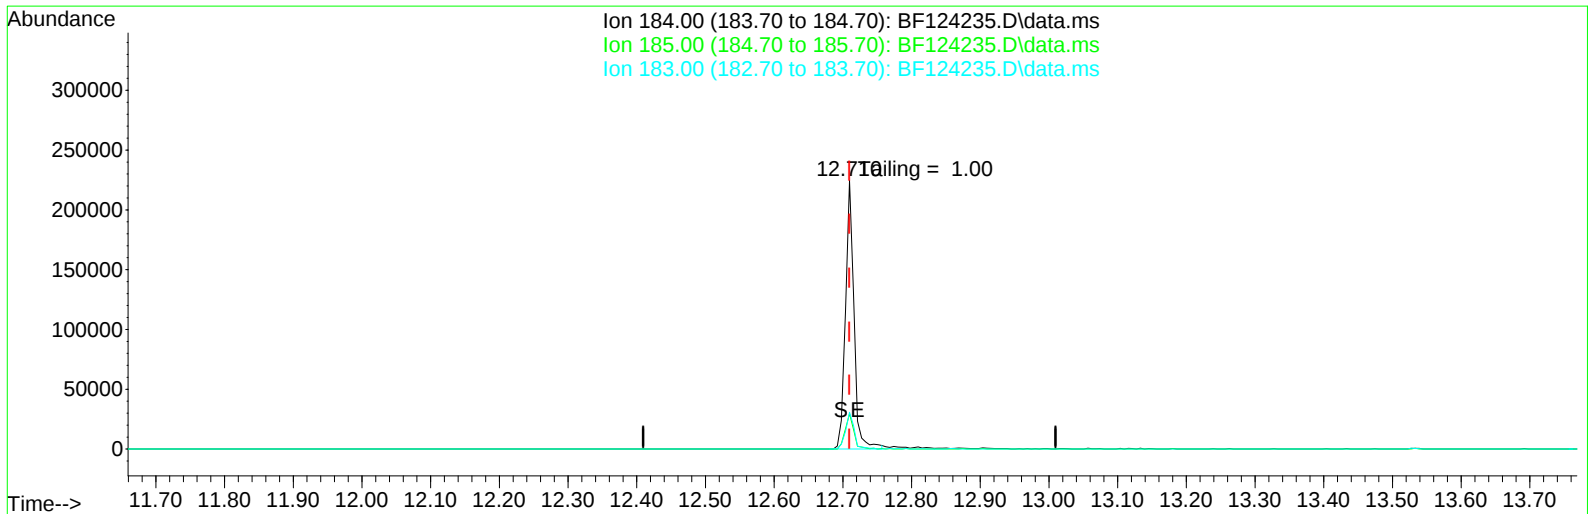

TIC: BF124235.D\data.ms

(77) Benzidine




12.710min (+ 0.000) 0.00 ng

response 194830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.11
183.00	9.80	13.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124235.D
Acq On : 10 Jun 2021 16:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 17:14:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

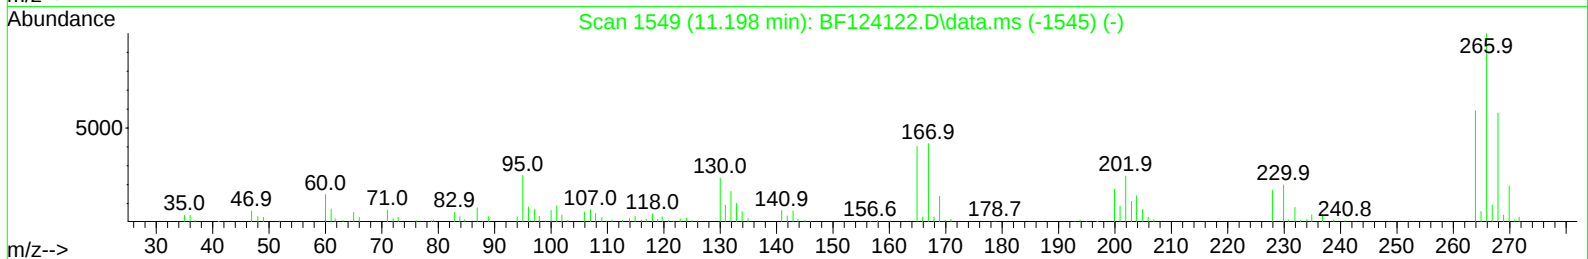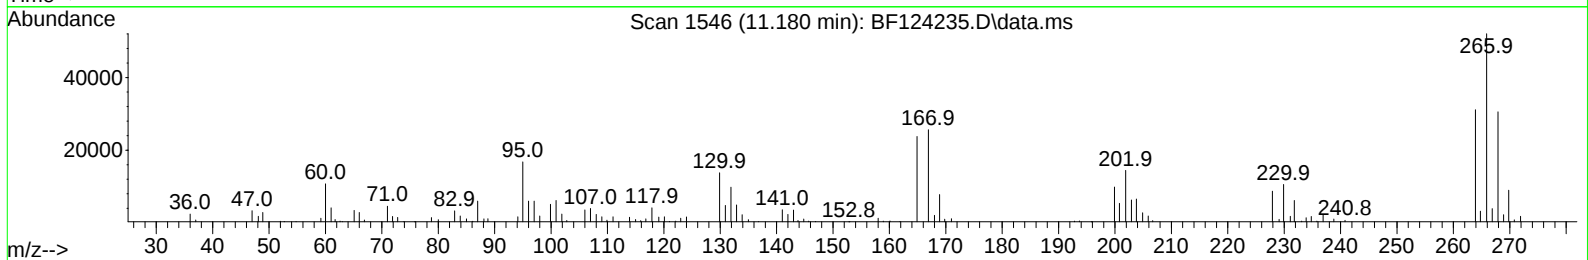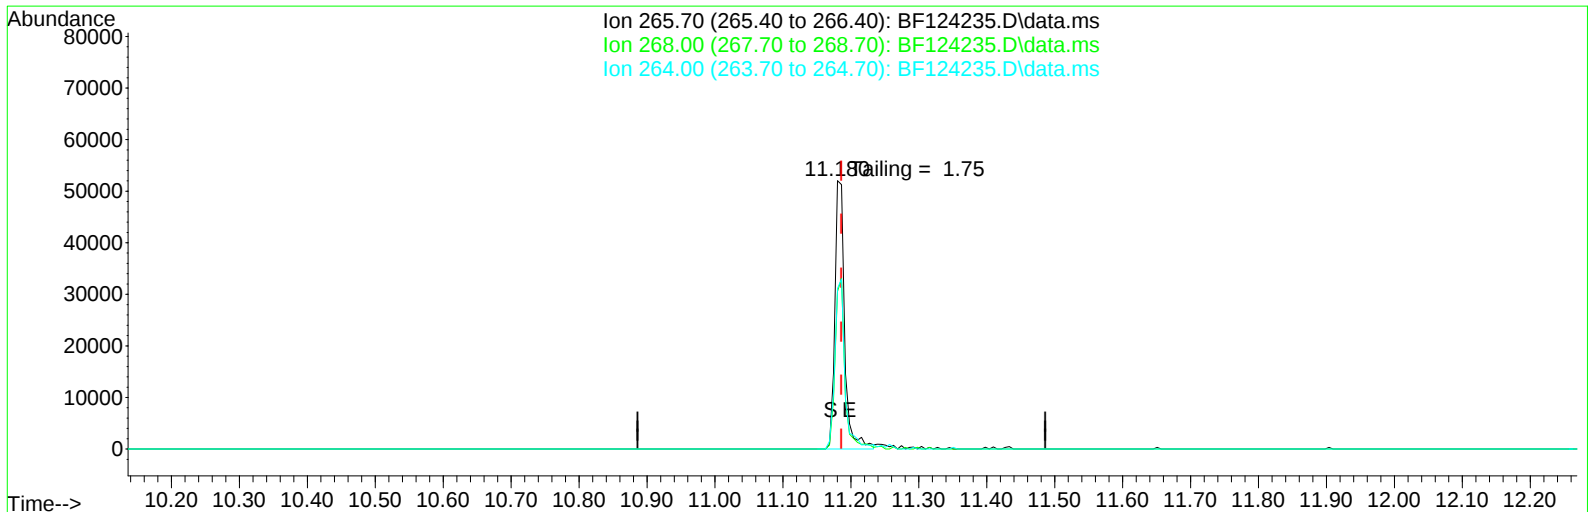

TIC: BF124235.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.006) 13238.78 ng

response 53306

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.75
264.00	65.70	59.81
0.00	0.00	0.00