

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124228.D
 Acq On : 10 Jun 2021 12:12
 Operator : JU/CG
 Sample : PB136974BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136974BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.193	6	18	24	rBB2	38705	58654	3.18%	0.554%
2	2.293	30	35	42	rBB	26608	35526	1.93%	0.336%
3	5.093	506	511	518	rBB	32841	47691	2.59%	0.451%
4	5.493	574	579	582	rBV	1427352	1319317	71.54%	12.464%
5	6.492	744	749	752	rBV	1233513	1289579	69.93%	12.183%
6	6.845	806	809	813	rBV	326146	274103	14.86%	2.590%
7	7.416	900	906	909	rBV	896506	886831	48.09%	8.378%
8	8.128	1023	1027	1031	rBV	357270	349387	18.95%	3.301%
9	9.210	1205	1211	1214	rBV	2106098	1731318	93.88%	16.356%
10	9.886	1320	1326	1329	rBV	568099	427238	23.17%	4.036%
11	10.680	1456	1461	1464	rBV	1371622	1188749	64.46%	11.231%
12	11.374	1575	1579	1582	rBV	574661	437202	23.71%	4.130%
13	12.963	1844	1849	1852	rBV	2099975	1844193	100.00%	17.423%
14	14.015	2024	2028	2033	rVB	373194	319267	17.31%	3.016%
15	15.498	2274	2280	2287	rBV	206173	279761	15.17%	2.643%
16	15.945	2353	2356	2361	rVB3	19736	28302	1.53%	0.267%
17	16.462	2439	2444	2446	rBV5	20488	34109	1.85%	0.322%
18	17.056	2540	2545	2553	rVB7	18801	33672	1.83%	0.318%




Sum of corrected areas: 10584899

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124228.D
Acq On : 10 Jun 2021 12:12
Operator : JU/CG
Sample : PB136974BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136974BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

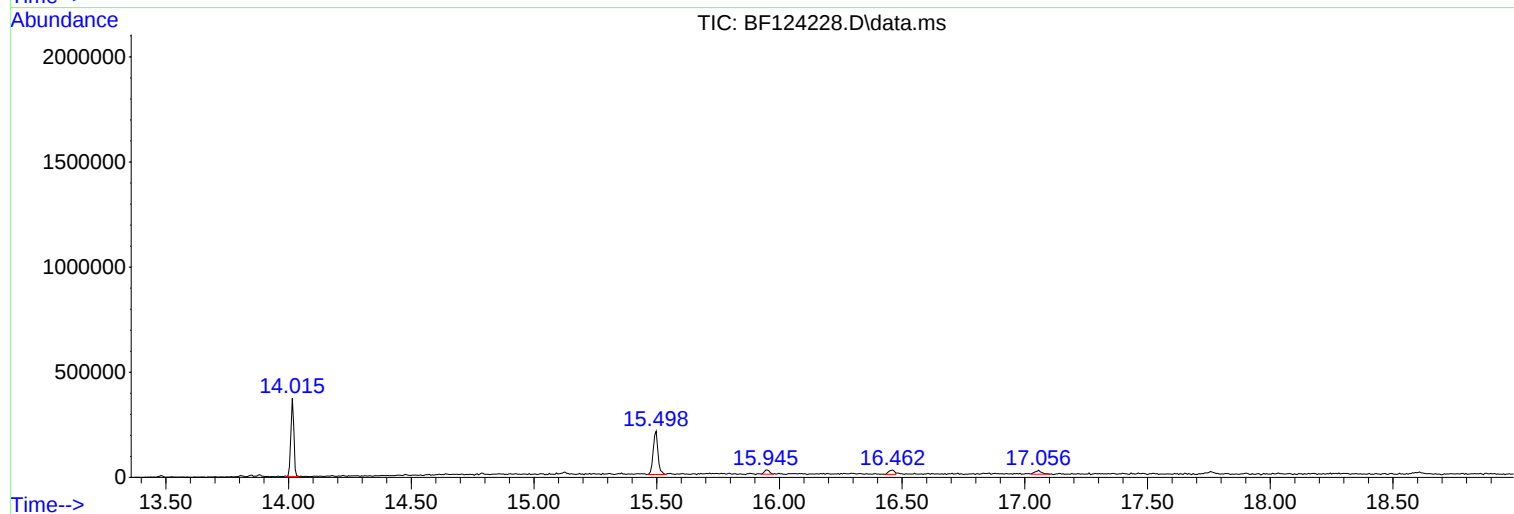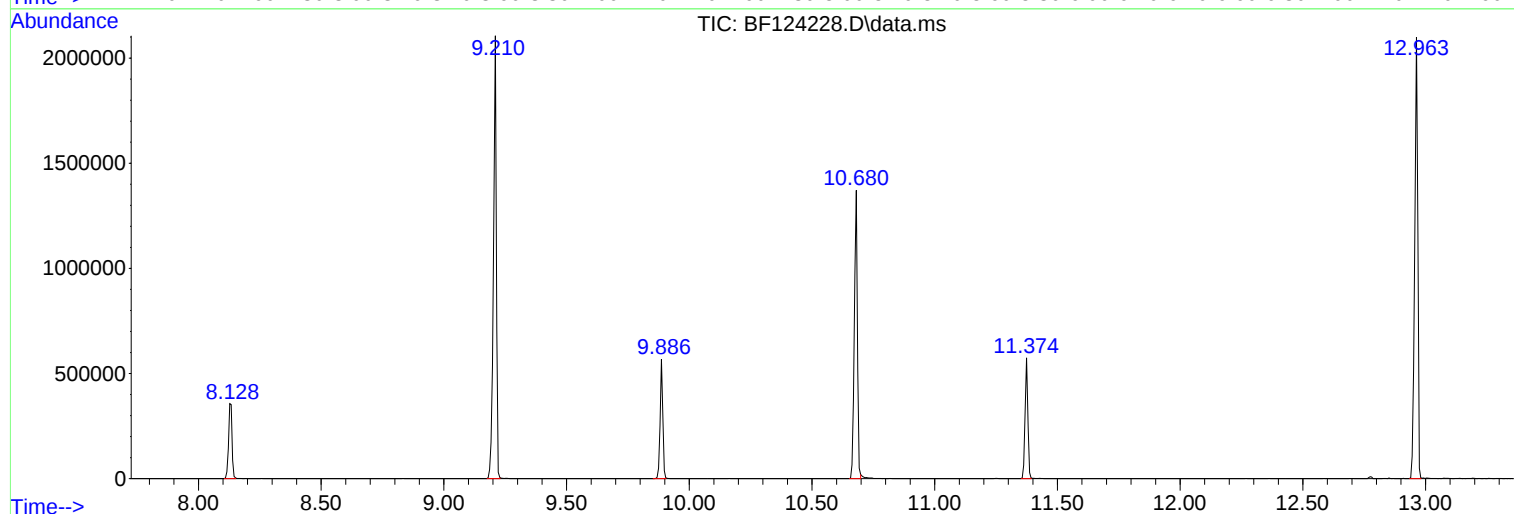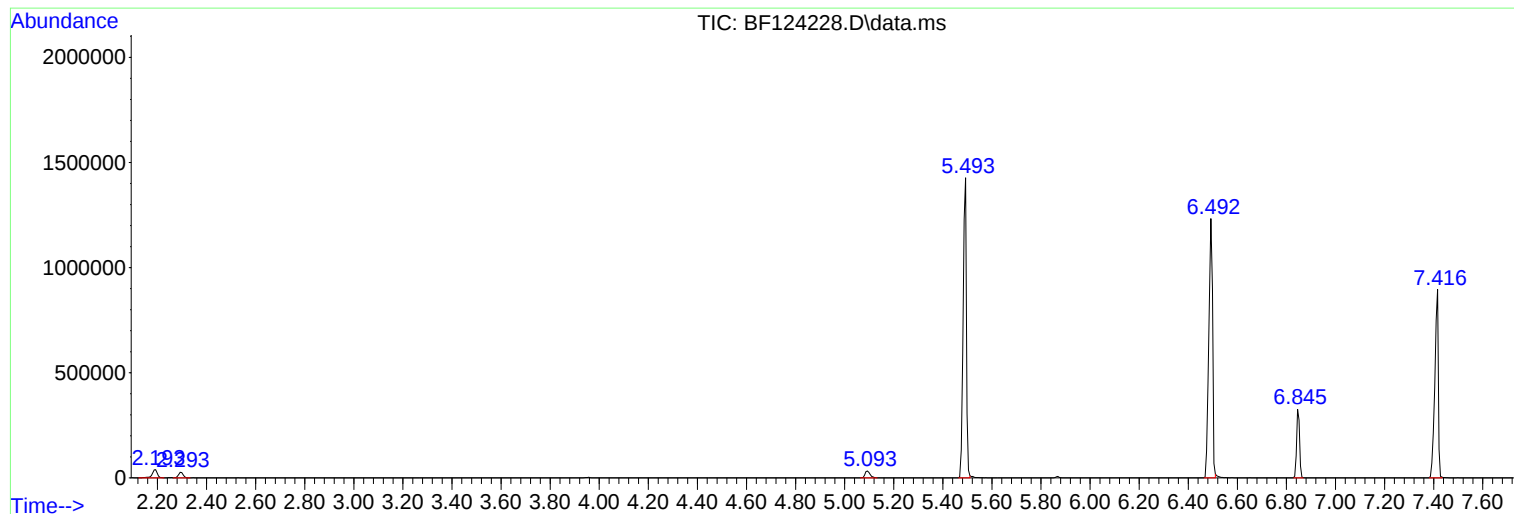

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124228.D
Acq On : 10 Jun 2021 12:12
Operator : JU/CG
Sample : PB136974BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136974BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124228.D
Acq On : 10 Jun 2021 12:12
Operator : JU/CG
Sample : PB136974BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136974BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------