


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124224.D
 Acq On : 10 Jun 2021 9:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 10 01:53:56 2021

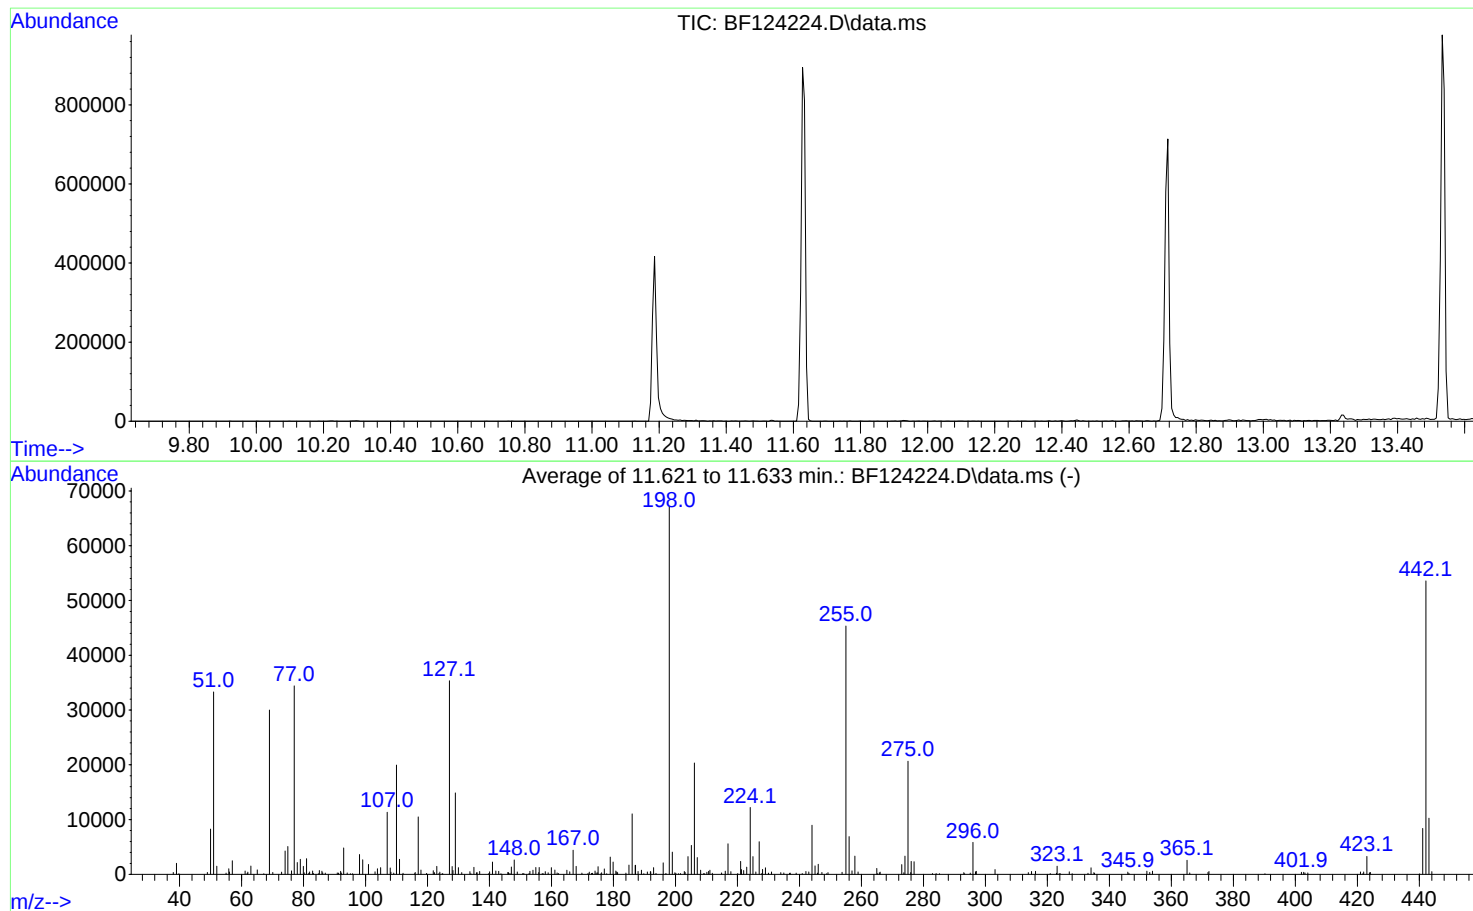




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	33293	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.7	29992	PASS
70	69	0.00	2	1.1	341	PASS
127	198	10	80	52.6	35349	PASS
197	198	0.00	2	0.3	180	PASS
198	198	100	100	100.0	67160	PASS
199	198	5	9	6.1	4070	PASS
275	198	10	60	30.8	20662	PASS
365	198	1	100	3.8	2566	PASS
441	198	0.01	100	12.5	8385	PASS
442	442	50	100	100.0	53589	PASS
443	442	15	24	19.2	10264	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124224.D
 Acq On : 10 Jun 2021 9:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 11:28:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

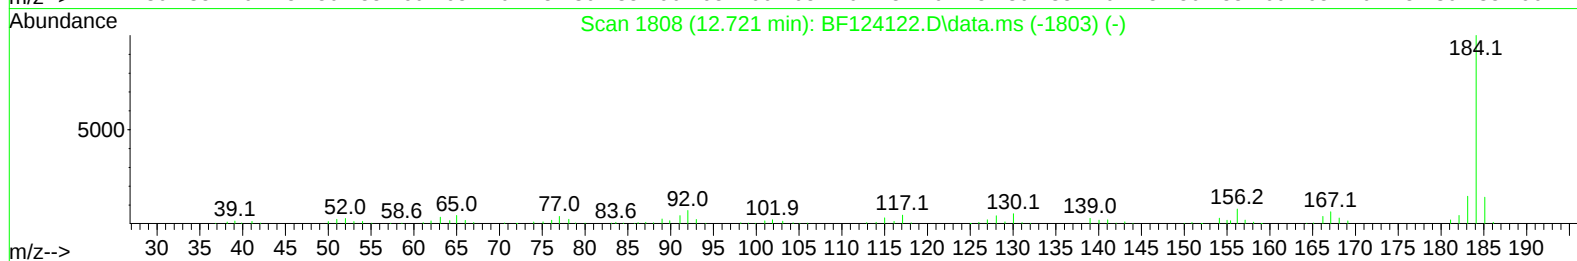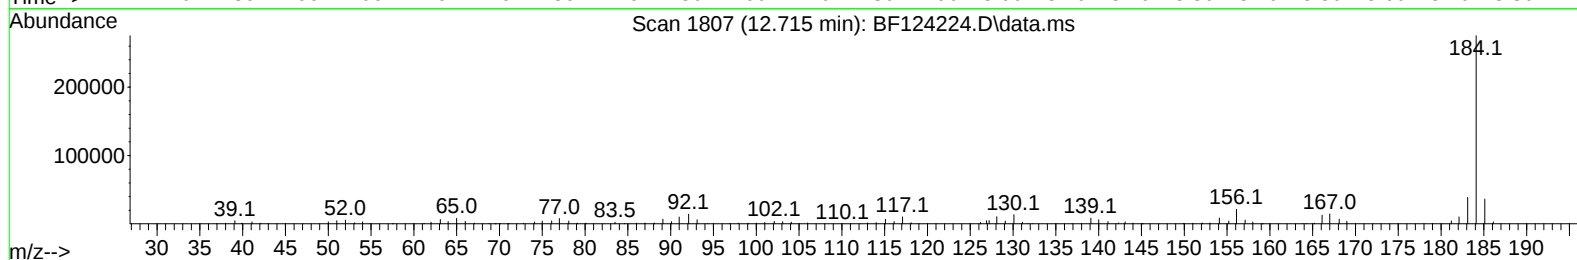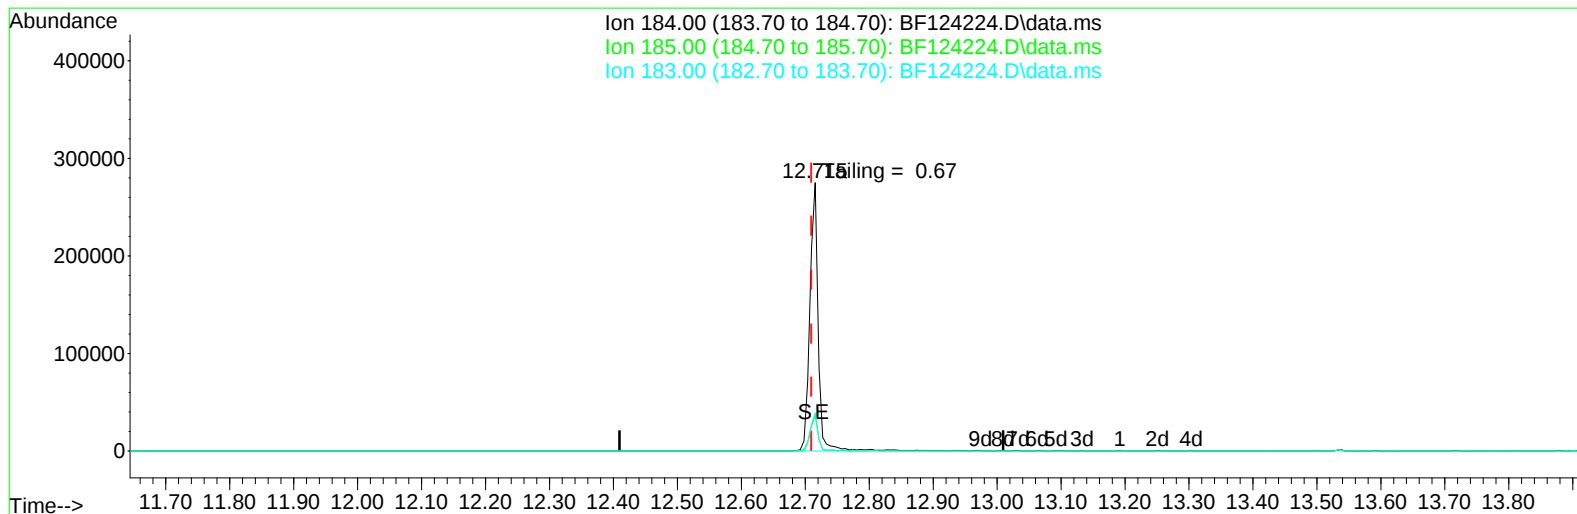

TIC: BF124224.D\data.ms

(77) Benzidine

12.715min (+ 0.006) 87525.96 ng m




response 251796

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.24
183.00	9.80	14.13#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124224.D
Acq On : 10 Jun 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:28:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

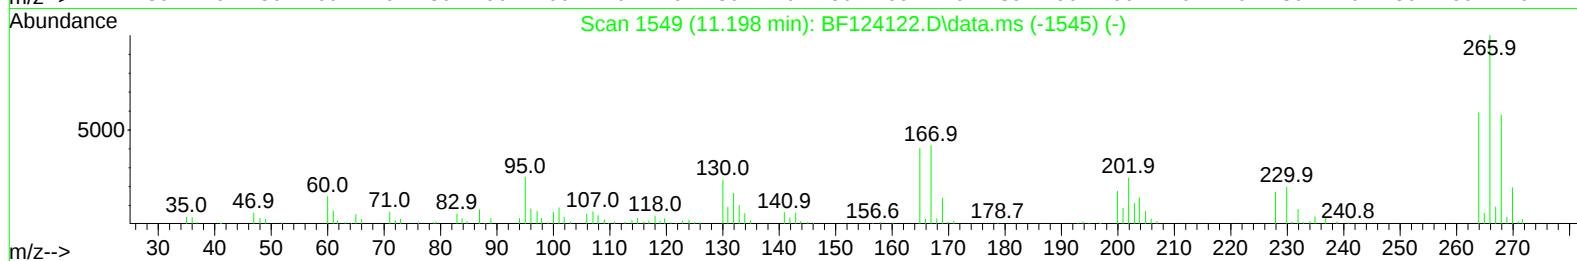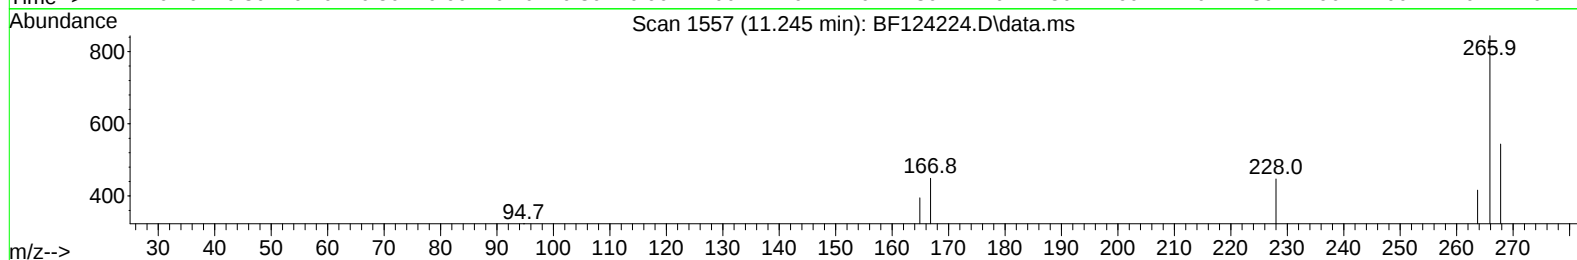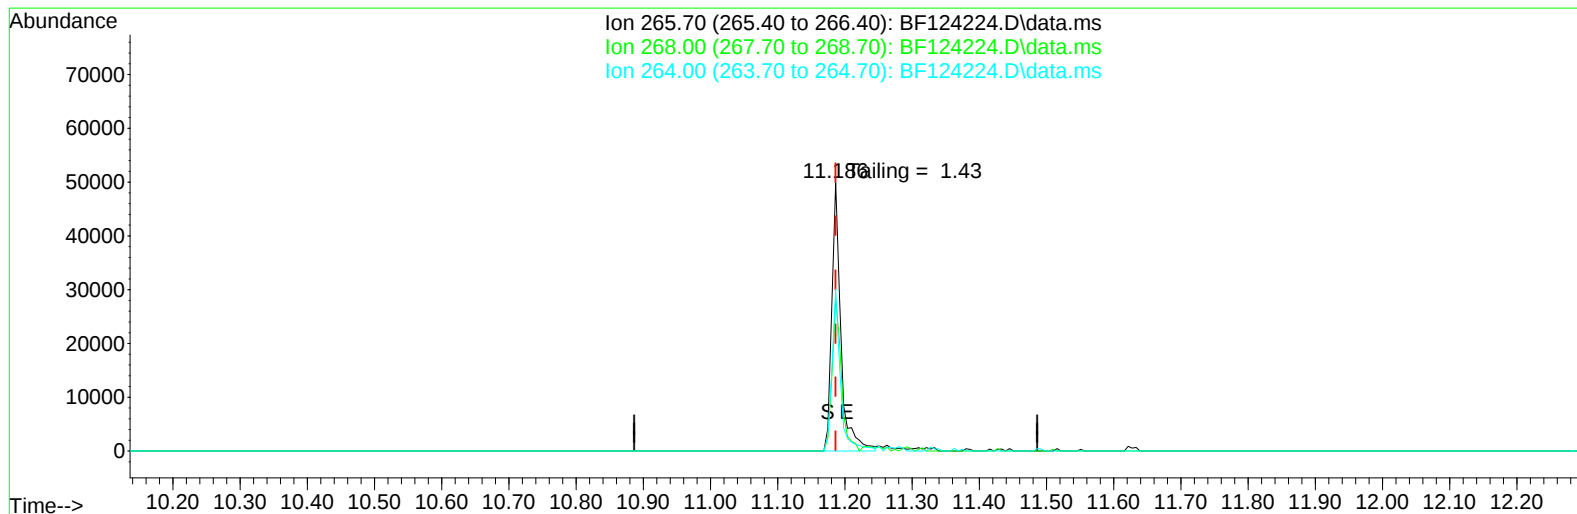

TIC: BF124224.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 9965.84 ng

response 48962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	56.59
264.00	65.70	60.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2021	BNA_F	<u>BF124224.D</u>
Compound Name	Response	Retention Time
DDT	154895	13.53
DDD	3839	13.23
DDE	726	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4565	159460	2.86

Instrument :
BNA_F
ClientSampleId :
DFTPP