
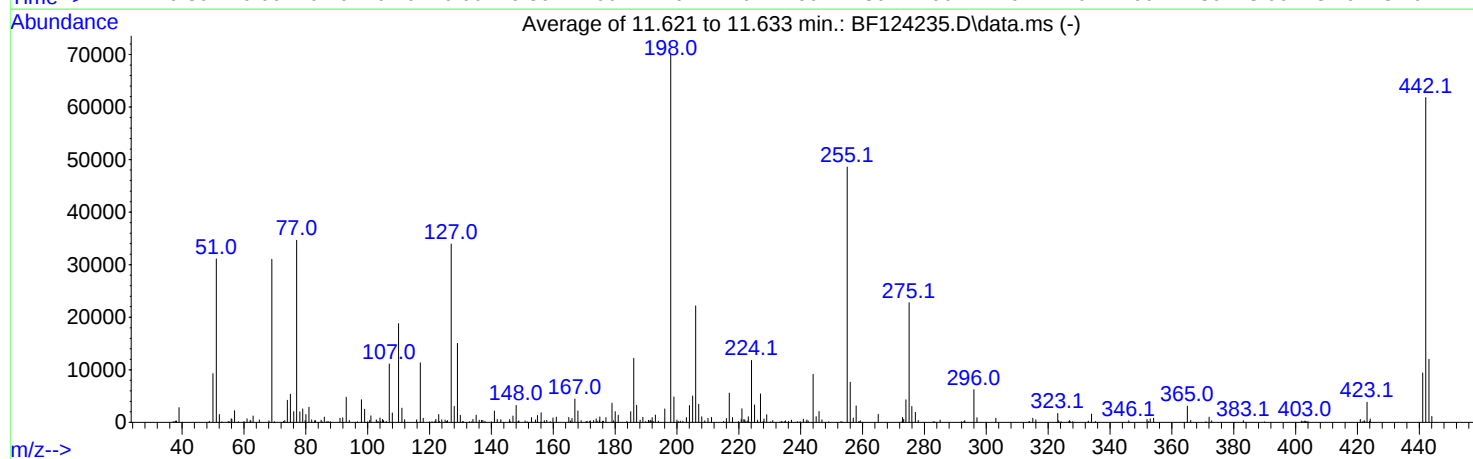


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124235.D
 Acq On : 10 Jun 2021 16:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 10 01:53:56 2021

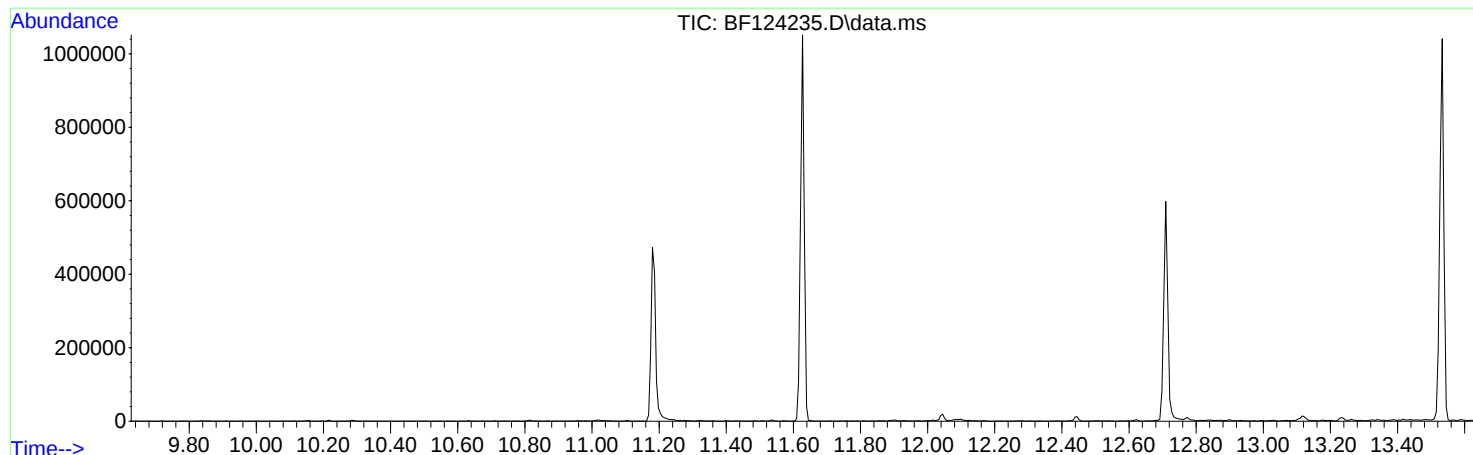




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	31121	PASS
68	69	0.00	2	1.0	296	PASS
69	198	0.00	100	44.3	31016	PASS
70	69	0.00	2	0.4	119	PASS
127	198	10	80	48.5	33955	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69997	PASS
199	198	5	9	6.9	4848	PASS
275	198	10	60	32.5	22782	PASS
365	198	1	100	4.4	3084	PASS
441	198	0.01	100	13.4	9396	PASS
442	442	50	100	100.0	61797	PASS
443	442	15	24	19.4	12011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
Data File : BF124235.D
Acq On : 10 Jun 2021 16:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 17:14:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

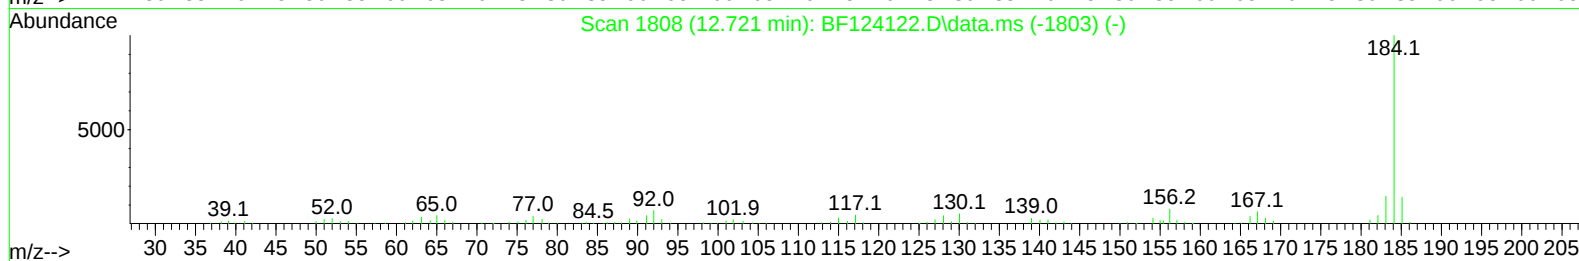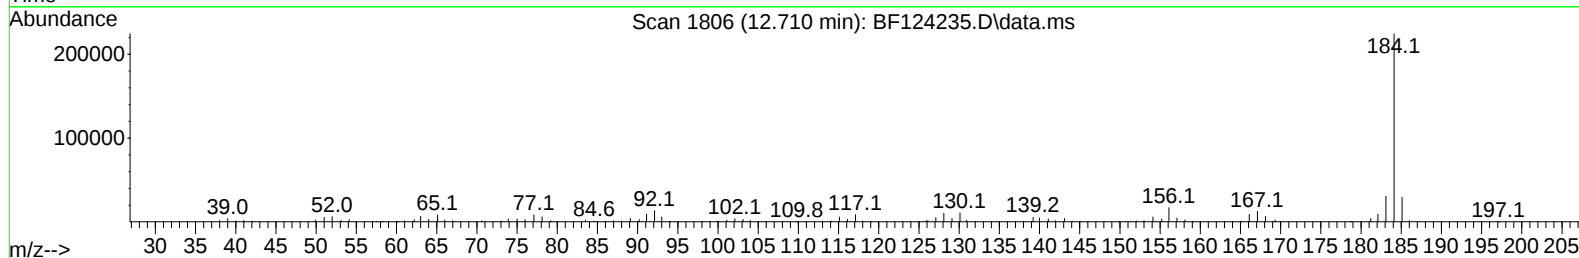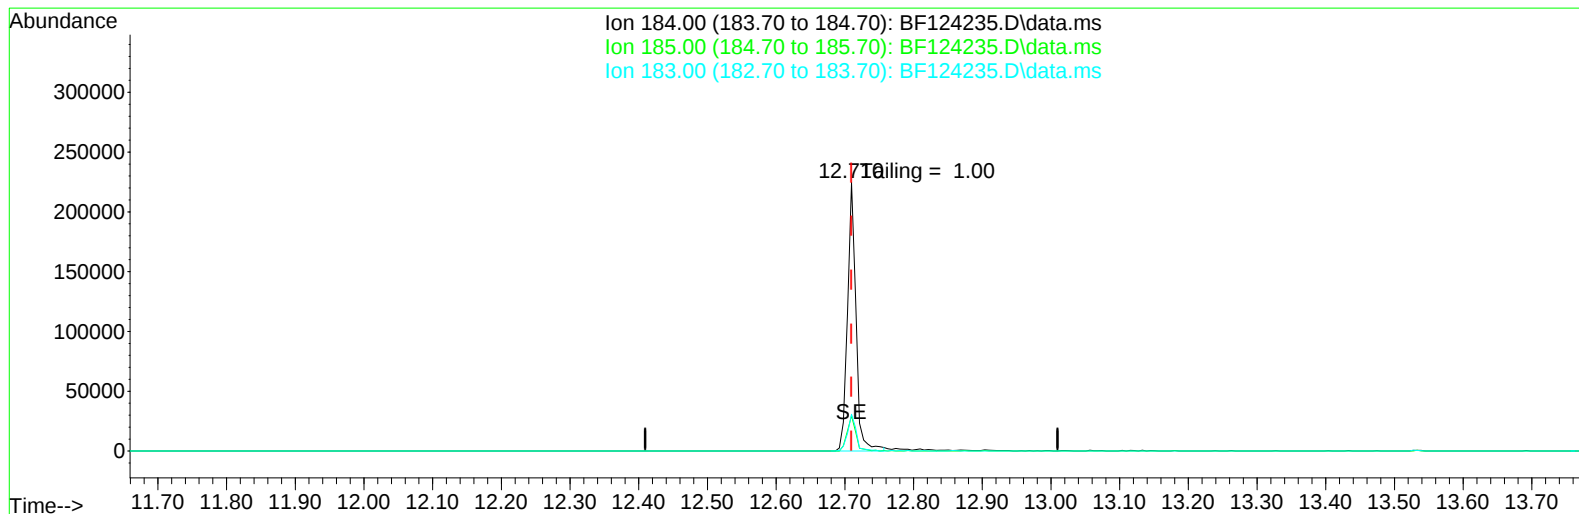

TIC: BF124235.D\data.ms

(77) Benzidine

12.710min (+ 0.000) 0.00 ng




response 194830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.11
183.00	9.80	13.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061021\
 Data File : BF124235.D
 Acq On : 10 Jun 2021 16:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 17:14:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

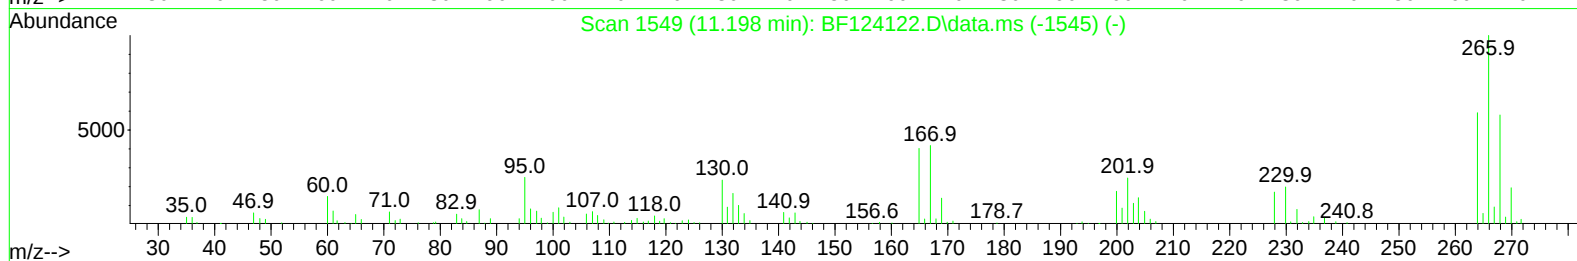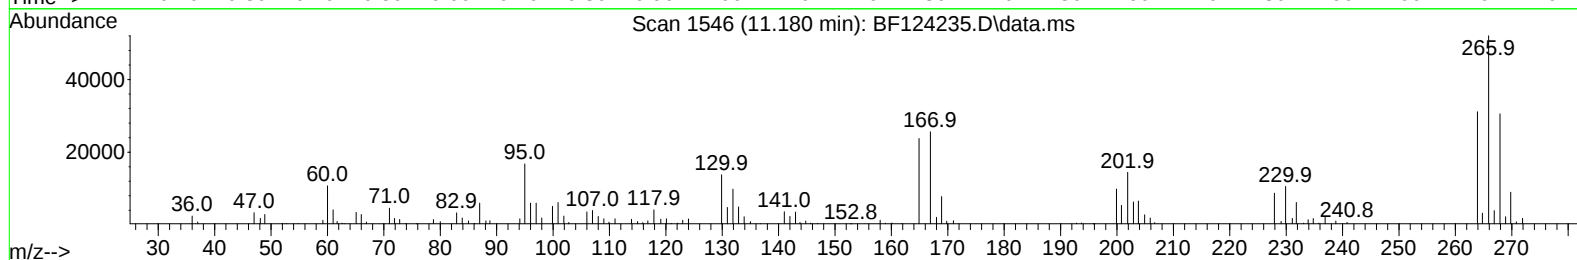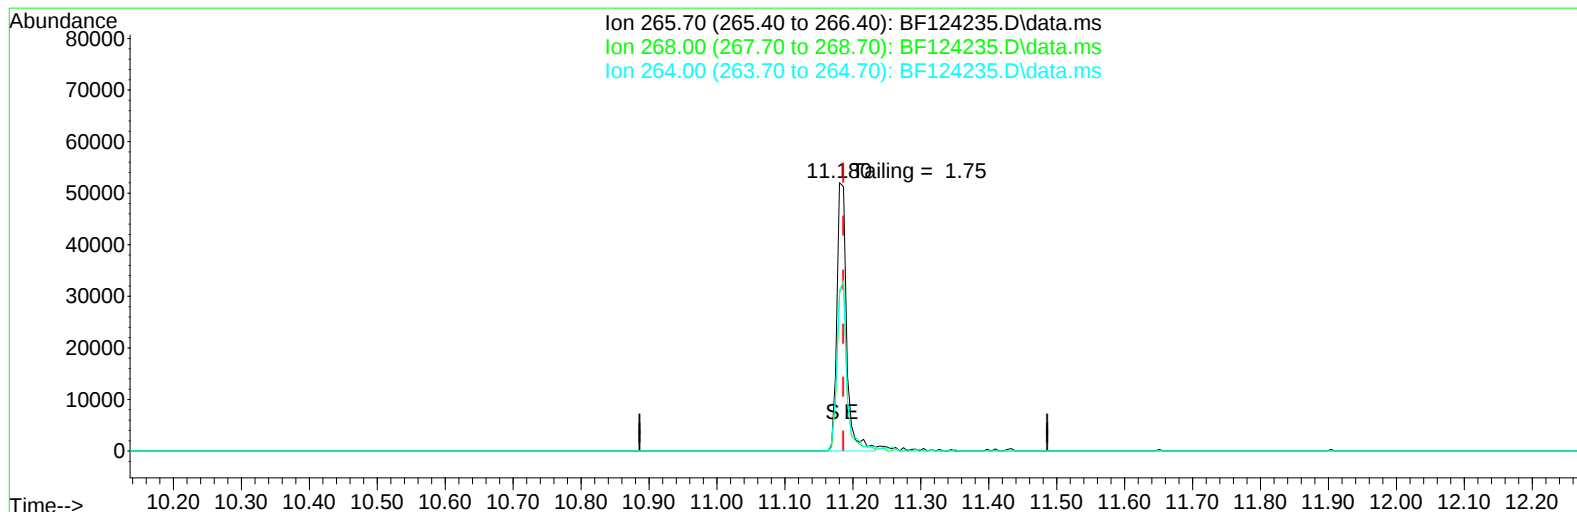

TIC: BF124235.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.006) 13238.78 ng

response 53306

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.75
264.00	65.70	59.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2021	BNA_F	<u>BF124235.D</u>
Compound Name	Response	Retention Time
DDT	155954	13.53
DDD	1985	13.23
DDE	398	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2383	158337	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP