

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061022\
 Data File : BF128765.D
 Acq On : 10 Jun 2022 18:16
 Operator : CG\JU
 Sample : N3301-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-SO-20220609

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	463	467	474	rVB	66496	91647	3.01%	0.514%
2	5.451	534	538	550	rBV	2602313	2396315	78.61%	13.446%
3	6.463	705	710	713	rBV	2580475	2438331	79.98%	13.682%
4	6.798	763	767	771	rBV	503323	395310	12.97%	2.218%
5	7.369	858	864	867	rBV	1625545	1677407	55.02%	9.412%
6	8.081	981	985	989	rBV	551506	525124	17.23%	2.947%
7	9.163	1163	1169	1172	rBV	3055639	3048518	100.00%	17.105%
8	9.839	1278	1284	1287	rBV	779543	634413	20.81%	3.560%
9	10.633	1413	1419	1423	rBV	1949074	1924441	63.13%	10.798%
10	11.327	1533	1537	1540	rBV	803159	642864	21.09%	3.607%
11	11.398	1546	1549	1552	rVB	49242	43755	1.44%	0.246%
12	11.857	1624	1627	1638	rBV2	49243	72657	2.38%	0.408%
13	12.921	1803	1808	1811	rBV	3042392	2706234	88.77%	15.185%
14	13.398	1881	1889	1894	rBV	86137	85226	2.80%	0.478%
15	13.821	1957	1961	1968	rBV2	73450	92054	3.02%	0.517%
16	13.968	1982	1986	1990	rBV	403501	372657	12.22%	2.091%
17	14.068	1997	2003	2006	rBV	99592	104560	3.43%	0.587%
18	14.821	2127	2131	2135	rVV	42236	45975	1.51%	0.258%
19	15.433	2229	2235	2243	rBV	296895	395918	12.99%	2.222%
20	15.886	2308	2312	2318	rVB2	25696	37655	1.24%	0.211%
21	16.386	2392	2397	2405	rVB4	22214	42008	1.38%	0.236%
22	16.968	2491	2496	2508	rVB7	17441	48852	1.60%	0.274%




Sum of corrected areas: 17821921

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061022\
Data File : BF128765.D
Acq On : 10 Jun 2022 18:16
Operator : CG\JU
Sample : N3301-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-SO-20220609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

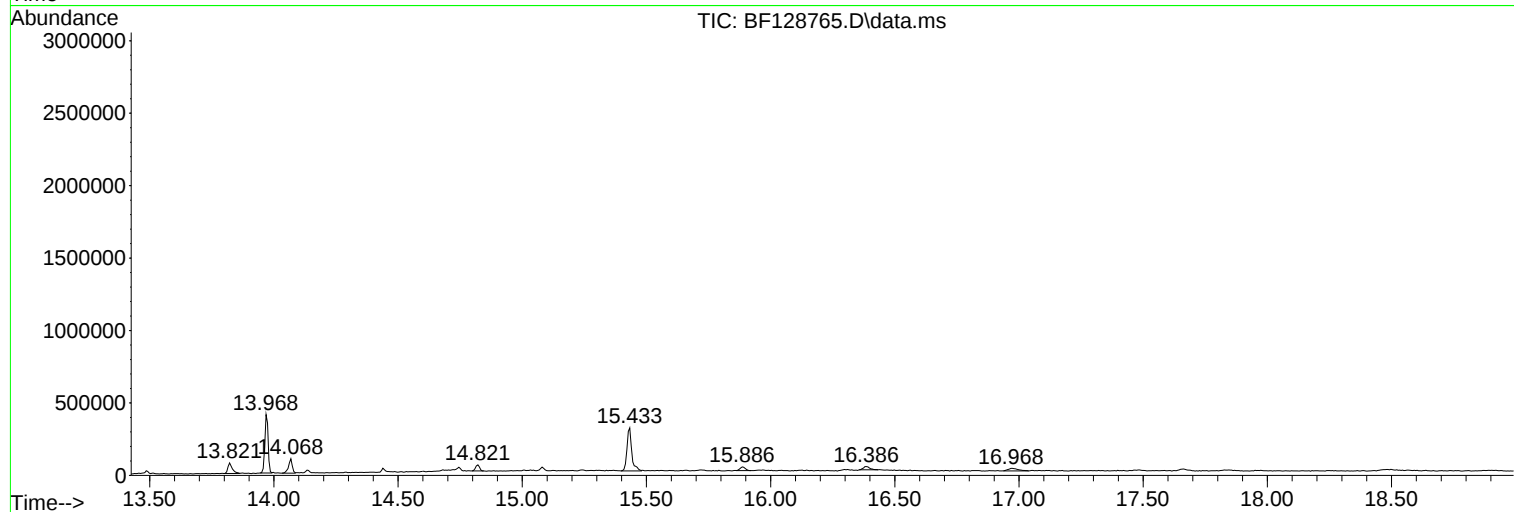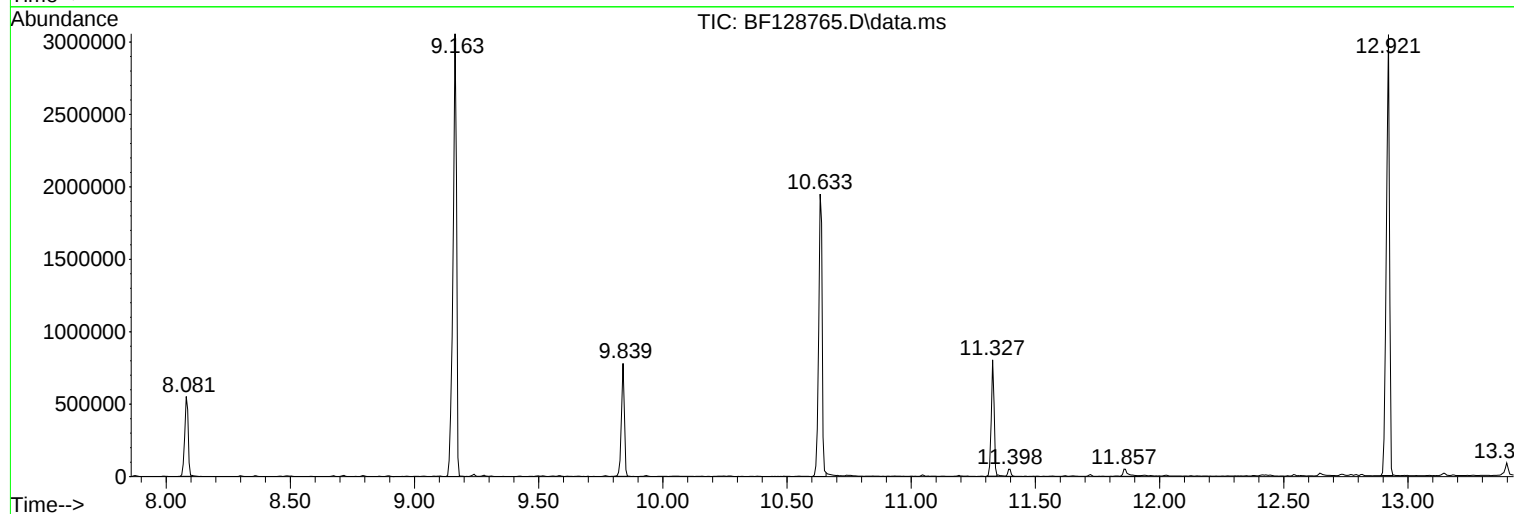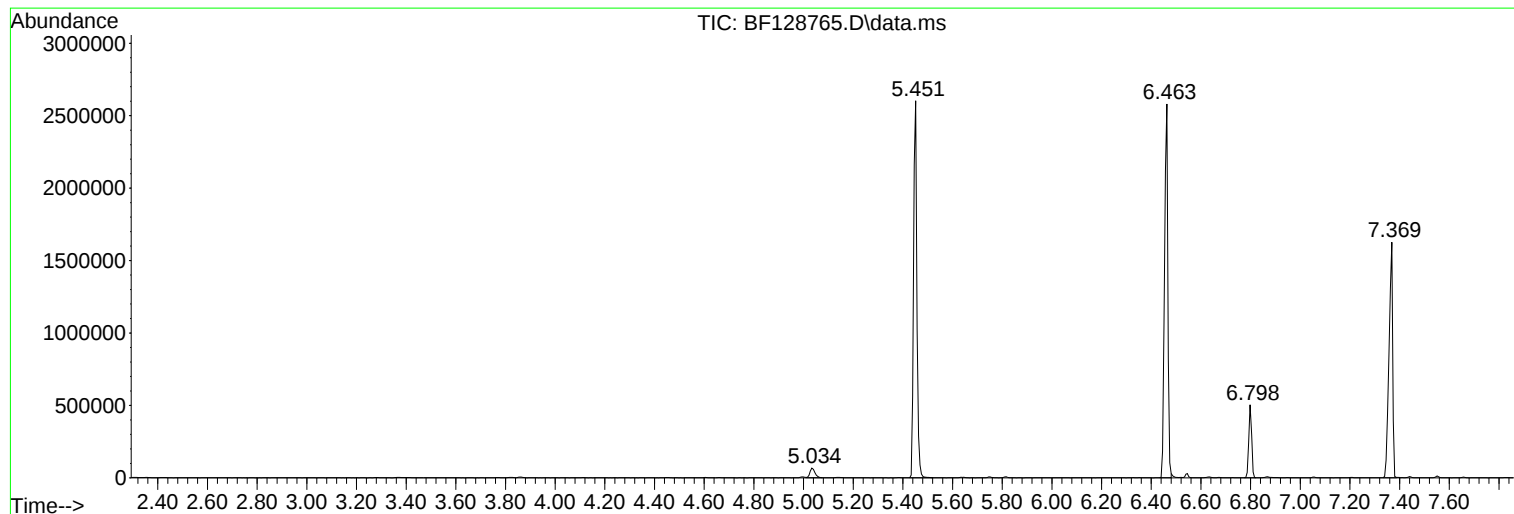

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061022\
Data File : BF128765.D
Acq On : 10 Jun 2022 18:16
Operator : CG\JU
Sample : N3301-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-SO-20220609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061022\
Data File : BF128765.D
Acq On : 10 Jun 2022 18:16
Operator : CG\JU
Sample : N3301-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-SO-20220609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------