

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
 Data File : BF138177.D
 Acq On : 10 Jun 2024 17:38
 Operator : CG\JU
 Sample : P2795-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1-(0-5)-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	13	20	26	rVB	5112616	6414906	82.66%	9.877%
2	5.116	512	515	521	rVB	320685	342506	4.41%	0.527%
3	5.516	576	583	586	rBV	6910634	6318105	81.42%	9.728%
4	6.516	748	753	756	rBV	6401230	6513558	83.93%	10.029%
5	6.716	784	787	793	rBV	126524	119094	1.53%	0.183%
6	6.892	814	817	821	rVB	2805055	2392505	30.83%	3.684%
7	7.457	908	913	916	rBV	4576983	3791014	48.85%	5.837%
8	8.175	1031	1035	1038	rBV	3922099	3212120	41.39%	4.946%
9	9.251	1214	1218	1221	rBV	9529831	7760299	100.00%	11.949%
10	9.927	1330	1333	1337	rVB	4136614	3580730	46.14%	5.513%
11	10.251	1379	1388	1400	rBV	117745	468440	6.04%	0.721%
12	10.716	1463	1467	1470	rBV	5196210	4228160	54.48%	6.510%
13	11.416	1582	1586	1588	rBV	4093895	3326927	42.87%	5.122%
14	11.439	1588	1590	1593	rVV	1055063	752737	9.70%	1.159%
15	11.486	1593	1598	1601	rVB	159100	171913	2.22%	0.265%
16	11.639	1619	1624	1627	rBV2	81070	93433	1.20%	0.144%
17	11.945	1673	1676	1680	rVB	395297	339312	4.37%	0.522%
18	12.027	1686	1690	1692	rBV	136827	132901	1.71%	0.205%
19	12.633	1789	1793	1797	rBV	1250054	949466	12.23%	1.462%
20	12.721	1805	1808	1811	rBV	106827	98448	1.27%	0.152%
21	12.857	1824	1831	1834	rBV	852265	847059	10.92%	1.304%
22	13.004	1852	1856	1859	rBV	6969869	5986515	77.14%	9.217%
23	13.233	1892	1895	1900	rBV3	65256	95510	1.23%	0.147%
24	13.486	1934	1938	1943	rBV	197536	243538	3.14%	0.375%
25	13.798	1987	1991	1994	rBV2	57964	91274	1.18%	0.141%
26	13.904	2005	2009	2018	rBV3	166439	255979	3.30%	0.394%
27	14.051	2029	2034	2037	rBV2	2643956	2539454	32.72%	3.910%
28	14.074	2037	2038	2045	rVB	380195	309793	3.99%	0.477%
29	14.839	2165	2168	2178	rVB3	59951	91303	1.18%	0.141%
30	15.092	2207	2211	2215	rBV	302026	502414	6.47%	0.774%
31	15.398	2259	2263	2270	rVB	174675	221342	2.85%	0.341%
32	15.462	2270	2274	2280	rBV	243159	286917	3.70%	0.442%
33	15.527	2280	2285	2290	rBV	1758396	2196489	28.30%	3.382%
34	17.003	2531	2536	2547	rVB2	77432	157298	2.03%	0.242%
35	17.451	2607	2612	2622	rVB2	54031	116120	1.50%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138177.D
Acq On : 10 Jun 2024 17:38
Operator : CG\JU
Sample : P2795-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1-(0-5)-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 64947579

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138177.D
Acq On : 10 Jun 2024 17:38
Operator : CG\JU
Sample : P2795-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1-(0-5)-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

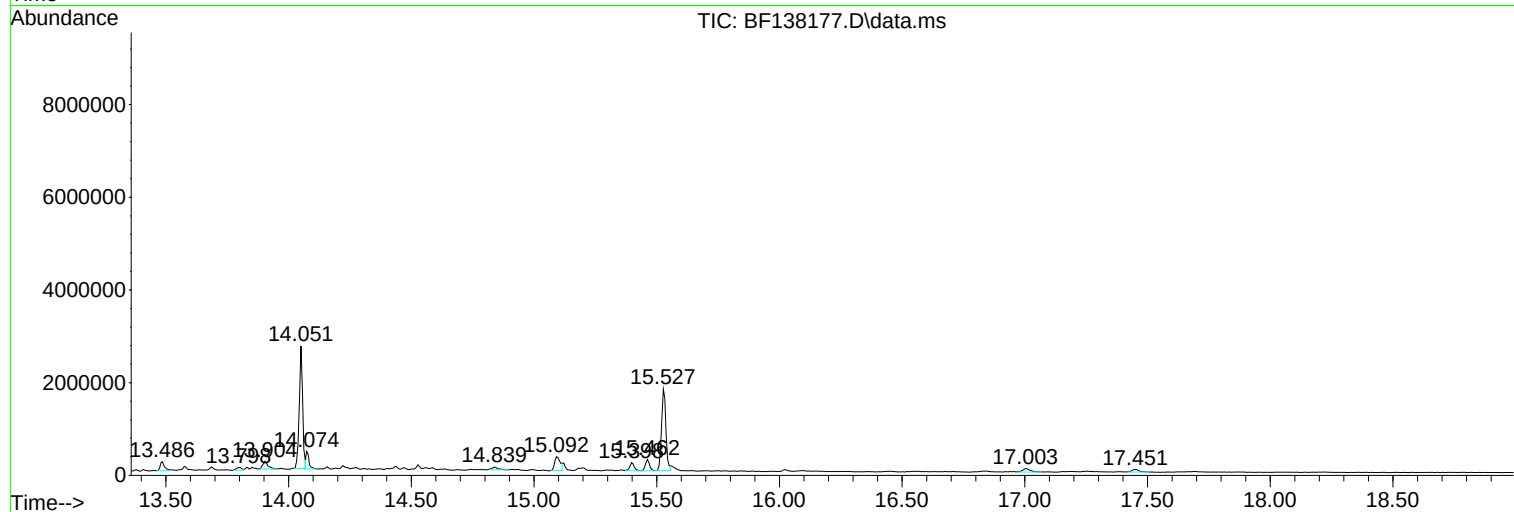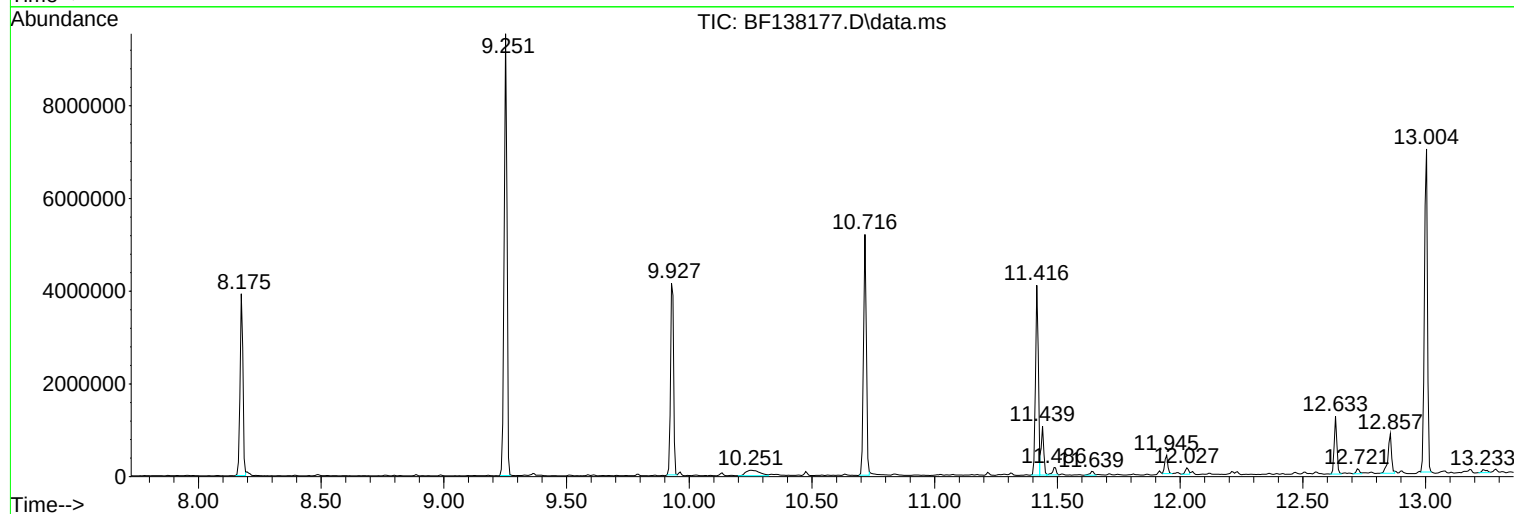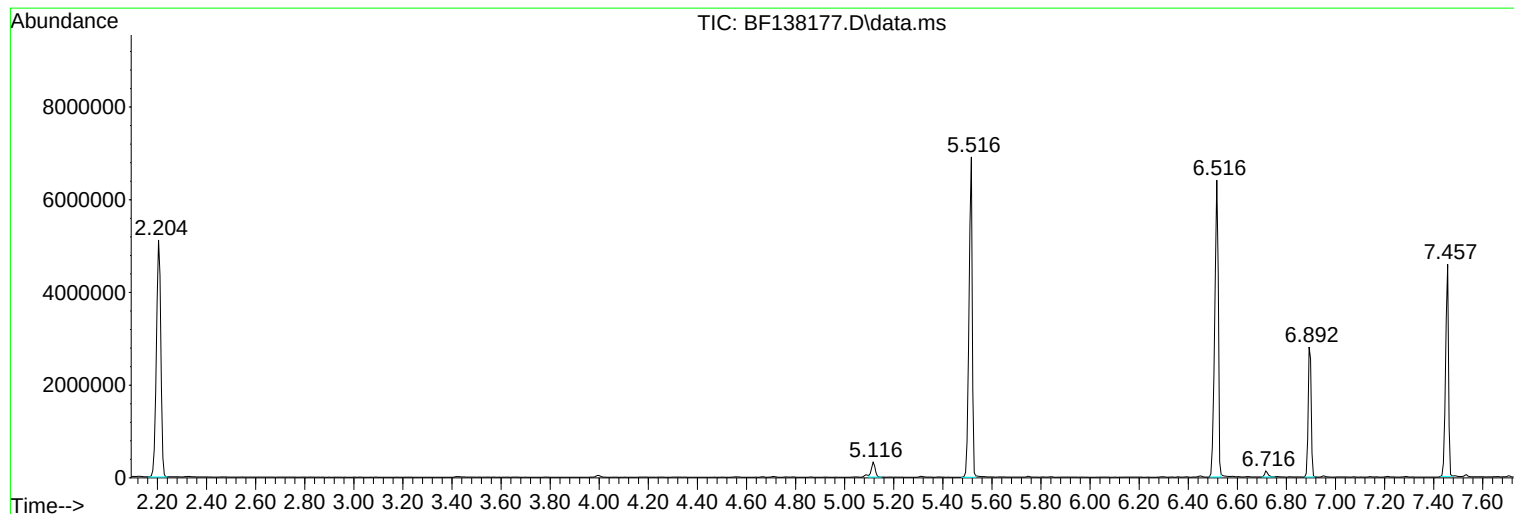

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138177.D
Acq On : 10 Jun 2024 17:38
Operator : CG\JU
Sample : P2795-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1-(0-5)-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138177.D
Acq On : 10 Jun 2024 17:38
Operator : CG\JU
Sample : P2795-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1-(0-5)-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------