


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138170.D
Acq On : 10 Jun 2024 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 06 05:19:29 2024

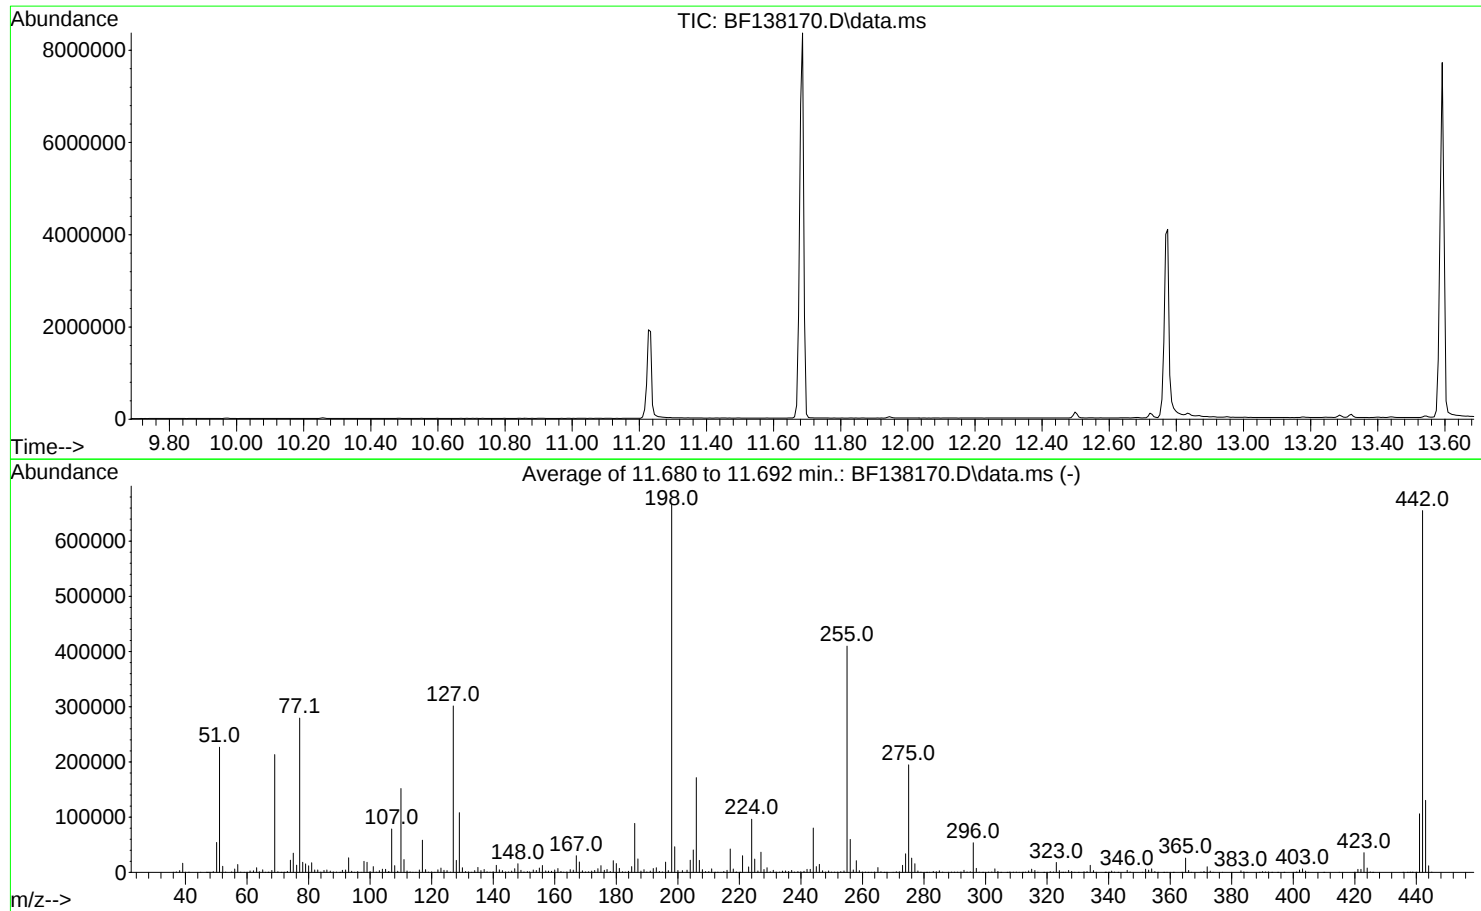

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	226647	PASS
68	69	0.00	2	1.6	3439	PASS
69	198	0.00	100	32.0	213341	PASS
70	69	0.00	2	0.5	1031	PASS
127	198	10	80	45.2	301392	PASS
197	198	0.00	2	0.5	3112	PASS
198	198	100	100	100.0	666389	PASS
199	198	5	9	6.9	46309	PASS
275	198	10	60	29.2	194736	PASS
365	198	1	100	3.9	25799	PASS
441	198	0.01	100	15.9	106221	PASS
442	442	50	100	100.0	655424	PASS
443	442	15	24	19.9	130499	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/10/2024	BNA_F	<u>BF138170.D</u>
Compound Name	Response	Retention Time
DDT	612315	13.592
DDD	10560	13.286
DDE	1616	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12176	624491	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138170.D
Acq On : 10 Jun 2024 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 15:29:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

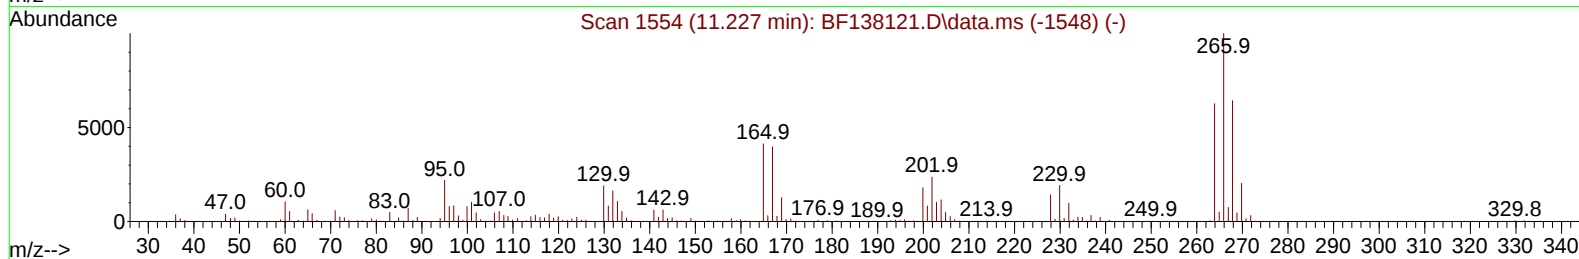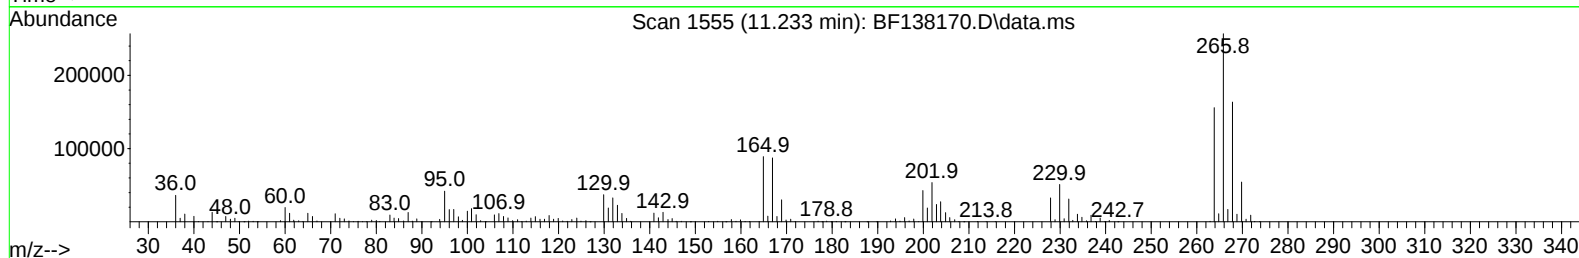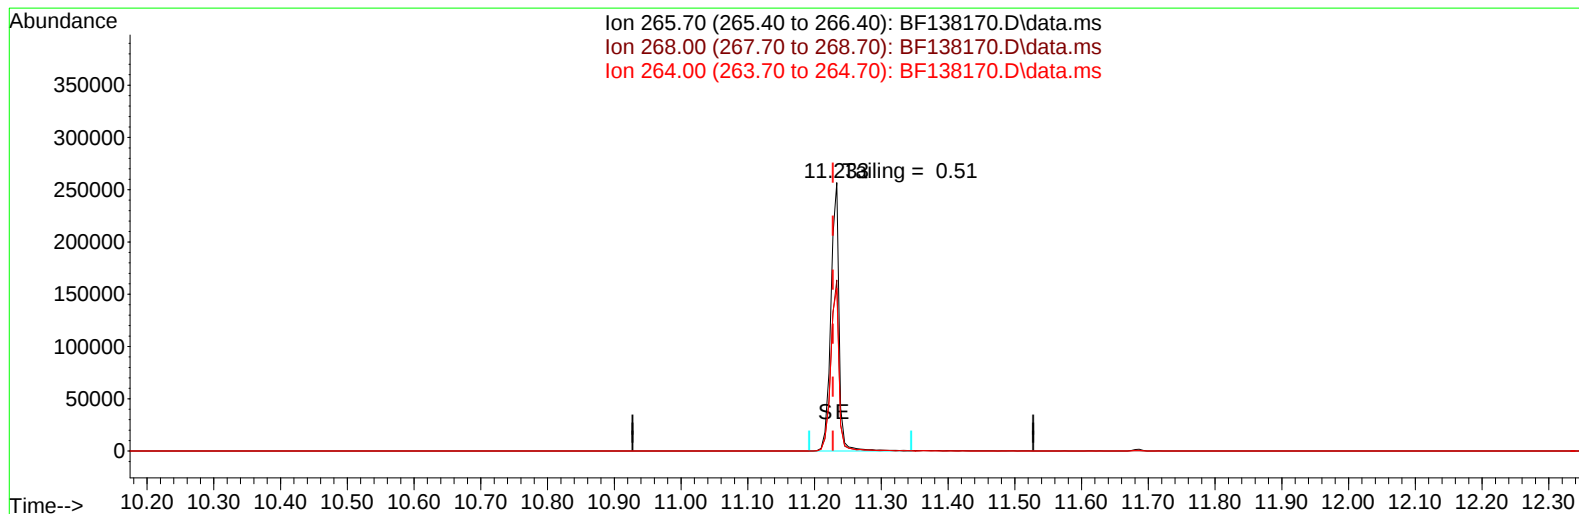

TIC: BF138170.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 165849.73 ng




response 222116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.71
264.00	62.60	60.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061024\
Data File : BF138170.D
Acq On : 10 Jun 2024 10:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 15:29:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

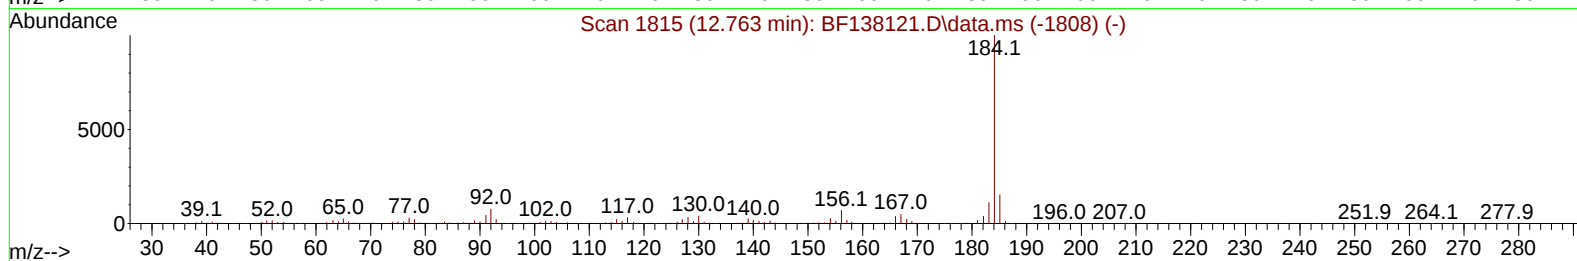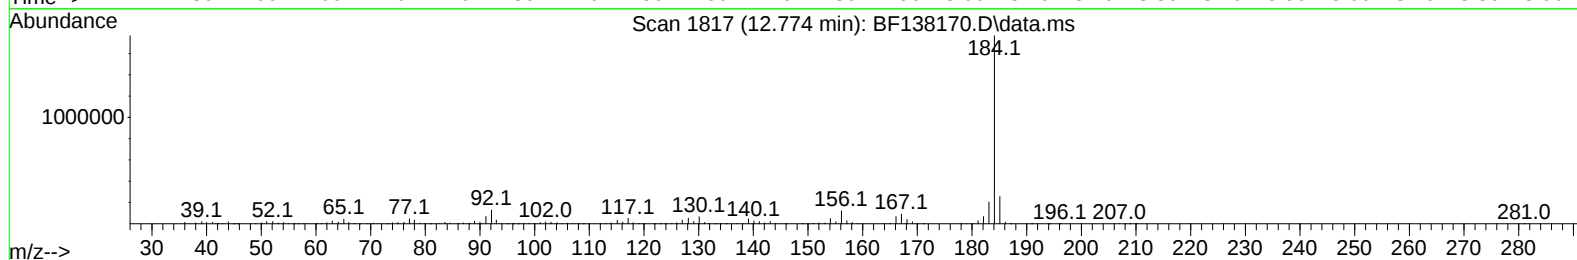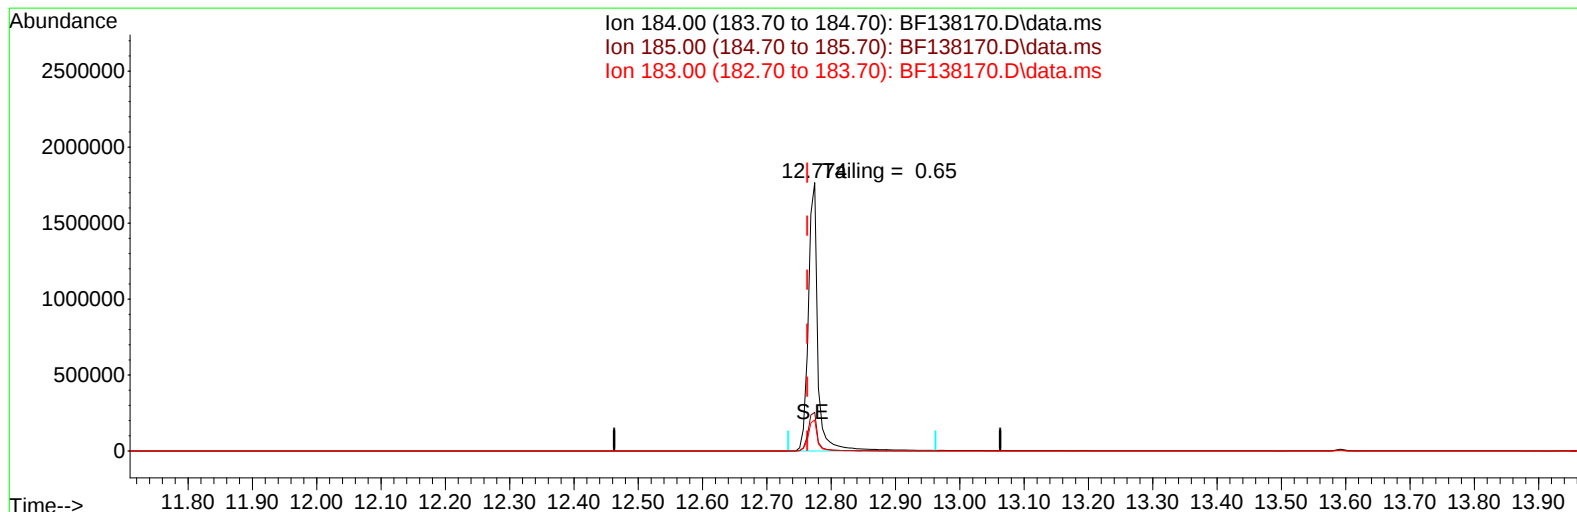

TIC: BF138170.D\data.ms

(77) Benzidine

12.774min (+ 0.012) 305345.30 ng

response 1825613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.45
183.00	11.20	11.60
0.00	0.00	0.00