
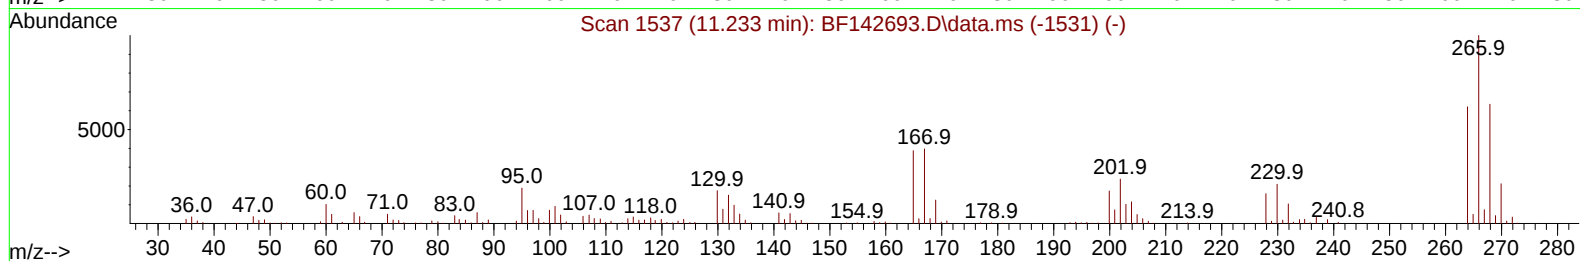
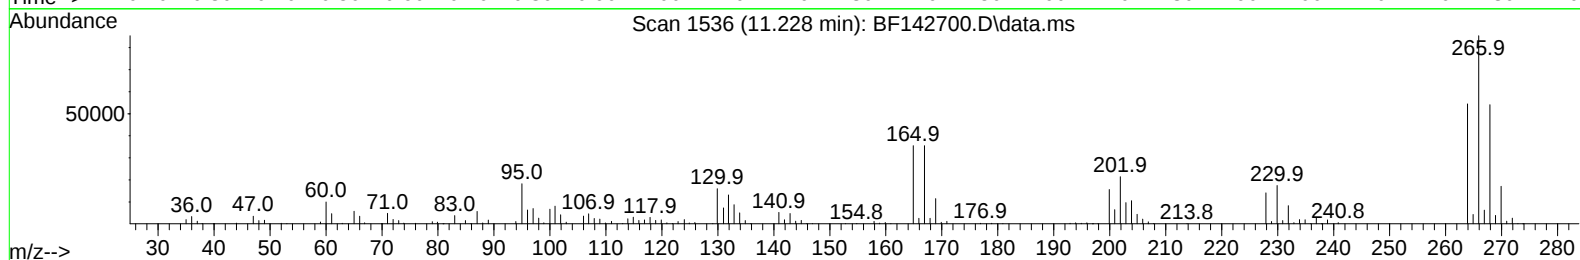


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142700.D
Acq On : 10 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:16:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

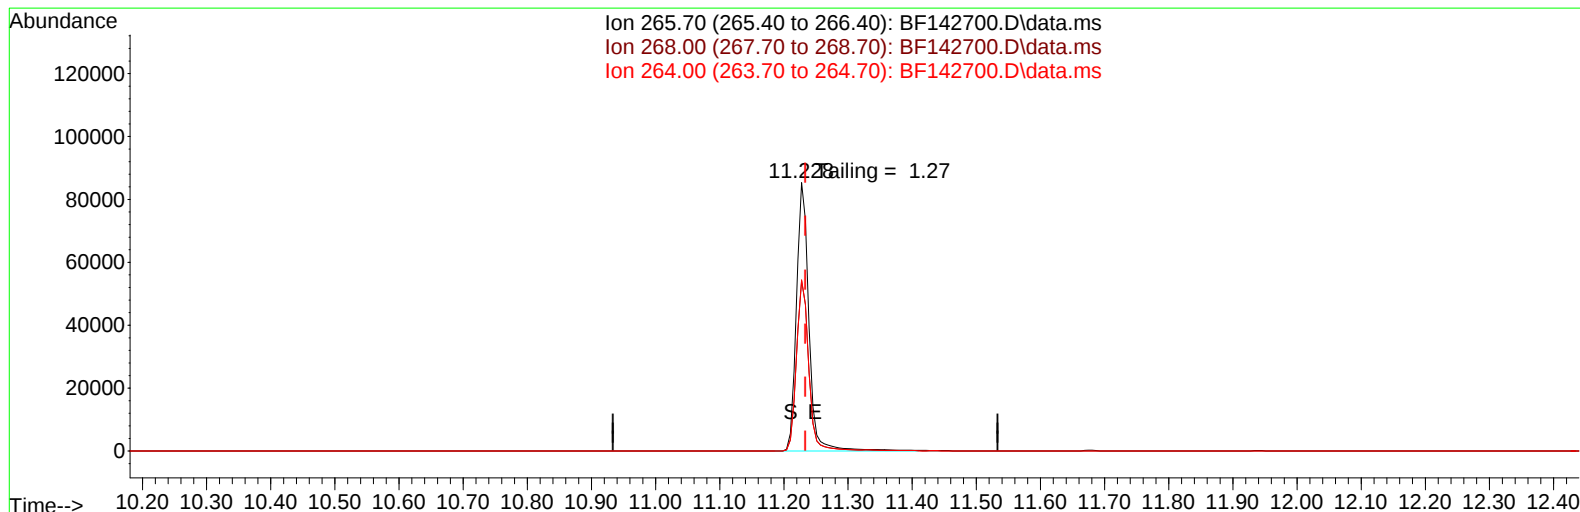

TIC: BF142700.D\data.ms

(70) Pentachlorophenol (C)




11.228min (-0.006) 58811.37 ng

response 116657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.43
264.00	62.10	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142700.D
Acq On : 10 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:16:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

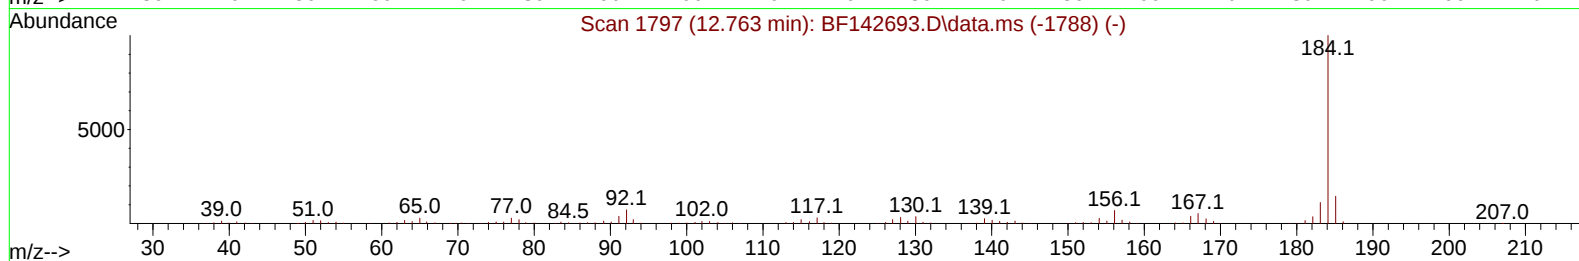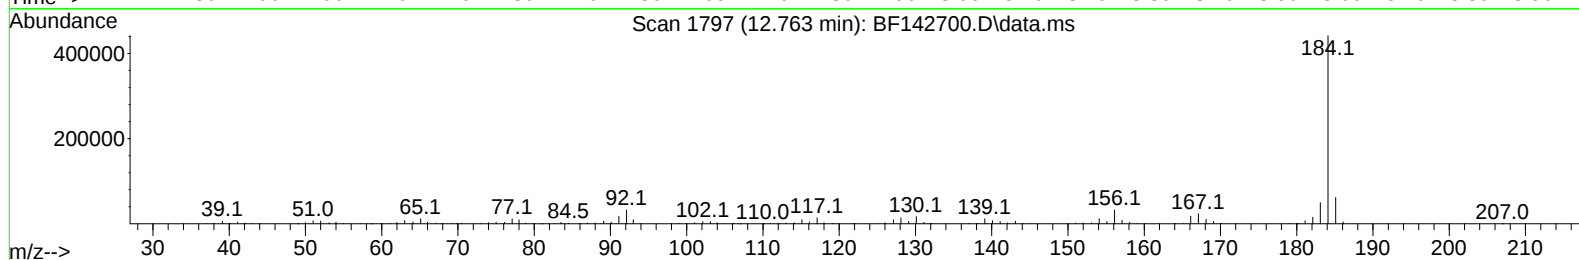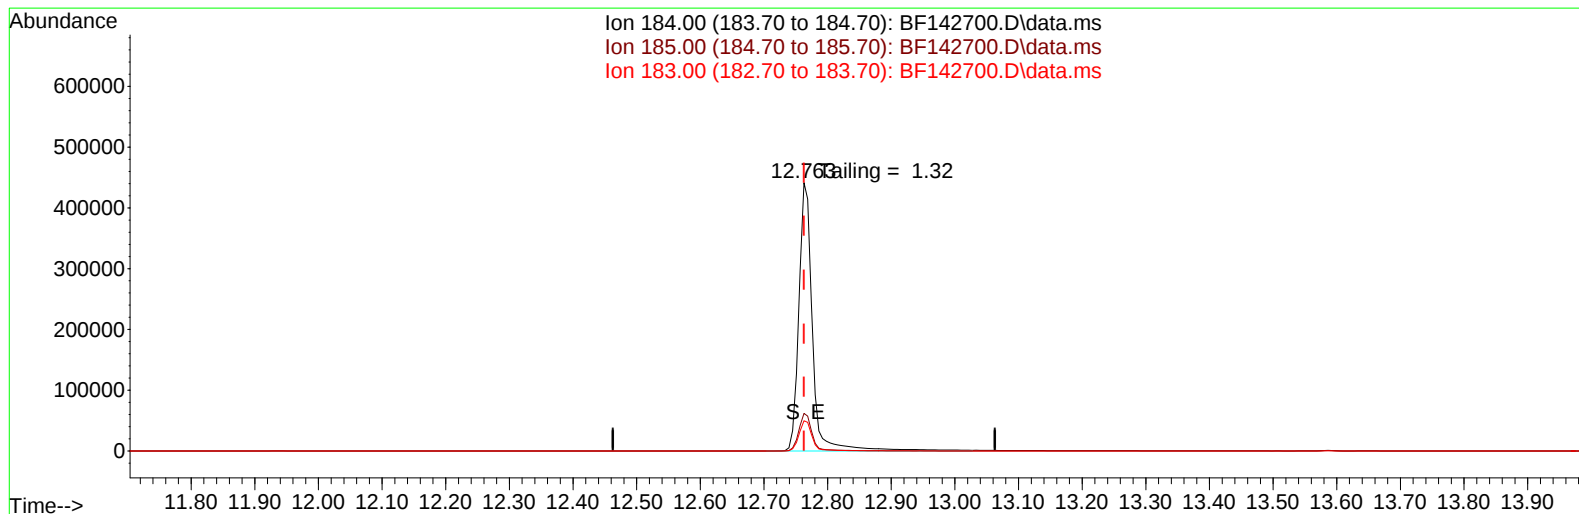

TIC: BF142700.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 44952.78 ng

response 659366

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.10	11.27
0.00	0.00	0.00