

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061025\  
Data File : BF142702.D  
Acq On : 10 Jun 2025 10:08  
Operator : RC/JU  
Sample : PB168351BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB168351BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142702.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.140       | 494           | 501         | 511          | rBV      | 146763         | 254148        | 7.58%           | 1.329%        |
| 2         | 5.528       | 560           | 567         | 572          | rBV      | 1641624        | 2384490       | 71.10%          | 12.473%       |
| 3         | 6.522       | 729           | 736         | 741          | rBV      | 1613249        | 2376229       | 70.85%          | 12.430%       |
| 4         | 6.892       | 794           | 799         | 804          | rBV      | 421756         | 516205        | 15.39%          | 2.700%        |
| 5         | 7.457       | 887           | 895         | 900          | rBV      | 1067623        | 1570140       | 46.82%          | 8.213%        |
| 6         | 8.175       | 1011          | 1017        | 1025         | rBV      | 496092         | 673403        | 20.08%          | 3.522%        |
| 7         | 9.251       | 1193          | 1200        | 1226         | rBV      | 2213927        | 3156836       | 94.12%          | 16.513%       |
| 8         | 9.933       | 1310          | 1316        | 1332         | rBV      | 623589         | 796221        | 23.74%          | 4.165%        |
| 9         | 10.728      | 1444          | 1451        | 1466         | rBV      | 1468270        | 1990326       | 59.34%          | 10.411%       |
| 10        | 11.422      | 1564          | 1569        | 1591         | rBV      | 631090         | 820019        | 24.45%          | 4.289%        |
| 11        | 13.010      | 1833          | 1839        | 1845         | rBV      | 2455000        | 3353895       | 100.00%         | 17.544%       |
| 12        | 14.068      | 2013          | 2019        | 2039         | rBV      | 507940         | 707912        | 21.11%          | 3.703%        |
| 13        | 15.562      | 2266          | 2273        | 2293         | rBV      | 314072         | 517721        | 15.44%          | 2.708%        |




Sum of corrected areas: 19117545

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061025\  
Data File : BF142702.D  
Acq On : 10 Jun 2025 10:08  
Operator : RC/JU  
Sample : PB168351BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB168351BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

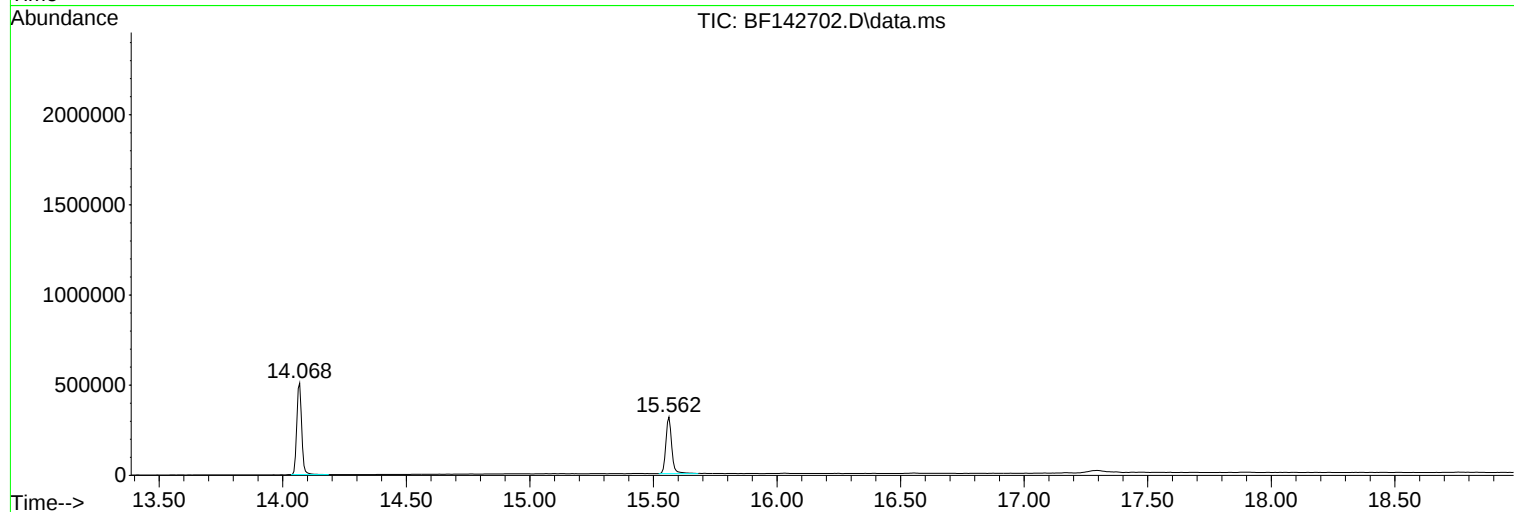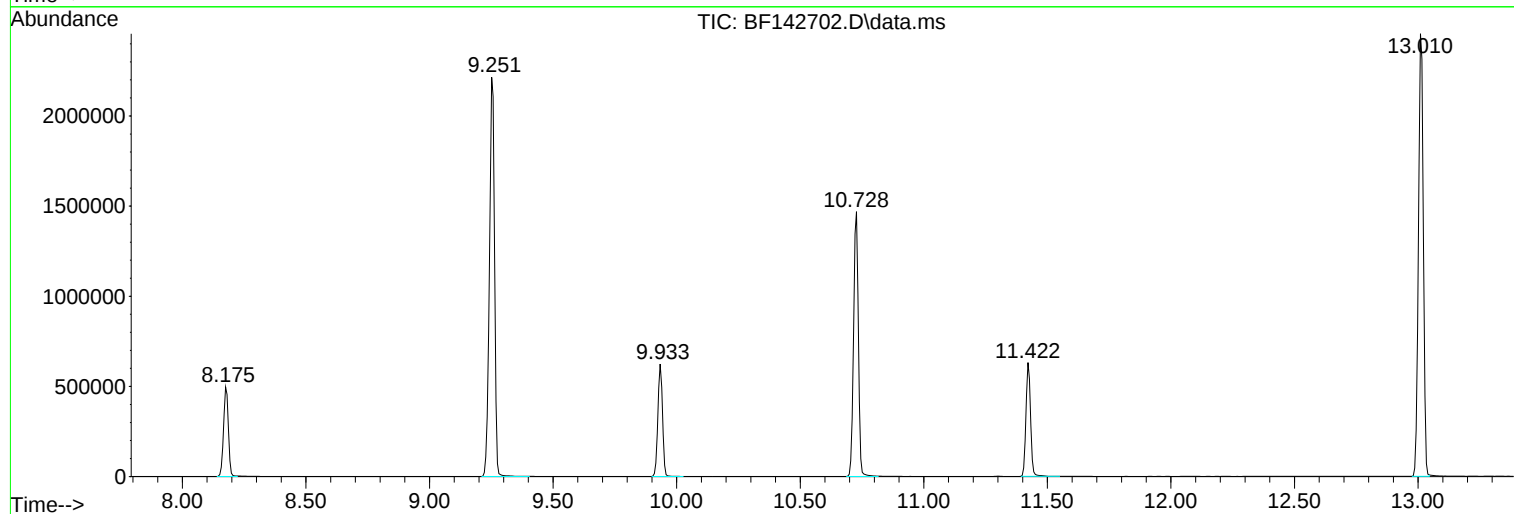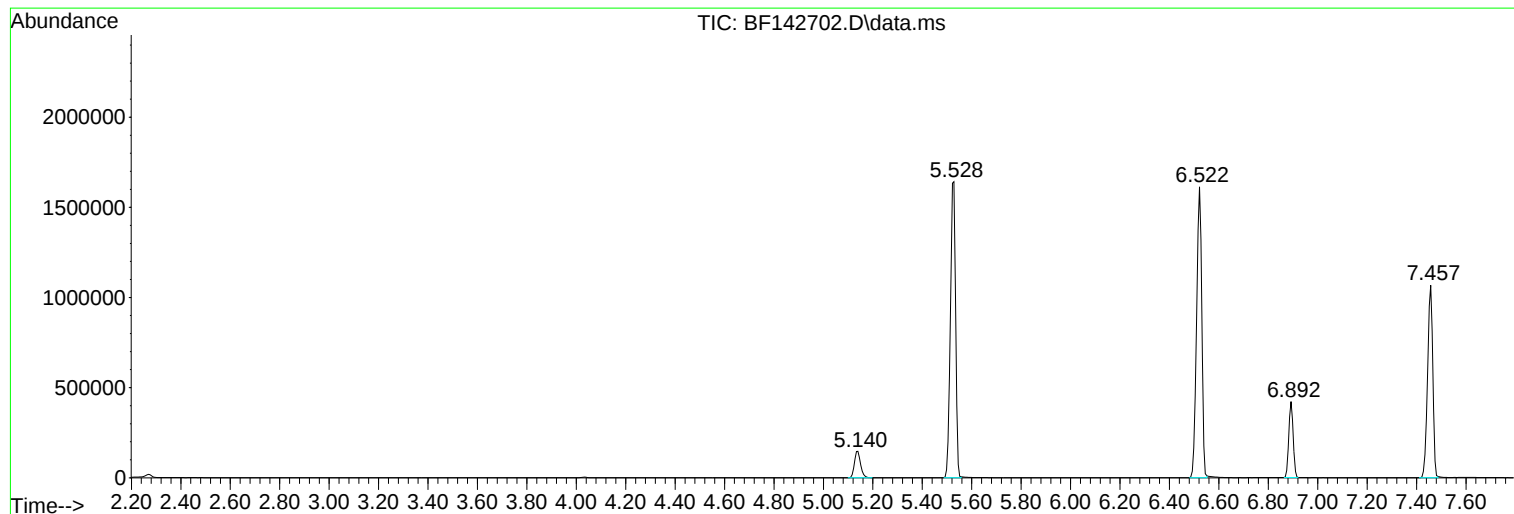

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061025\  
Data File : BF142702.D  
Acq On : 10 Jun 2025 10:08  
Operator : RC/JU  
Sample : PB168351BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB168351BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061025\  
Data File : BF142702.D  
Acq On : 10 Jun 2025 10:08  
Operator : RC/JU  
Sample : PB168351BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB168351BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|