

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
 Data File : BF142704.D
 Acq On : 10 Jun 2025 11:13
 Operator : RC/JU
 Sample : Q2259-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-36-060525

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	483	496	503	rBV	102963	152374	8.28%	1.253%
2	5.516	559	565	570	rBV	1028186	1357463	73.75%	11.165%
3	6.516	730	735	755	rVB	962062	1339232	72.76%	11.015%
4	6.892	794	799	804	rBV	321294	386916	21.02%	3.182%
5	7.451	888	894	905	rBV	657261	893221	48.53%	7.347%
6	8.175	1012	1017	1028	rBV	395603	505969	27.49%	4.162%
7	9.251	1194	1200	1205	rBV	1463753	1840676	100.00%	15.139%
8	9.933	1311	1316	1325	rVB	459155	570036	30.97%	4.688%
9	10.339	1380	1385	1392	rVB2	21574	33080	1.80%	0.272%
10	10.645	1429	1437	1442	rBV	189842	242089	13.15%	1.991%
11	10.722	1445	1450	1460	rBV	843239	1080769	58.72%	8.889%
12	10.957	1486	1490	1495	rVB	33023	42431	2.31%	0.349%
13	11.074	1502	1510	1516	rBV4	19106	31584	1.72%	0.260%
14	11.422	1564	1569	1575	rVB	428977	533960	29.01%	4.392%
15	11.798	1626	1633	1640	rVB7	13509	29869	1.62%	0.246%
16	11.939	1651	1657	1675	rBV2	205443	368439	20.02%	3.030%
17	12.439	1735	1742	1750	rBV3	11216	28583	1.55%	0.235%
18	12.727	1786	1791	1803	rBV	50296	87137	4.73%	0.717%
19	13.010	1833	1839	1844	rBV	1175580	1541071	83.72%	12.675%
20	13.210	1866	1873	1874	rBV3	12140	19337	1.05%	0.159%
21	13.574	1931	1935	1945	rVB3	14899	23261	1.26%	0.191%
22	13.904	1985	1991	2007	rBV	63667	119379	6.49%	0.982%
23	14.063	2009	2018	2027	rBV	278301	388197	21.09%	3.193%
24	14.221	2041	2045	2051	rBV	15402	21944	1.19%	0.180%
25	14.333	2059	2064	2069	rBV	13445	20575	1.12%	0.169%
26	14.527	2093	2097	2102	rBV	18329	27282	1.48%	0.224%
27	15.557	2266	2272	2284	rBV	265030	449836	24.44%	3.700%
28	15.857	2320	2323	2337	rVB2	10420	23510	1.28%	0.193%




Sum of corrected areas: 12158220

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142704.D
Acq On : 10 Jun 2025 11:13
Operator : RC/JU
Sample : Q2259-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-36-060525

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

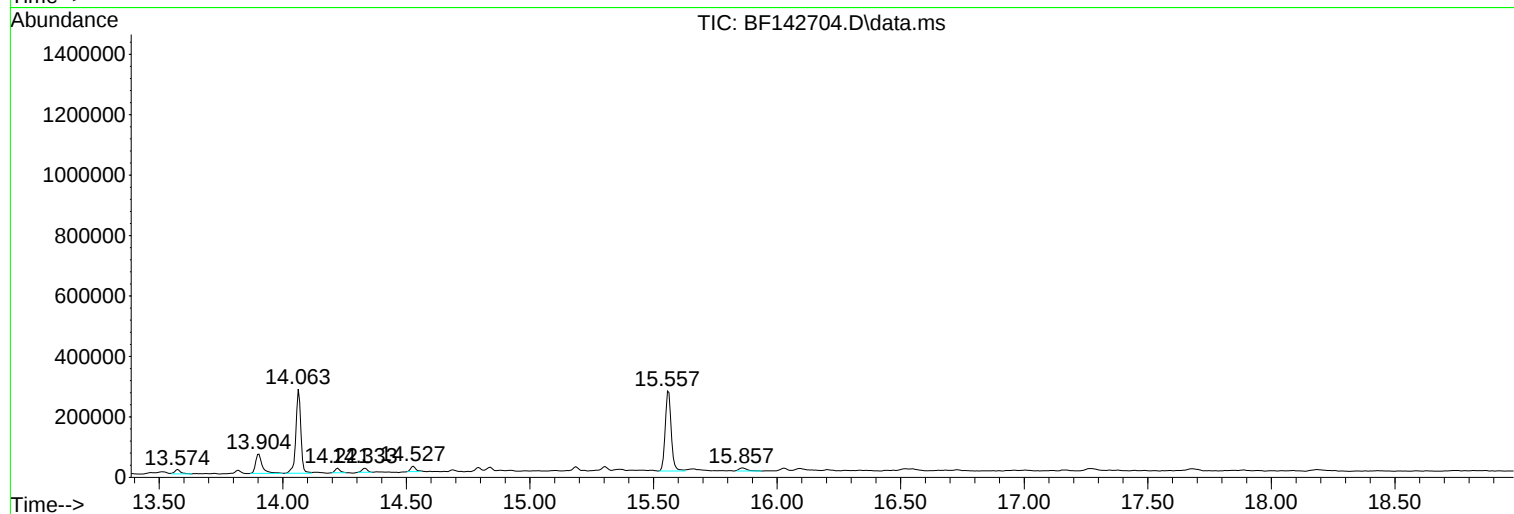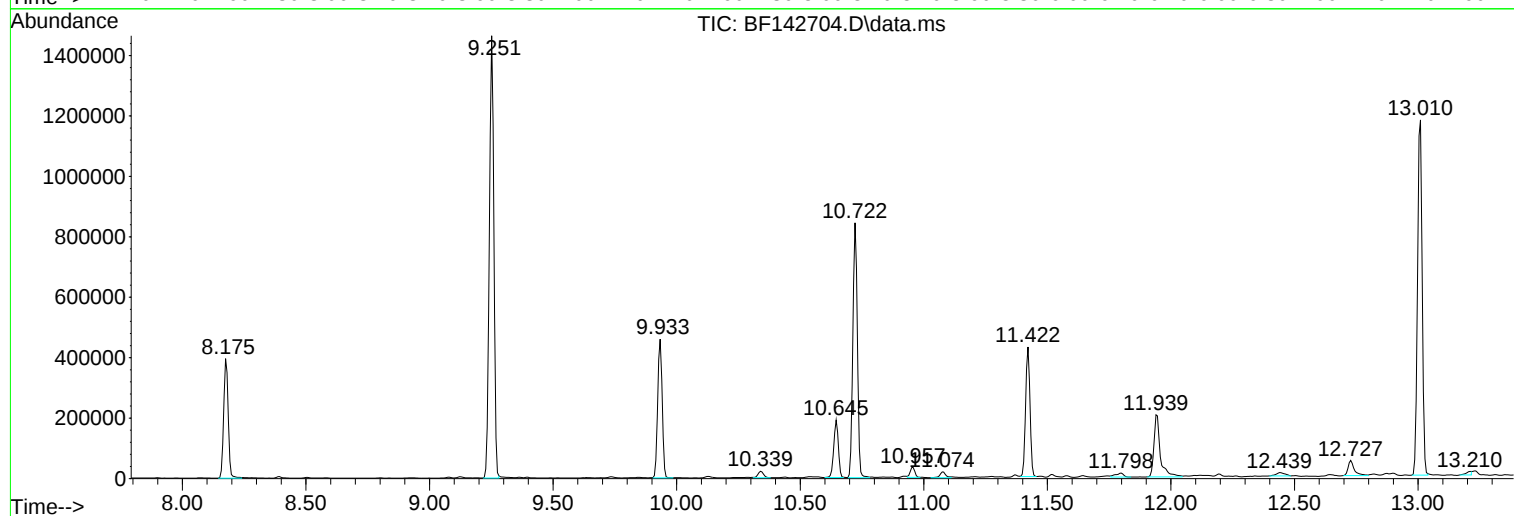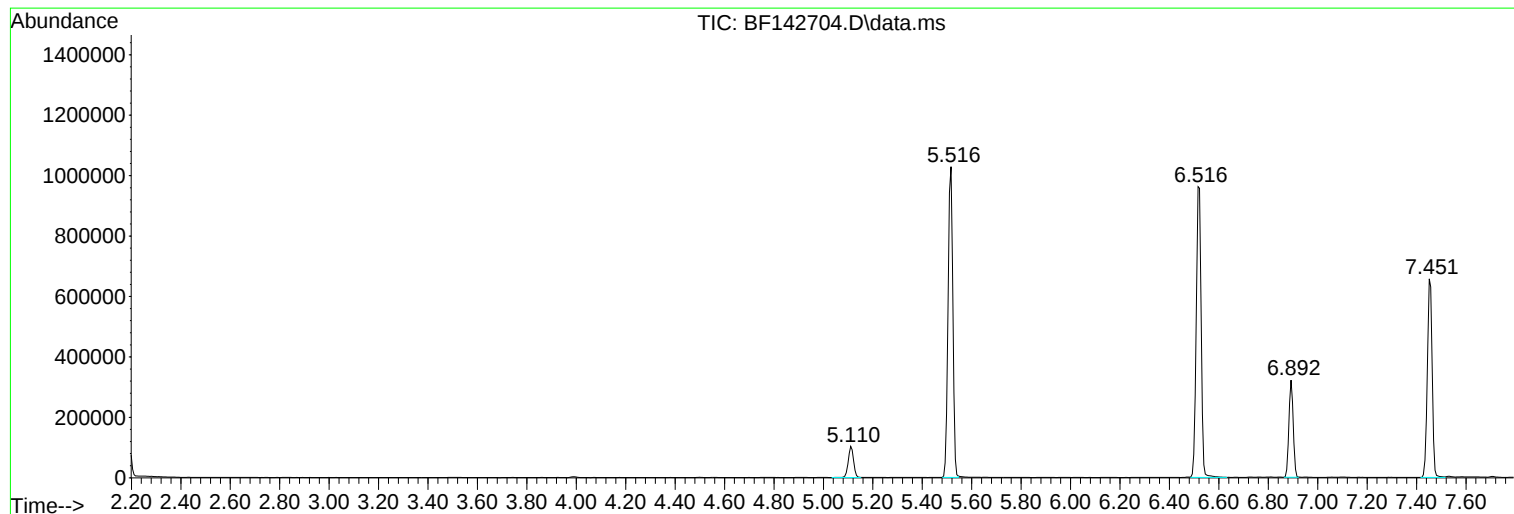

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142704.D
Acq On : 10 Jun 2025 11:13
Operator : RC/JU
Sample : Q2259-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-36-060525

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142704.D
Acq On : 10 Jun 2025 11:13
Operator : RC/JU
Sample : Q2259-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-36-060525

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------