

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
 Data File : BF079891.D
 Acq On : 11 Jun 2015 13:09
 Operator : TP/IZ
 Sample : SSTDICC025
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Quant Time: Jun 12 01:02:14 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 12 00:59:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	48484	20.00	ng	0.00
21) Naphthalene-d8	8.68	136	191335	20.00	ng	0.00
38) Acenaphthene-d10	10.46	164	93413	20.00	ng	0.00
63) Phenanthrene-d10	11.99	188	196130	20.00	ng	0.01
75) Chrysene-d12	0.00	240	0	0.00	ng	-14.99
86) Perylene-d12	0.00	264	0	0.00	ng	-16.93

System Monitoring Compounds

5) 2-Fluorophenol	6.00	112	131910	45.59	ng	0.00
7) Phenol-d6	6.99	99	178496	47.15	ng	0.00
23) Nitrobenzene-d5	7.95	82	142497	44.30	ng	0.00
41) 2,4,6-Tribromophenol	11.26	330	42302	50.74	ng	0.00
44) 2-Fluorobiphenyl	9.76	172	354632	53.50	ng	0.00
78) Terphenyl-d14	13.78	244	471262	0.00	ng	0.09

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.34	88	30013	22.68	ng	94
3) Pyridine	4.14	79	68967	19.93	ng	99
4) n-Nitrosodimethylamine	4.03	42	39119	22.65	ng	94
6) Aniline	7.05	93	127277	23.34	ng	100
8) 2-Chlorophenol	7.18	128	79978	24.01	ng	99
9) Benzaldehyde	6.94	77	56141	25.81	ng	98
10) Phenol	7.00	94	99791	24.57	ng	99
11) bis(2-Chloroethyl)ether	7.11	93	81961	25.46	ng	99
12) 1,3-Dichlorobenzene	7.34	146	93547	24.57	ng	100
13) 1,4-Dichlorobenzene	7.42	146	94035	22.09	ng	100
14) 1,2-Dichlorobenzene	7.56	146	87123	23.59	ng	99
15) Benzyl Alcohol	7.52	79	67967	22.46	ng	100
16) 2,2'-oxybis(1-Chloropropan	7.66	45	116411	23.70	ng	99
17) 2-Methylphenol	7.62	107	70343	24.75	ng	97
18) Hexachloroethane	7.92	117	30454	22.92	ng	97
19) n-Nitroso-di-n-propylamine	7.78	70	65344	24.38	ng	99
20) 3+4-Methylphenols	7.77	107	88286	23.93	ng	98
22) Acetophenone	7.79	105	115295	24.41	ng	99
24) Nitrobenzene	7.96	77	78658	23.83	ng	99
25) Isophorone	8.20	82	170835	24.63	ng	99
26) 2-Nitrophenol	8.30	139	23771	18.81	ng	98
27) 2,4-Dimethylphenol	8.31	122	75473	24.31	ng	98
28) bis(2-Chloroethoxy)methane	8.41	93	98404	23.69	ng	99
29) 2,4-Dichlorophenol	8.52	162	62012	23.61	ng	99
30) 1,2,4-Trichlorobenzene	8.63	180	79500	23.58	ng	97
31) Naphthalene	8.71	128	264646	25.86	ng	99
32) Benzoic acid	8.35	122	15903	16.93	ng	97
33) 4-Chloroaniline	8.74	127	139848	33.93	ng	98
34) Hexachlorobutadiene	8.83	225	46484	25.17	ng	95
35) Caprolactam	9.07	113	18284	22.98	ng	# 65
36) 4-Chloro-3-methylphenol	9.21	107	73693	25.53	ng	100
37) 2-Methylnaphthalene	9.40	142	178451	24.65	ng	99
39) 1,2,4,5-Tetrachlorobenzene	9.58	216	80511	24.95	ng	99
40) Hexachlorocyclopentadiene	9.56	237	24646	16.58	ng	99

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
 Data File : BF079891.D
 Acq On : 11 Jun 2015 13:09
 Operator : TP/IZ
 Sample : SSTDICC025
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025


Quant Time: Jun 12 01:02:14 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 12 00:59:58 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	9.68	196	48231	24.47	ng	99
43) 2,4,5-Trichlorophenol	9.71	196	54930	26.59	ng	97
45) 1,1'-Biphenyl	9.87	154	196869	25.58	ng	92
46) 2-Chloronaphthalene	9.90	162	167225	26.35	ng	98
47) 2-Nitroaniline	9.98	65	27696	20.07	ng	97
48) Acenaphthylene	10.32	152	278200	25.68	ng	99
49) Dimethylphthalate	10.15	163	186041	25.27	ng	99
50) 2,6-Dinitrotoluene	10.22	165	30052	23.40	ng	98
51) Acenaphthene	10.49	154	157063	25.03	ng	98
52) 3-Nitroaniline	10.39	138	37911	24.08	ng	95
53) 2,4-Dinitrophenol	10.49	184	2544	9.23	ng	# 1
54) Dibenzofuran	10.66	168	226400	25.57	ng	99
55) 4-Nitrophenol	10.52	139	25718	22.68	ng	95
56) 2,4-Dinitrotoluene	10.63	165	32774	20.10	ng	98
57) Fluorene	11.02	166	204581	26.01	ng	100
58) 2,3,4,6-Tetrachlorophenol	10.78	232	39018	25.39	ng	97
59) Diethylphthalate	10.86	149	195870	27.06	ng	99
60) 4-Chlorophenyl-phenylether	10.99	204	87855	25.74	ng	96
61) 4-Nitroaniline	11.00	138	38566	24.71	ng	97
62) Azobenzene	11.15	77	174110	24.57	ng	97
64) 4,6-Dinitro-2-methylphenol	11.04	198	6682	12.64	ng	92
65) n-Nitrosodiphenylamine	11.11	169	159797	24.36	ng	99
66) 4-Bromophenyl-phenylether	11.51	248	52227	22.77	ng	# 88
67) Hexachlorobenzene	11.59	284	60900	25.50	ng	# 90
68) Atrazine	11.64	200	45351	24.04	ng	98
69) Pentachlorophenol	11.78	266	19764	22.24	ng	91
70) Phenanthrene	12.01	178	295245	24.94	ng	99
71) Anthracene	12.07	178	290879	25.43	ng	98
72) Carbazole	12.23	167	280893	26.01	ng	100
73) Di-n-butylphthalate	12.57	149	303600	27.13	ng	99
74) Fluoranthene	13.35	202	321367	25.82	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_F
ClientSampleId :
SSTDICC025

Quant Time: Jun 12 01:02:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 00:59:58 2015
Response via : Initial Calibration

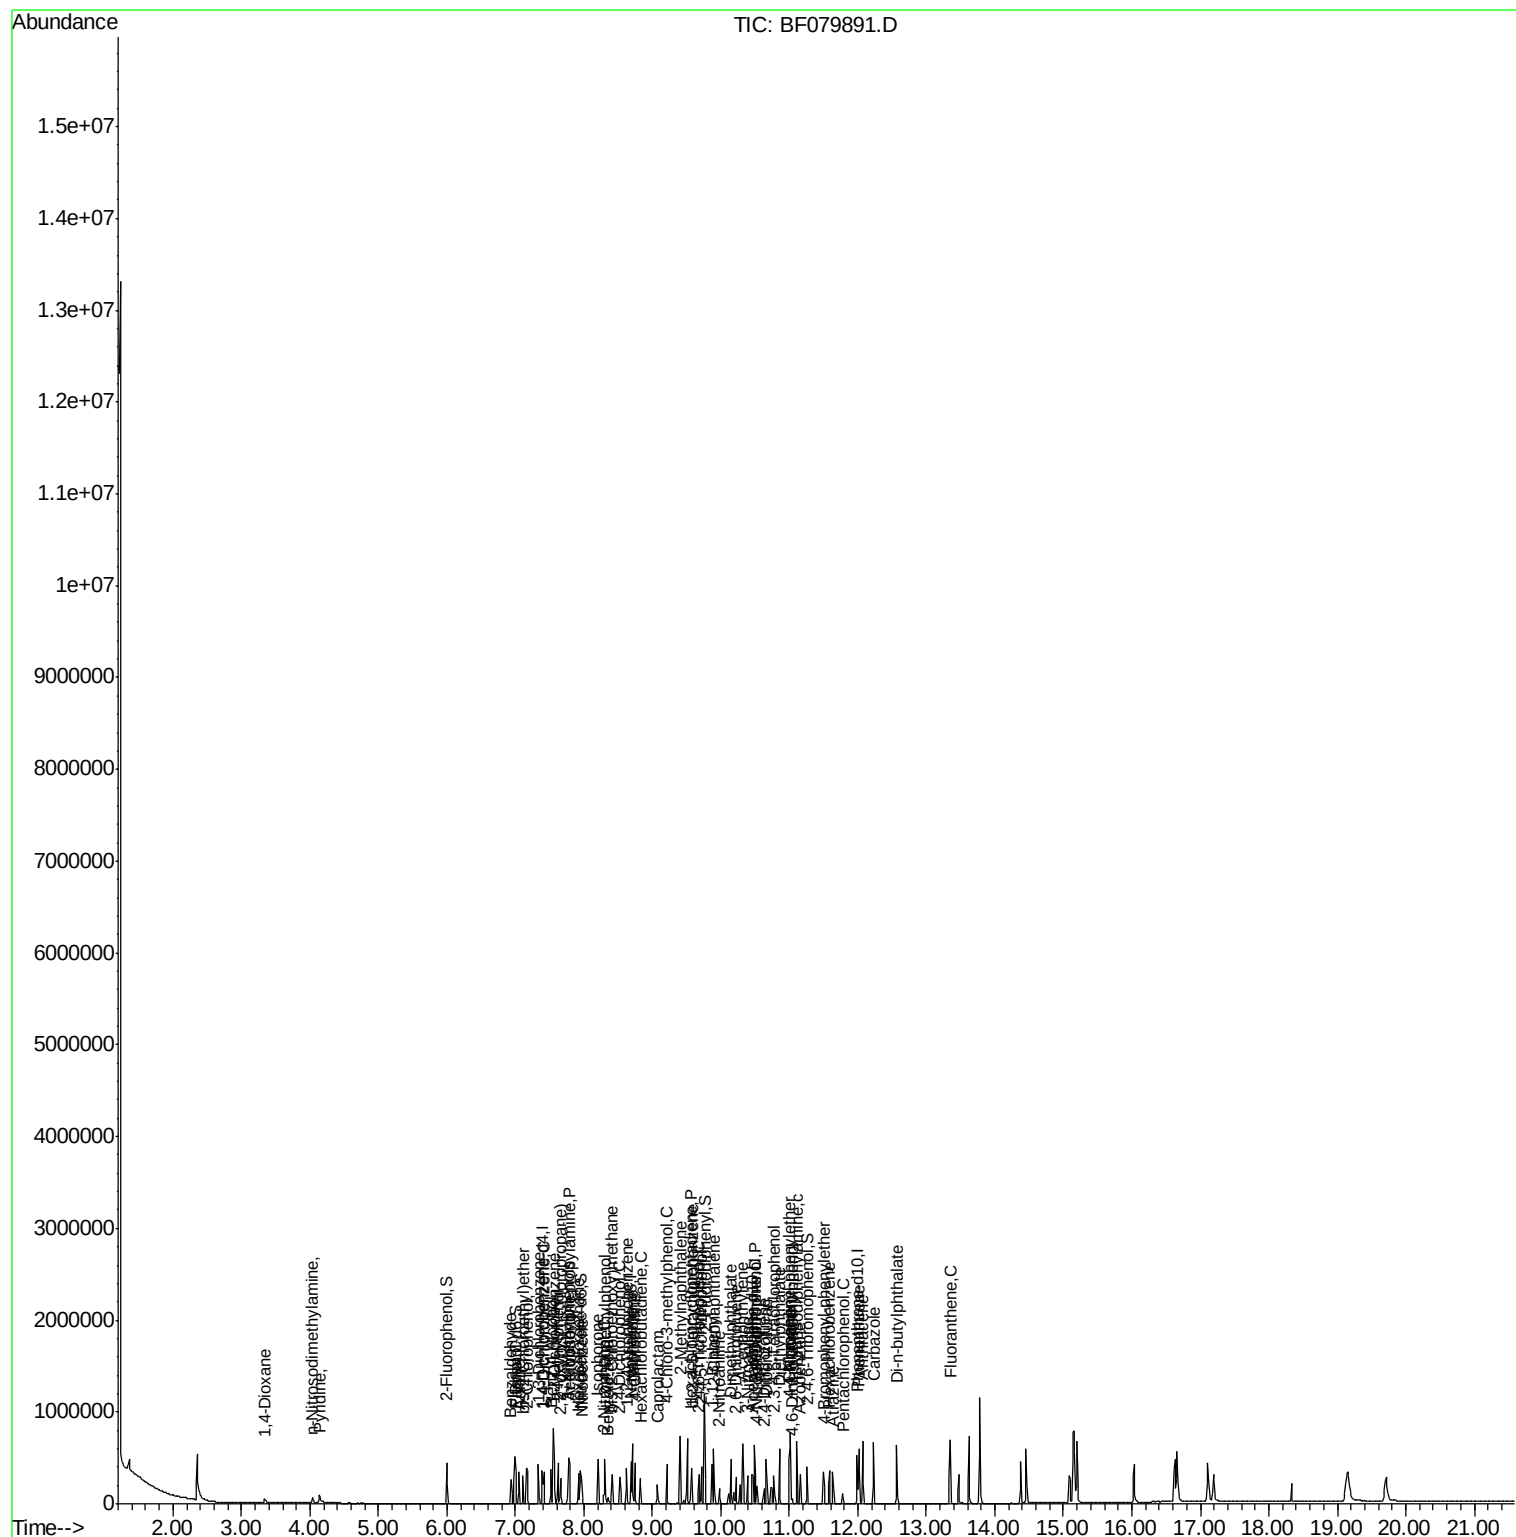

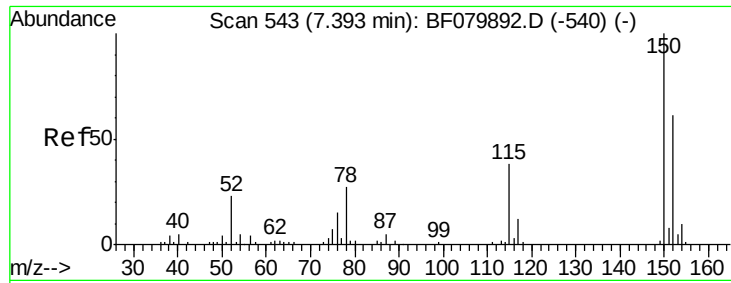

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.39 min Scan# 543

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025


Tgt Ion:152 Resp: 48484

Ion Ratio Lower Upper

152 100

150 162.1 131.0 196.4




115 60.2 49.8 74.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

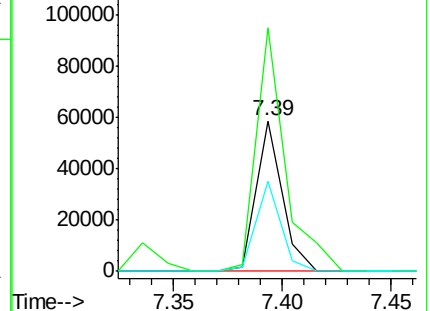

#2

1,4-Dioxane

Concen: 22.68 ng

RT: 3.34 min Scan# 188

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion: 88 Resp: 30013

Ion Ratio Lower Upper

88 100

58 71.9 63.0 94.4



43 28.3 23.2 34.8




Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

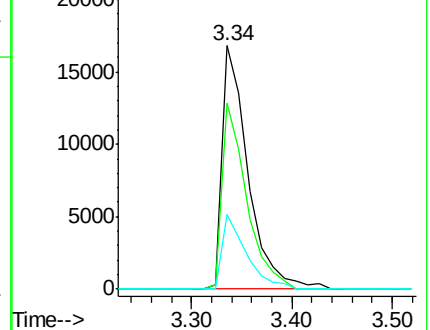



#3

Pyridine

Concen: 19.93 ng

RT: 4.14 min Scan# 258

Delta R.T. 0.01 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion: 79 Resp: 68967

Ion Ratio Lower Upper

79 100

52 71.0 56.7 85.1

51 35.3 29.8 44.6

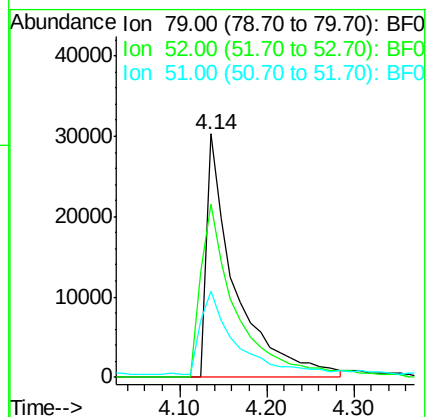

#4

n-Nitrosodimethylamine

Concen: 22.65 ng

RT: 4.03 min Scan# 249

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09




Tgt Ion: 42 Resp: 39119


Ion Ratio Lower Upper

42 100

74 129.4 109.0 163.6

44 8.3 7.7 11.5

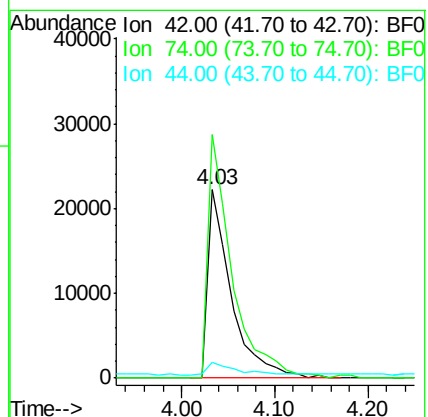



#5

2-Fluorophenol

Concen: 45.59 ng

RT: 6.00 min Scan# 421

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025


Tgt Ion: 112 Resp: 131910

Ion Ratio Lower Upper




112 100

64 70.2 54.5 81.7

63 35.2 27.9 41.9



Abundance Ion 112.00 (111.70 to 112.70): BF079891.D (-404) (-)

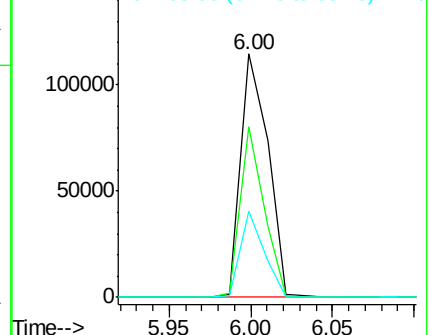

#6

Aniline

Concen: 23.34 ng

RT: 7.05 min Scan# 513

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion: 93 Resp: 127277

Ion Ratio Lower Upper



93 100


66 36.6 29.4 44.0

65 18.7 14.9 22.3



Abundance Ion 93.00 (92.70 to 93.70): BF079891.D (-496) (-)

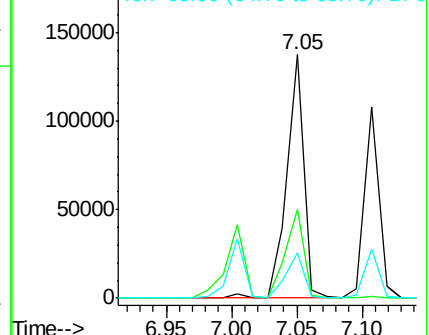

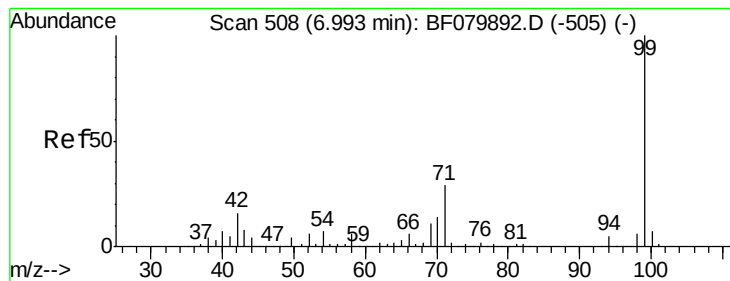

#7

Phenol-d6

Concen: 47.15 ng

RT: 6.99 min Scan# 508

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion: 99 Resp: 178496

Ion Ratio Lower Upper

99 100

42 15.0 12.9 19.3

71 28.3 23.4 35.2

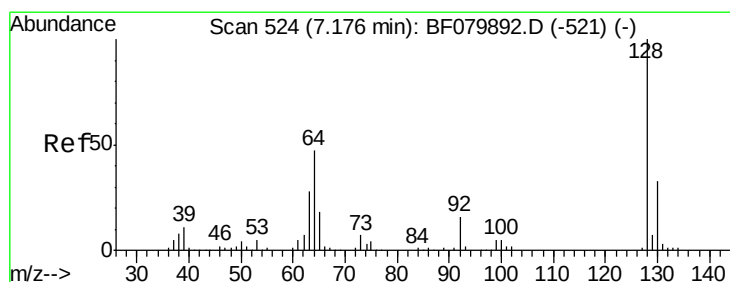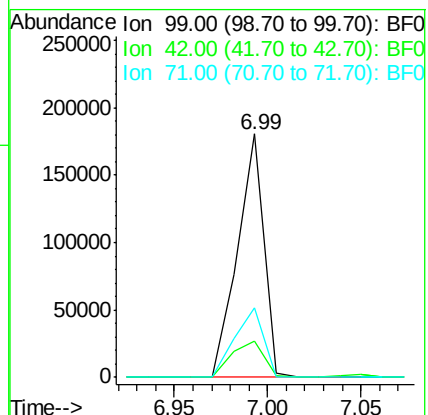

#8

2-Chlorophenol

Concen: 24.01 ng

RT: 7.18 min Scan# 524

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09




Tgt Ion: 128 Resp: 79978


Ion Ratio Lower Upper

128 100

130 31.8 13.1 53.1

64 47.1 26.8 66.8

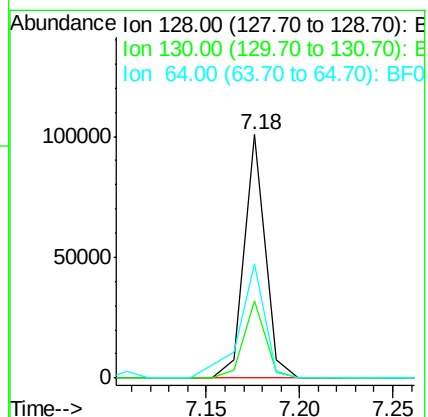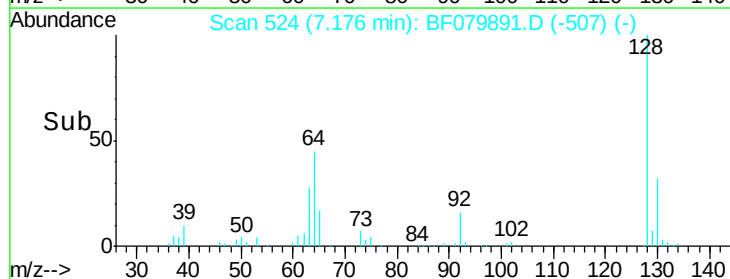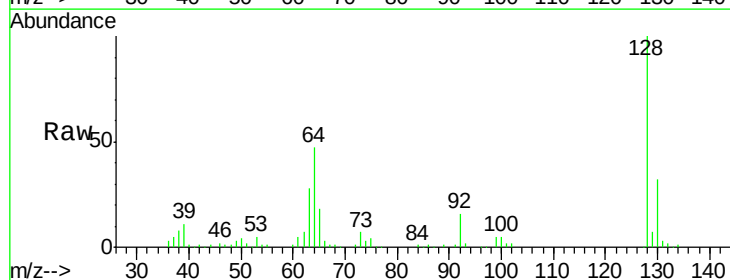

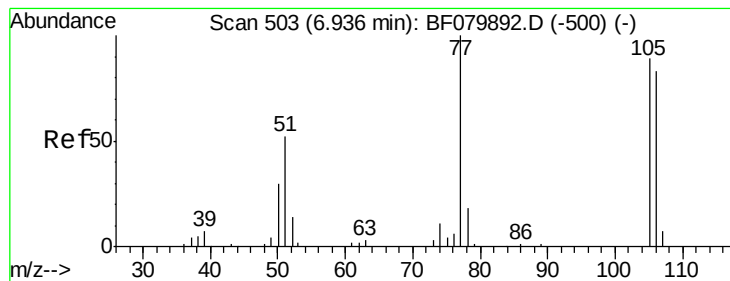

#9

Benzaldehyde

Concen: 25.81 ng

RT: 6.94 min Scan# 503

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDICC025


Tgt Ion: 77 Resp: 56141

Ion Ratio Lower Upper




77 100

105 86.4 68.6 108.6

106 82.2 63.3 103.3



Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 105.00 (104.70 to 105.70): BF0
Ion 106.00 (105.70 to 106.70): BF0

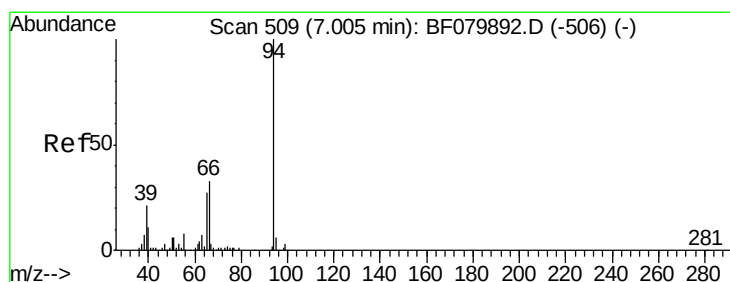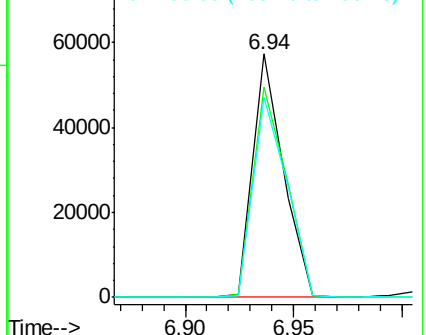

#10

Phenol

Concen: 24.57 ng

RT: 7.00 min Scan# 509

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion: 94 Resp: 99791

Ion Ratio Lower Upper



94 100


65 26.7 7.0 47.0

66 32.6 13.3 53.3

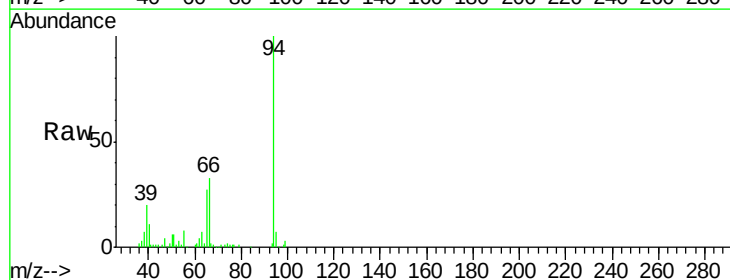

Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0

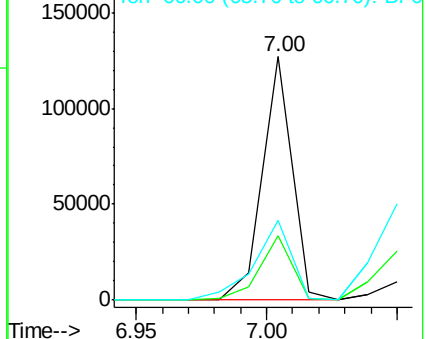

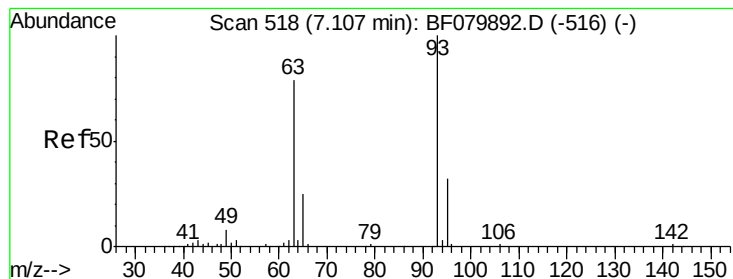

#11

bis(2-Chloroethyl)ether

Concen: 25.46 ng

RT: 7.11 min Scan# 518

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion: 93 Resp: 81961

Ion Ratio Lower Upper

93 100

63 78.4 58.7 98.7

95 32.9 11.5 51.5

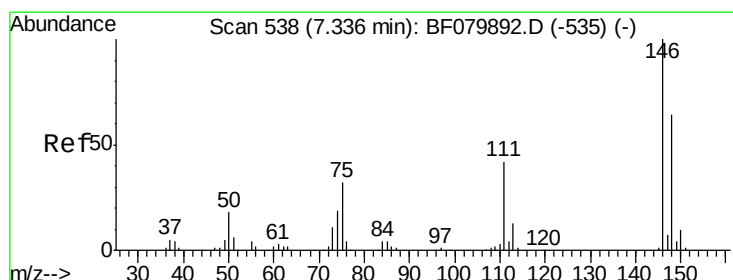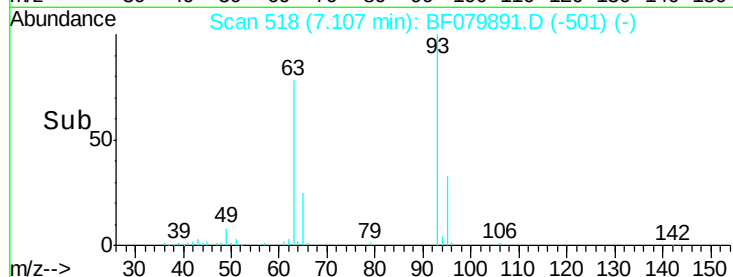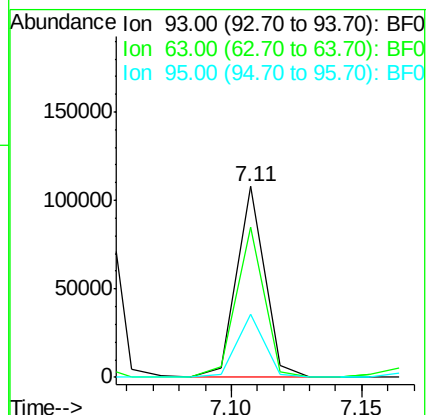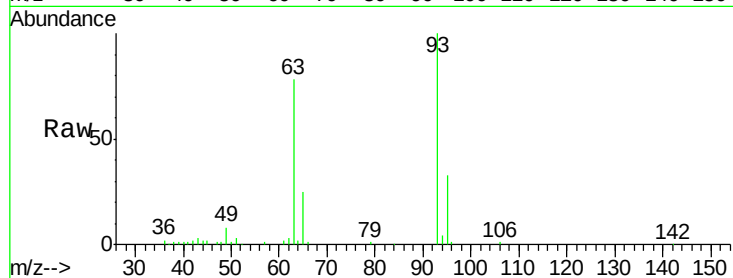

#12

1,3-Dichlorobenzene

Concen: 24.57 ng

RT: 7.34 min Scan# 538

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09




Tgt Ion: 146 Resp: 93547


Ion Ratio Lower Upper

146 100

148 63.6 50.9 76.3

75 31.8 25.8 38.6

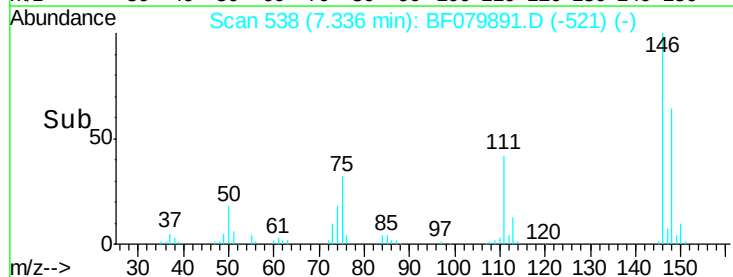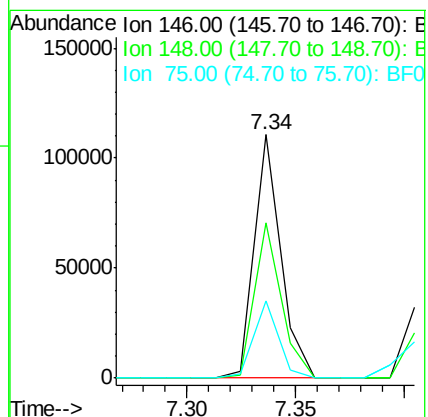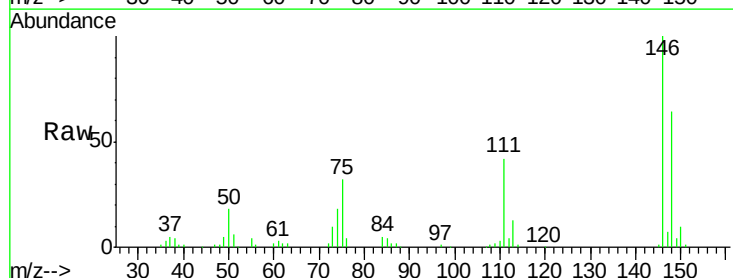







#13
 1,4-Dichlorobenzene
 Concen: 22.09 ng
 RT: 7.42 min Scan# 545
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion:146 Resp: 94035
 Ion Ratio Lower Upper
 146 100
 148 66.5 53.0 79.6
 111 35.0 28.2 42.2




Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E


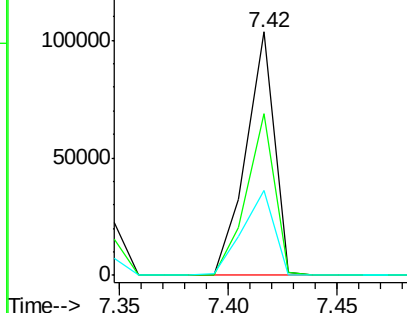



#14
 1,2-Dichlorobenzene
 Concen: 23.59 ng
 RT: 7.56 min Scan# 558
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:146 Resp: 87123
 Ion Ratio Lower Upper
 146 100
 148 62.9 51.2 76.8
 111 47.1 37.3 55.9



Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E

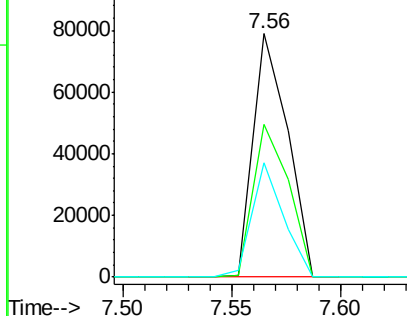



#15

Benzyl Alcohol

Concen: 22.46 ng

RT: 7.52 min Scan# 554

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDICC025


Tgt Ion: 79 Resp: 67967

Ion Ratio Lower Upper

79 100

108 82.7 66.4 99.6




77 62.0 49.4 74.0

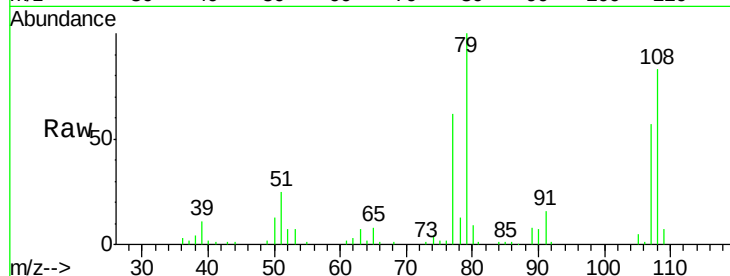

Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

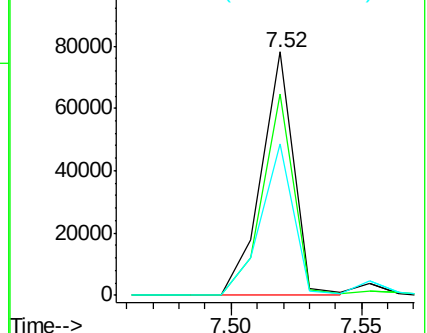

#16

2,2'-oxybis(1-Chloropropane)

Concen: 23.70 ng

RT: 7.66 min Scan# 566

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion: 45 Resp: 116411

Ion Ratio Lower Upper

45 100

77 12.3 0.0 31.9



79 9.4 0.0 29.6




Abundance Ion 45.00 (44.70 to 45.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

Ion 79.00 (78.70 to 79.70): BF0

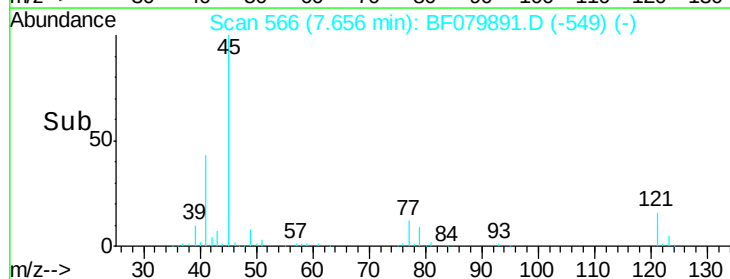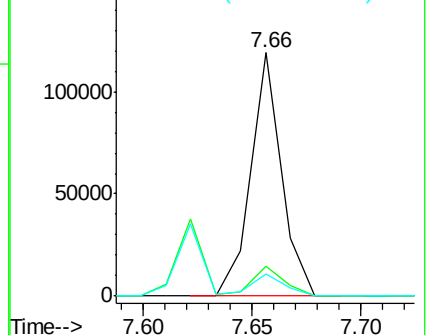

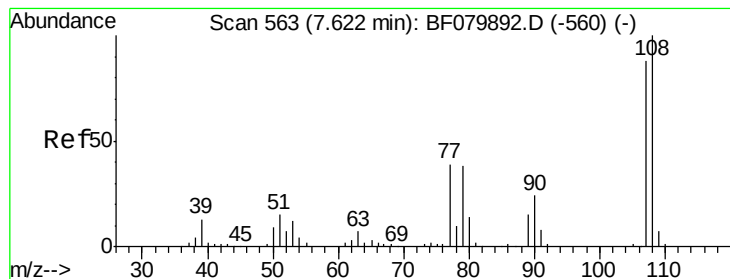

#17

2-Methylphenol

Concen: 24.75 ng

RT: 7.62 min Scan# 563

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025

Tgt Ion:107 Resp: 70343


Ion Ratio Lower Upper

107 100

108 110.9 90.8 136.2

77 42.6 35.4 53.2

79 39.7 34.7 52.1






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF0

Ion 79.00 (78.70 to 79.70): BF0

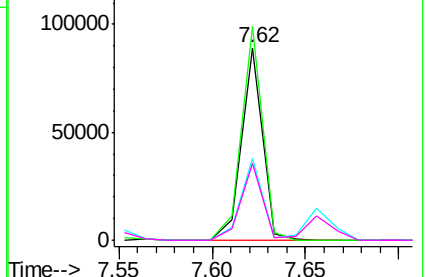

#18

Hexachloroethane

Concen: 22.92 ng

RT: 7.92 min Scan# 589

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion:117 Resp: 30454

Ion Ratio Lower Upper

117 100

119 96.7 79.0 118.6



201 95.4 79.0 118.6






Abundance Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E



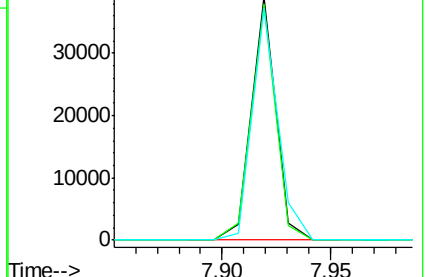



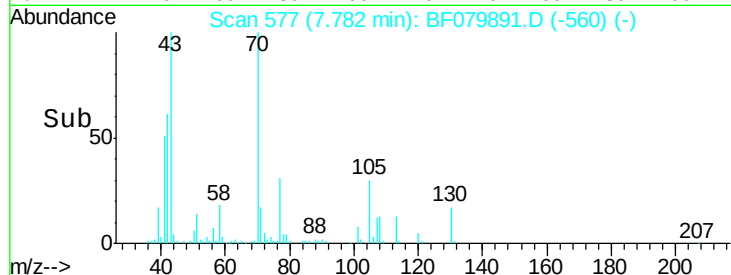

#19
n-Nitroso-di-n-propylamine
Concen: 24.38 ng
RT: 7.78 min Scan# 577
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09


Instrument :
BNA_F
ClientSampleId :
SSTDICC025


Tgt Ion:	70	Resp:	65344
Ion	Ratio	Lower	Upper
70	100		
42	60.8	49.0	73.4
101	8.0	6.6	9.8
130	17.1	12.7	19.1

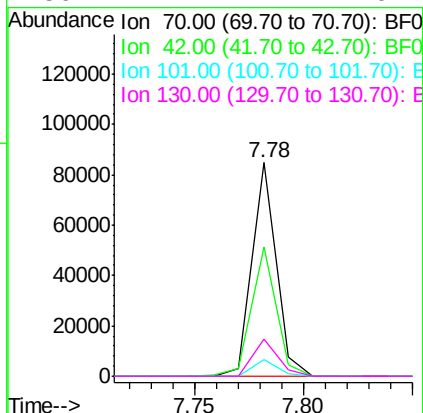

#20
3+4-Methylphenols
Concen: 23.93 ng
RT: 7.77 min Scan# 576
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:	107	Resp:	88286
Ion	Ratio	Lower	Upper
107	100		
108	89.3	71.1	111.1
77	31.1	12.2	52.2
79	27.5	8.5	48.5

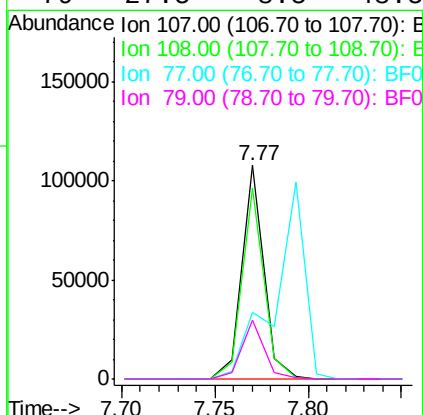







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.68 min Scan# 656
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:	136	Resp:	191335
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	9.6	7.3	10.9
68	6.8	5.9	8.9




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0


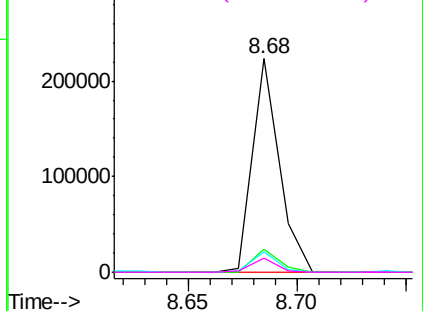



#22
Acetophenone
Concen: 24.41 ng
RT: 7.79 min Scan# 578
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:	105	Resp:	115295
Ion	Ratio	Lower	Upper
105	100		
71	1.0	1.0	1.4
51	23.7	19.8	29.6
120	22.2	17.6	26.4



Abundance Ion 105.00 (104.70 to 105.70): E
Ion 71.00 (70.70 to 71.70): BF0
Ion 51.00 (50.70 to 51.70): BF0
Ion 120.00 (119.70 to 120.70): E




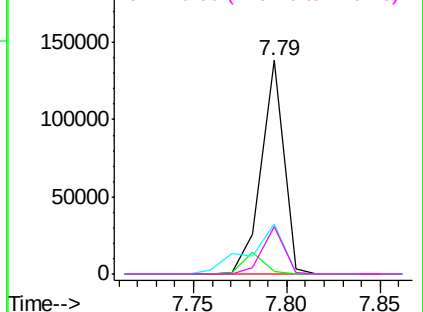




#23
 Nitrobenzene-d5
 Concen: 44.30 ng
 RT: 7.95 min Scan# 592
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09




Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025


Tgt Ion	Ratio	Lower	Upper
82	100		
128	51.4	40.3	60.5
54	46.1	38.0	57.0

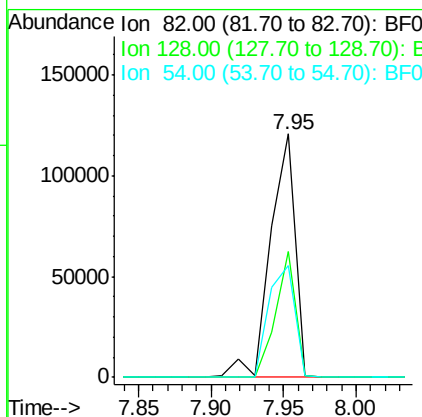

#24
 Nitrobenzene
 Concen: 23.83 ng
 RT: 7.96 min Scan# 593
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion	Ratio	Lower	Upper
77	100		
123	35.9	28.8	43.2
65	13.5	10.3	15.5

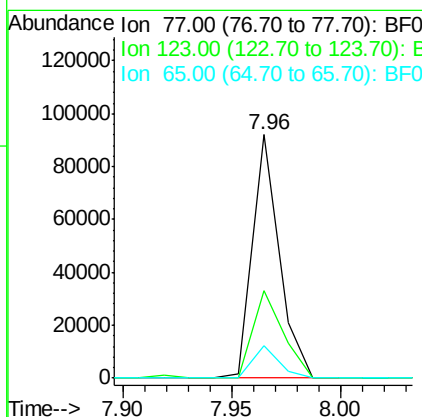



#25

Isophorone

Concen: 24.63 ng

RT: 8.20 min Scan# 614

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion: 82 Resp: 170835

Ion Ratio Lower Upper

82 100

95 6.7 5.2 7.8

138 17.2 13.3 19.9

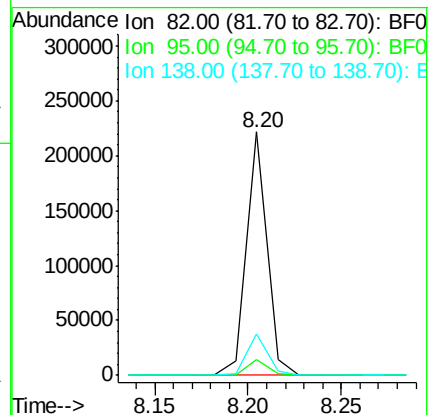

#26

2-Nitrophenol

Concen: 18.81 ng

RT: 8.30 min Scan# 622

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09




Tgt Ion: 139 Resp: 23771


Ion Ratio Lower Upper

139 100

109 23.3 17.8 26.6

65 35.6 29.4 44.0

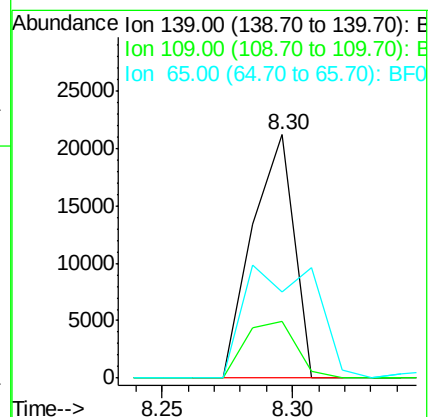



#27

2,4-Dimethylphenol

Concen: 24.31 ng

RT: 8.31 min Scan# 623

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025


Tgt Ion:122 Resp: 75473

Ion Ratio Lower Upper

122 100

107 115.4 91.7 137.5




121 57.1 47.8 71.6



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

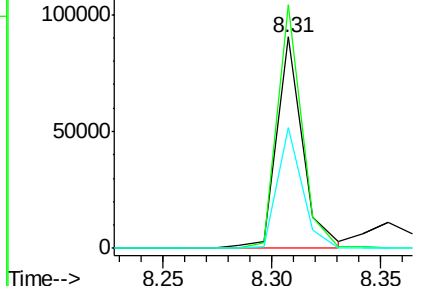

#28

bis(2-Chloroethoxy)methane

Concen: 23.69 ng

RT: 8.41 min Scan# 632

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion: 93 Resp: 98404

Ion Ratio Lower Upper

93 100

95 33.4 26.1 39.1



123 11.5 8.9 13.3




Abundance Ion 93.00 (92.70 to 93.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 123.00 (122.70 to 123.70): E

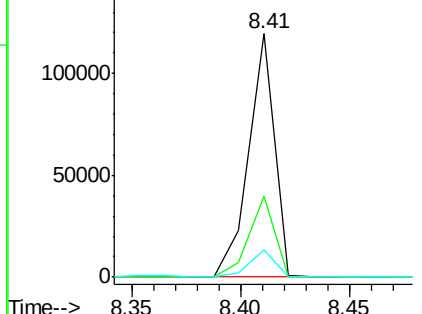


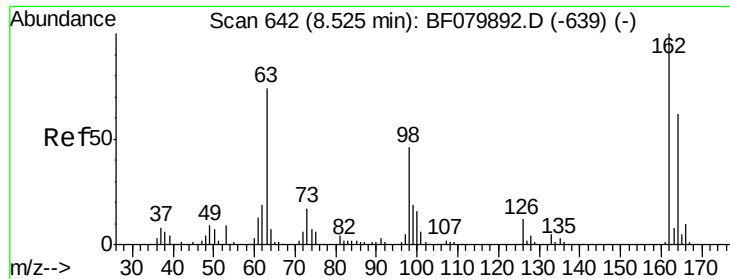




#29
 2,4-Dichlorophenol
 Concen: 23.61 ng
 RT: 8.52 min Scan# 642
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion	Ratio	Lower	Upper
162	100		
164	62.8	42.2	82.2
98	44.4	26.0	66.0

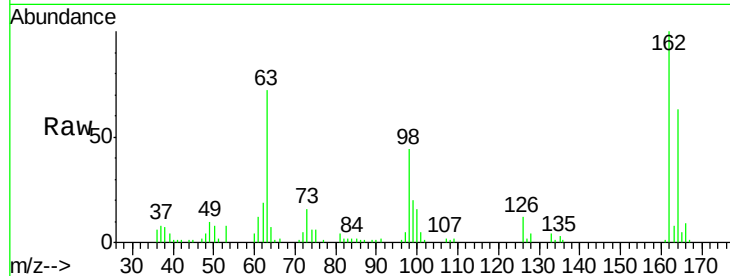


Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): BF0


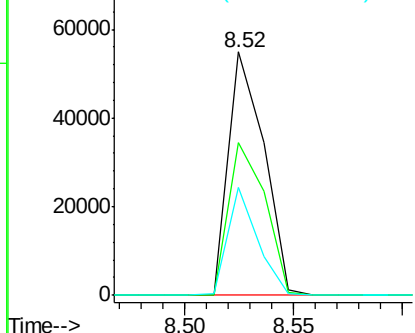



#30
 1,2,4-Trichlorobenzene
 Concen: 23.58 ng
 RT: 8.63 min Scan# 651
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion	Ratio	Lower	Upper
180	100		
182	97.7	75.7	113.5
145	27.0	21.1	31.7



Abundance Ion 180.00 (179.70 to 180.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 145.00 (144.70 to 145.70): E

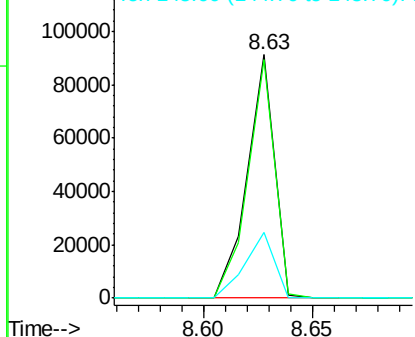







#31
Naphthalene
Concen: 25.86 ng
RT: 8.71 min Scan# 658
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:128 Resp: 264646
Ion Ratio Lower Upper
128 100
129 11.2 8.8 13.2
127 13.3 10.5 15.7




Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E


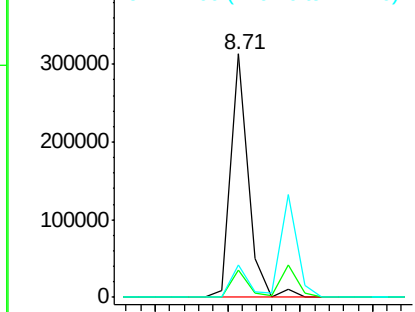



#32
Benzoic acid
Concen: 16.93 ng
RT: 8.35 min Scan# 627
Delta R.T. -0.01 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:122 Resp: 15903
Ion Ratio Lower Upper
122 100
105 127.7 102.7 142.7
77 96.9 77.1 117.1



Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0

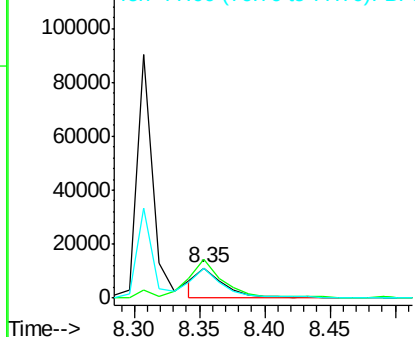


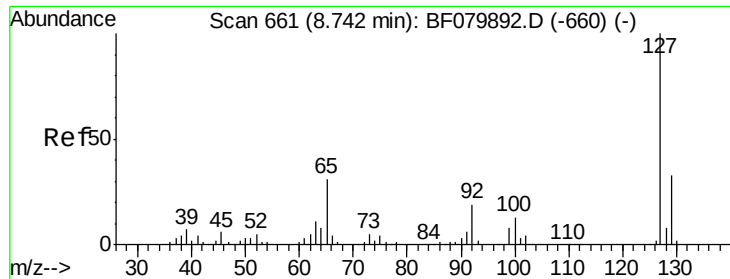




#33
4-Chloroaniline
Concen: 33.93 ng
RT: 8.74 min Scan# 661
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:	127	Resp:	139848
Ion	Ratio	Lower	Upper
127	100		
129	31.6	26.1	39.1
65	31.1	25.5	38.3
92	18.7	15.7	23.5




Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 65.00 (64.70 to 65.70): BF0
Ion 92.00 (91.70 to 92.70): BF0

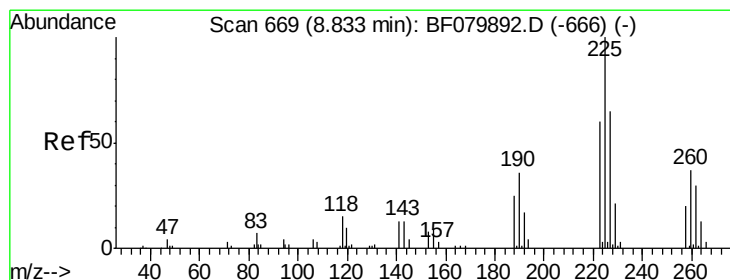
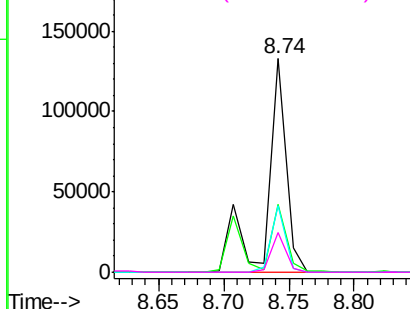



#34
Hexachlorobutadiene
Concen: 25.17 ng
RT: 8.83 min Scan# 669
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:	225	Resp:	46484
Ion	Ratio	Lower	Upper
225	100		
223	57.9	47.8	71.6
227	59.7	52.0	78.0



Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E



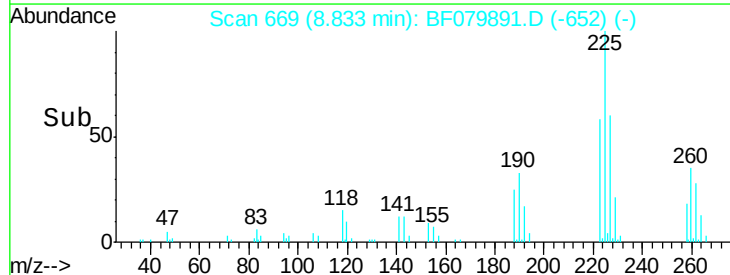
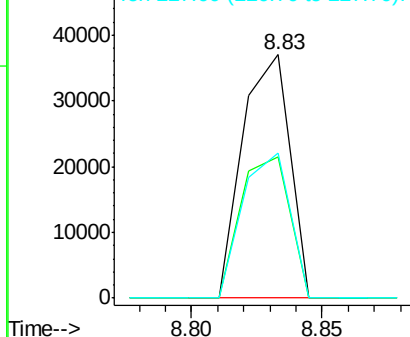




#35
 Caprolactam
 Concen: 22.98 ng
 RT: 9.07 min Scan# 690
 Delta R.T. -0.01 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09




Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025


Tgt Ion:113 Resp: 18284
 Ion Ratio Lower Upper
 113 100
 55 210.3 141.4 181.4#
 56 152.4 95.9 135.9#

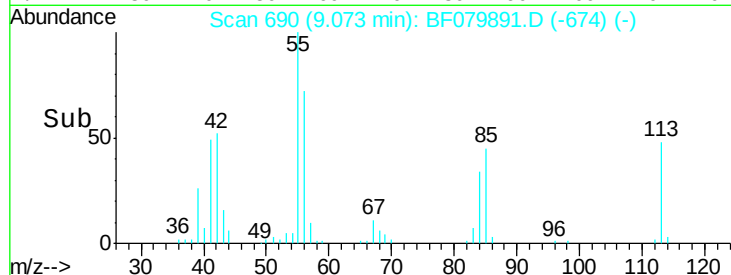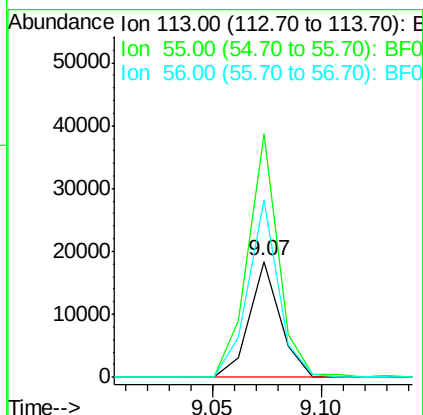

#36
 4-Chloro-3-methylphenol
 Concen: 25.53 ng
 RT: 9.21 min Scan# 702
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:107 Resp: 73693
 Ion Ratio Lower Upper
 107 100
 144 25.9 21.0 31.6
 142 80.4 64.5 96.7



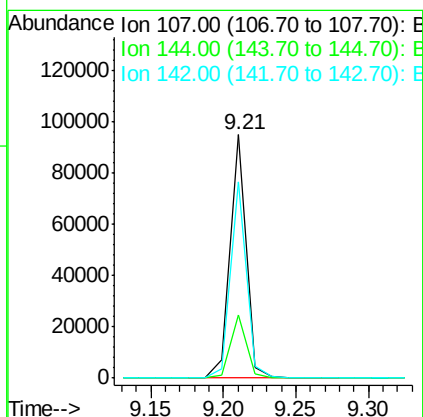





#37
2-Methylnaphthalene
Concen: 24.65 ng
RT: 9.40 min Scan# 719
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09




Instrument :
BNA_F
ClientSampleId :
SSTDIC025


Tgt Ion:142 Resp: 178451
Ion Ratio Lower Upper
142 100
141 89.3 70.9 106.3
115 31.4 25.0 37.4

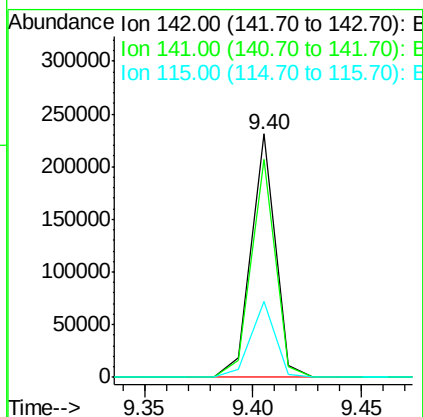

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.46 min Scan# 811
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:164 Resp: 93413
Ion Ratio Lower Upper
164 100
162 100.8 80.7 121.1
160 44.2 34.6 51.8

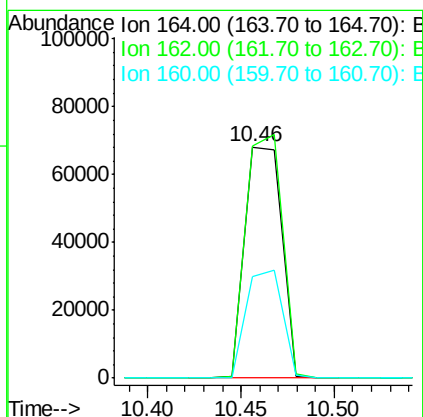



#39

1,2,4,5-Tetrachlorobenzene

Concen: 24.95 ng

RT: 9.58 min Scan# 734

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampled :

SSTDICC025

Tgt Ion:216 Resp: 80511


Ion Ratio Lower Upper

216 100

214 78.4 63.5 95.3

179 19.7 15.8 23.8

108 16.2 13.7 20.5






Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

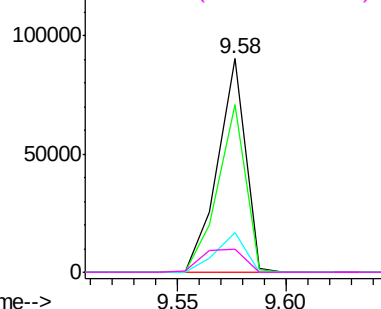

#40

Hexachlorocyclopentadiene

Concen: 16.58 ng

RT: 9.56 min Scan# 733

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion:237 Resp: 24646

Ion Ratio Lower Upper

237 100

235 60.2 41.3 81.3



272 12.5 0.0 32.2




Abundance Ion 236.80 (236.50 to 237.50): E

Ion 234.90 (234.60 to 235.60): E

Ion 271.75 (271.45 to 272.45): E

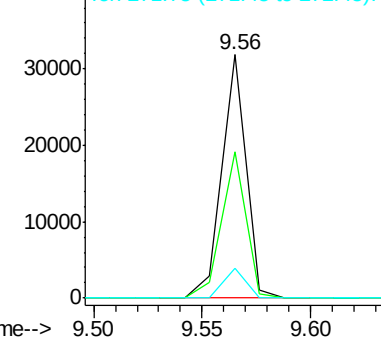







#41
 2,4,6-Tribromophenol
 Concen: 50.74 ng
 RT: 11.26 min Scan# 881
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion:330 Resp: 42302
 Ion Ratio Lower Upper
 330 100
 332 95.3 77.3 115.9
 141 35.3 26.8 40.2

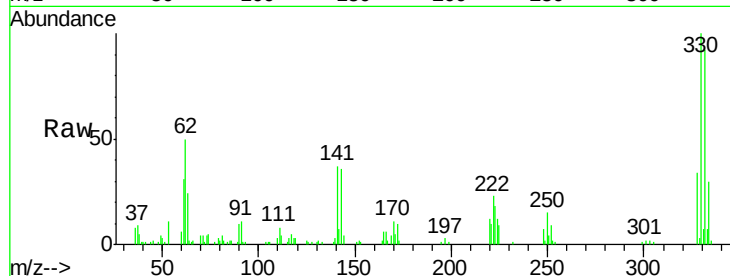


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


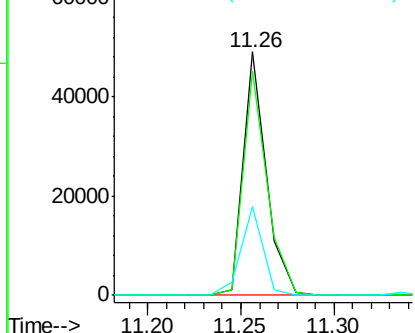



#42
 2,4,6-Trichlorophenol
 Concen: 24.47 ng
 RT: 9.68 min Scan# 743
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:196 Resp: 48231
 Ion Ratio Lower Upper
 196 100
 198 95.9 76.0 114.0
 200 30.0 24.9 37.3



Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 200.00 (199.70 to 200.70): E

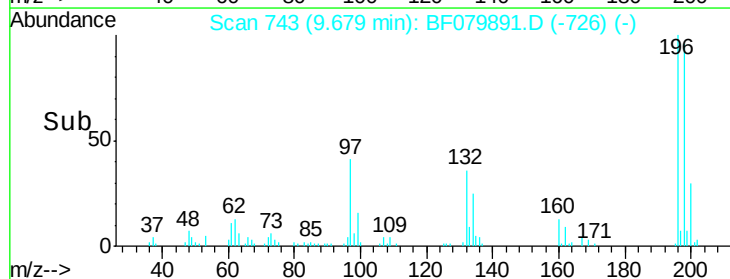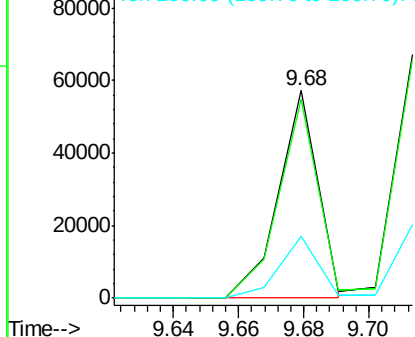







#43
 2,4,5-Trichlorophenol
 Concen: 26.59 ng
 RT: 9.71 min Scan# 746
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion:196 Resp: 54930
 Ion Ratio Lower Upper
 196 100
 198 98.2 76.0 114.0
 97 47.5 39.4 59.2
 132 28.6 23.6 35.4




Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 97.00 (96.70 to 97.70): BF0
 Ion 132.00 (131.70 to 132.70): E


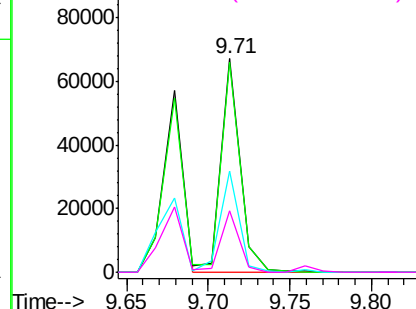



#44
 2-Fluorobiphenyl
 Concen: 53.50 ng
 RT: 9.76 min Scan# 750
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:172 Resp: 354632
 Ion Ratio Lower Upper
 172 100
 171 35.4 28.3 42.5
 170 23.1 19.0 28.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

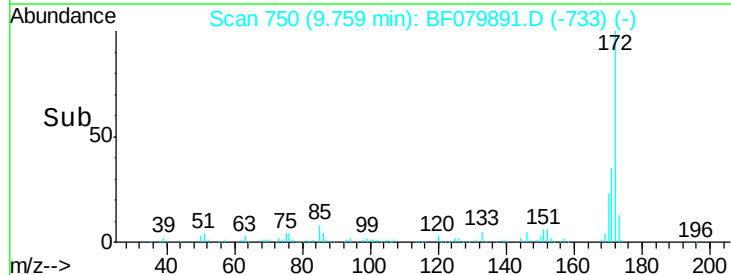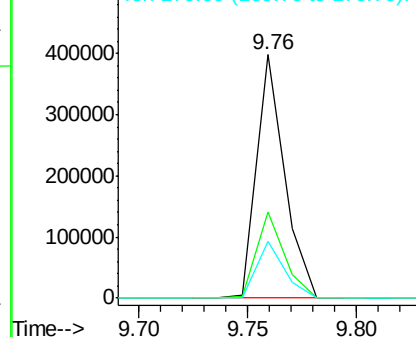


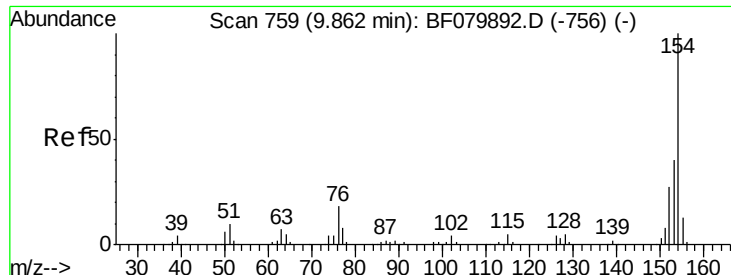




#45
 1,1'-Biphenyl
 Concen: 25.58 ng
 RT: 9.87 min Scan# 760
 Delta R.T. 0.01 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion:	154	Resp:	196869
Ion	Ratio	Lower	Upper
154	100		
153	40.1	20.1	60.1
76	7.7	0.0	38.4




Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BF0


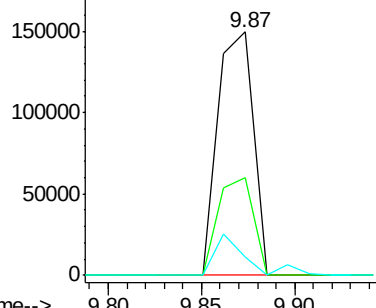



#46
 2-Chloronaphthalene
 Concen: 26.35 ng
 RT: 9.90 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:	162	Resp:	167225
Ion	Ratio	Lower	Upper
162	100		
127	40.3	33.1	49.7
164	31.4	26.2	39.4



Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 127.00 (126.70 to 127.70): E
 Ion 164.00 (163.70 to 164.70): E

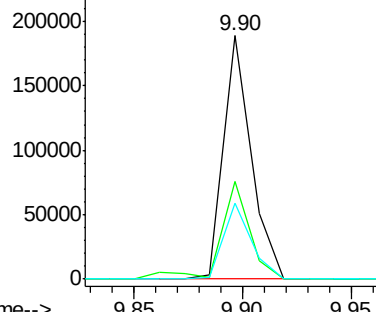



#47

2-Nitroaniline

Concen: 20.07 ng

RT: 9.98 min Scan# 769

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion: 65 Resp: 27696

Ion Ratio Lower Upper

65 100

92 62.1 51.1 76.7

138 81.4 62.0 93.0

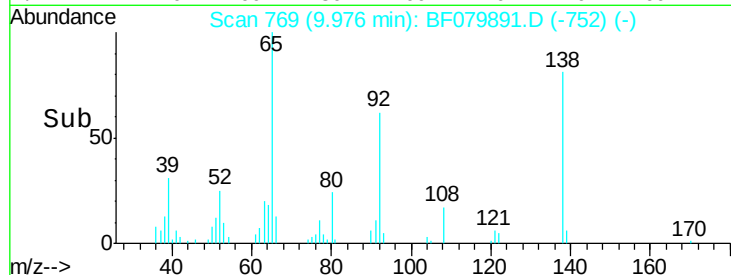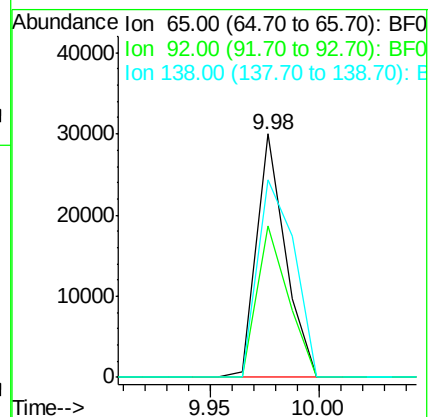

#48

Acenaphthylene

Concen: 25.68 ng

RT: 10.32 min Scan# 799

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09




Tgt Ion: 152 Resp: 278200


Ion Ratio Lower Upper

152 100

151 20.2 16.8 25.2

153 13.3 10.8 16.2



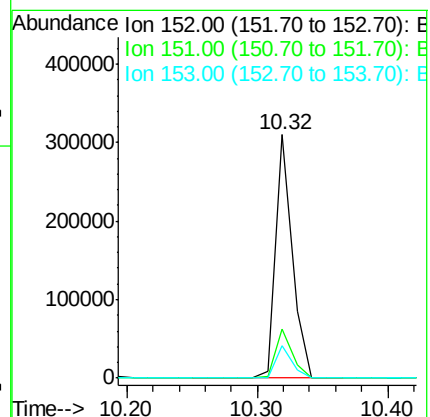



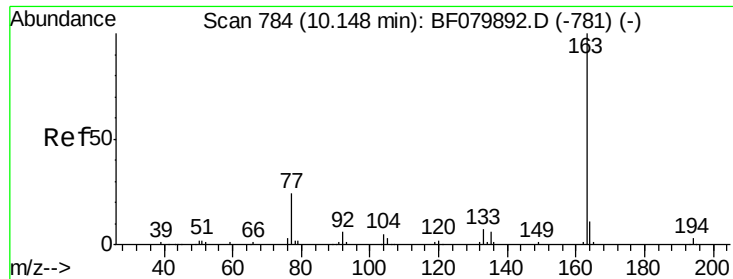

#49
Dimethylphthalate
Concen: 25.27 ng
RT: 10.15 min Scan# 784
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09




Instrument :
BNA_F
ClientSampleId :
SSTDIC025


Tgt Ion:163 Resp: 186041
Ion Ratio Lower Upper
163 100
194 3.2 2.6 4.0
164 10.4 8.6 12.8

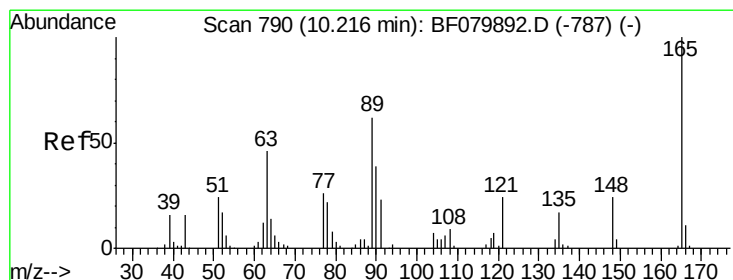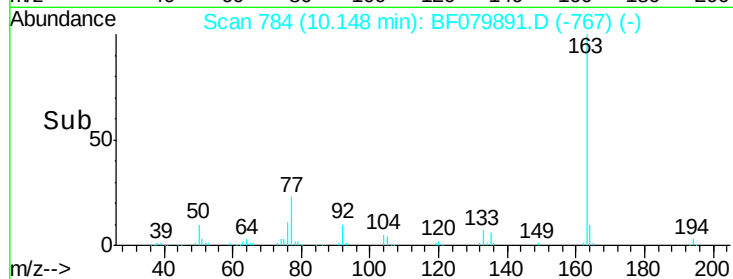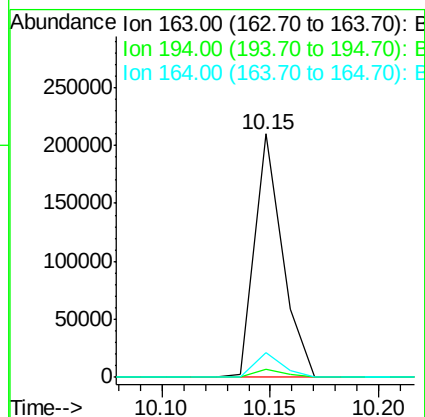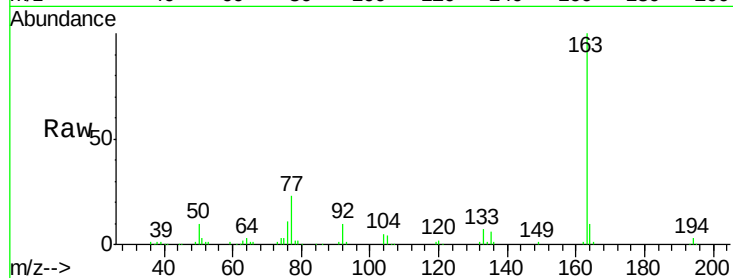

#50
2,6-Dinitrotoluene
Concen: 23.40 ng
RT: 10.22 min Scan# 790
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:165 Resp: 30052
Ion Ratio Lower Upper
165 100
63 58.4 46.4 69.6
89 59.3 49.6 74.4

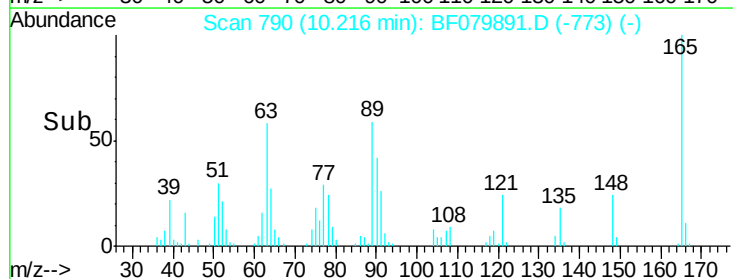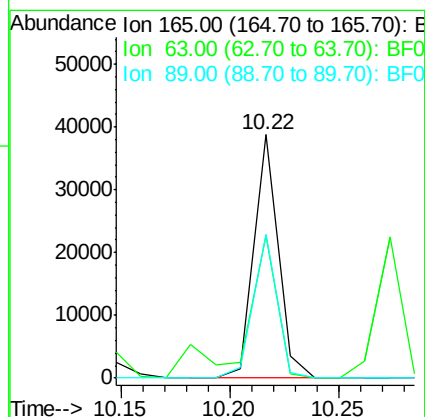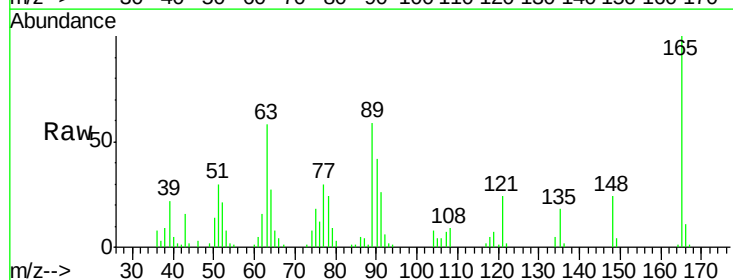

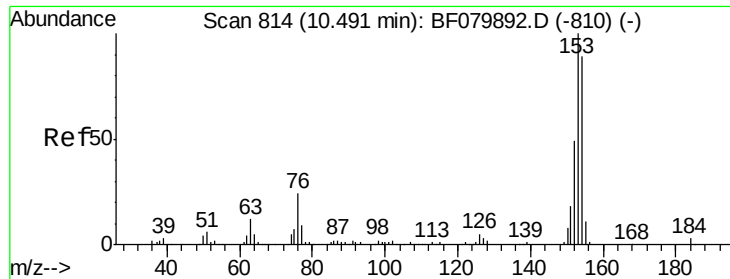

#51

Acenaphthene

Concen: 25.03 ng

RT: 10.49 min Scan# 814

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025


Tgt Ion:154 Resp: 157063

Ion Ratio Lower Upper

154 100

153 111.6 90.0 135.0




152 52.2 43.7 65.5

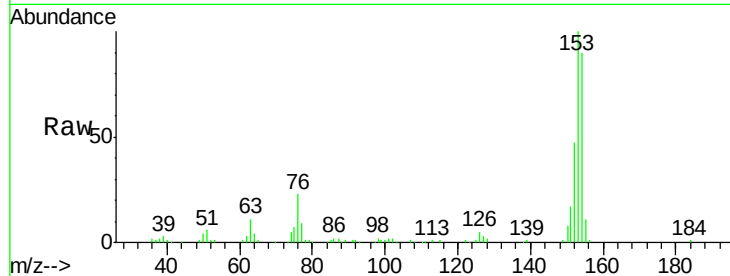

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

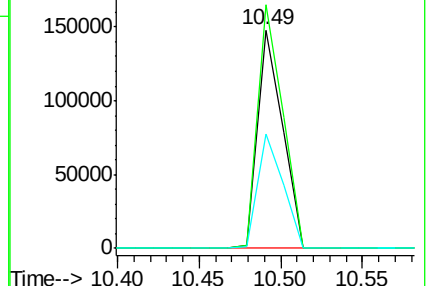

#52

3-Nitroaniline

Concen: 24.08 ng

RT: 10.39 min Scan# 805

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion:138 Resp: 37911

Ion Ratio Lower Upper

138 100

108 12.3 9.0 13.6



92 122.5 103.1 154.7




Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BF0

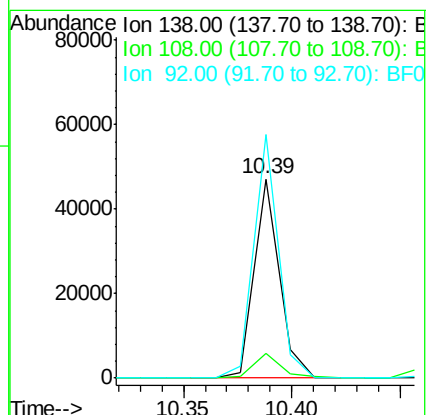

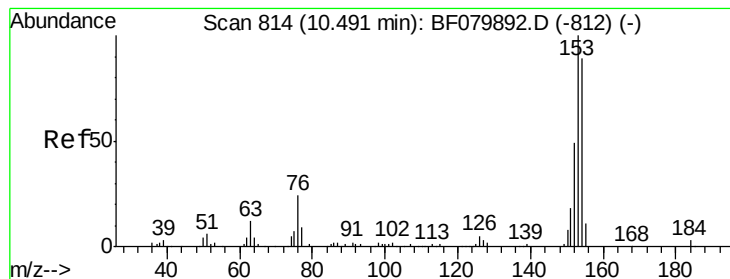

#53

2,4-Dinitrophenol

Concen: 9.23 ng

RT: 10.49 min Scan# 814

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025



Tgt Ion:184 Resp: 2544

Ion Ratio Lower Upper

184 100

63 808.6 357.0 535.4#



154 6869.9 2660.2 3990.4#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 154.00 (153.70 to 154.70): E

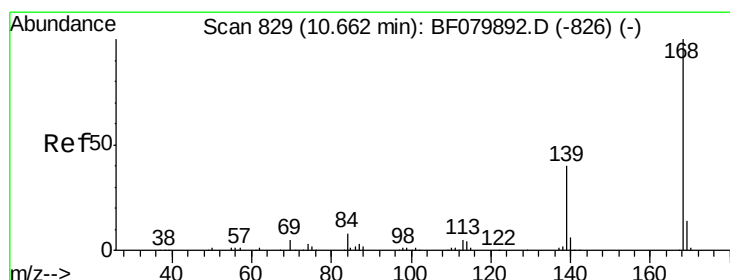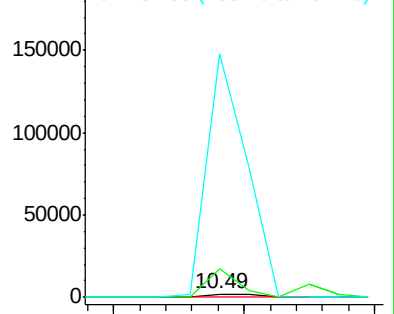

#54

Dibenzofuran

Concen: 25.57 ng

RT: 10.66 min Scan# 829

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09



Tgt Ion:168 Resp: 226400

Ion Ratio Lower Upper

168 100

139 39.2 32.2 48.2


169 13.6 11.0 16.6




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

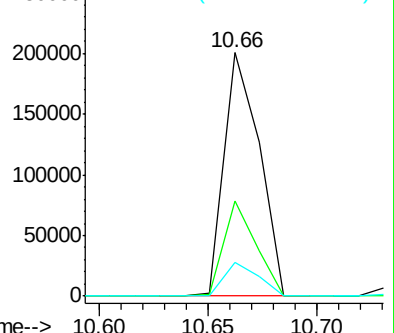

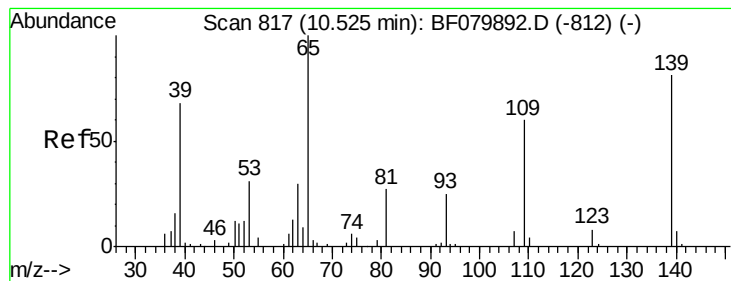

#55

4-Nitrophenol

Concen: 22.68 ng

RT: 10.52 min Scan# 817

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDIC025





Tgt Ion:139 Resp: 25718

Ion Ratio Lower Upper

139 100

109 71.7 54.8 94.8

65 117.6 104.8 144.8

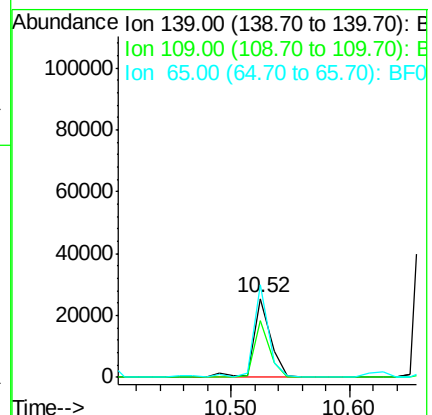

#56

2,4-Dinitrotoluene

Concen: 20.10 ng

RT: 10.63 min Scan# 826

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Tgt Ion:165 Resp: 32774




Ion Ratio Lower Upper


165 100

63 29.1 24.3 36.5

89 55.2 45.4 68.2

182 2.2 1.8 2.8

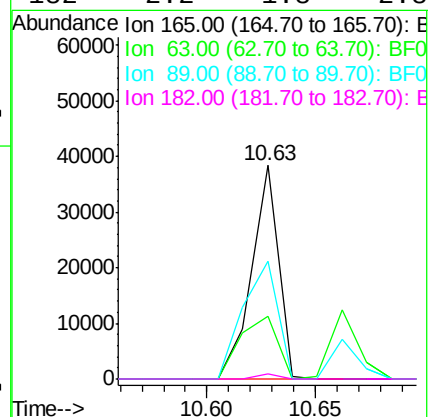

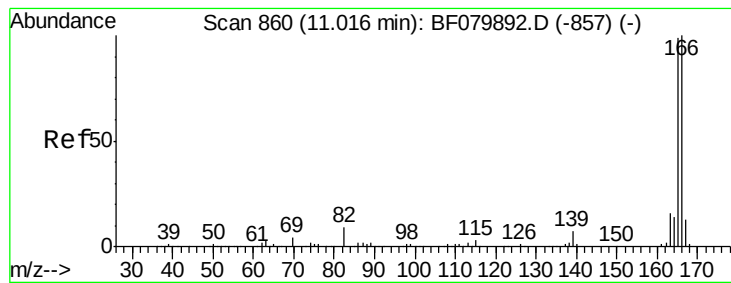

#57

Fluorene

Concen: 26.01 ng

RT: 11.02 min Scan# 860

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDICC025





Tgt Ion:166 Resp: 204581

Ion Ratio Lower Upper

166 100

165 99.0 79.0 118.6

167 12.9 10.3 15.5

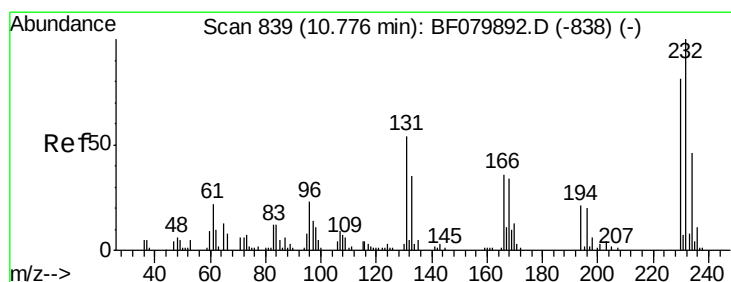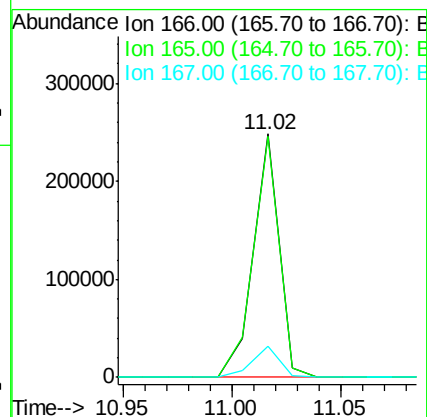

#58

2,3,4,6-Tetrachlorophenol

Concen: 25.39 ng

RT: 10.78 min Scan# 839

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Tgt Ion:232 Resp: 39018




Ion Ratio Lower Upper


232 100

131 47.0 35.4 53.2

130 1.9 1.5 2.3

166 30.0 24.1 36.1

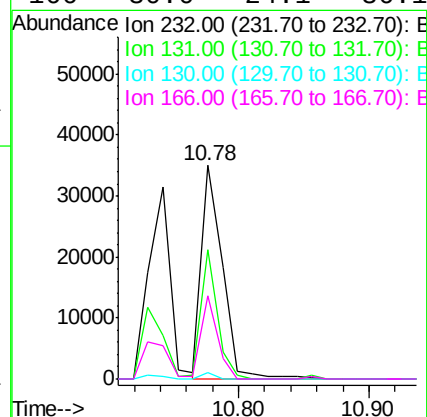







#59
Diethylphthalate
Concen: 27.06 ng
RT: 10.86 min Scan# 846
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:149 Resp: 195870
Ion Ratio Lower Upper
149 100
177 21.6 16.9 25.3
150 12.9 10.4 15.6




Abundance Ion 149.00 (148.70 to 149.70): E
Ion 177.00 (176.70 to 177.70): E
Ion 150.00 (149.70 to 150.70): E


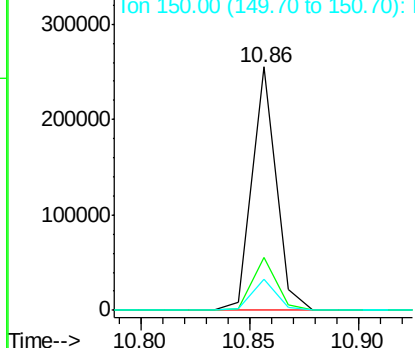



#60
4-Chlorophenyl-phenylether
Concen: 25.74 ng
RT: 10.99 min Scan# 858
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:204 Resp: 87855
Ion Ratio Lower Upper
204 100
206 32.4 28.0 42.0
141 72.4 55.3 82.9



Abundance Ion 204.00 (203.70 to 204.70): E
Ion 206.00 (205.70 to 206.70): E
Ion 141.00 (140.70 to 141.70): E

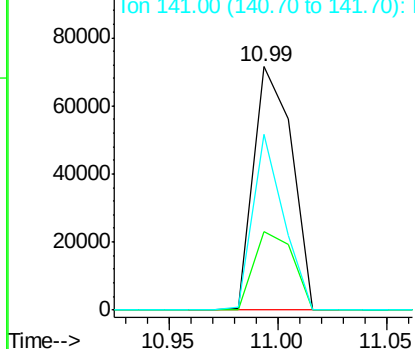


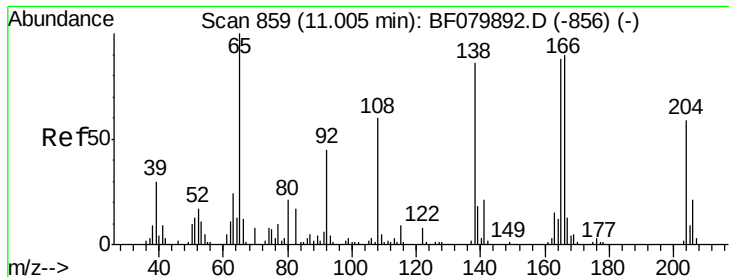




#61
4-Nitroaniline
Concen: 24.71 ng
RT: 11.00 min Scan# 859
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:138 Resp: 38566
Ion Ratio Lower Upper
138 100
92 50.8 32.9 72.9
108 68.2 50.4 90.4

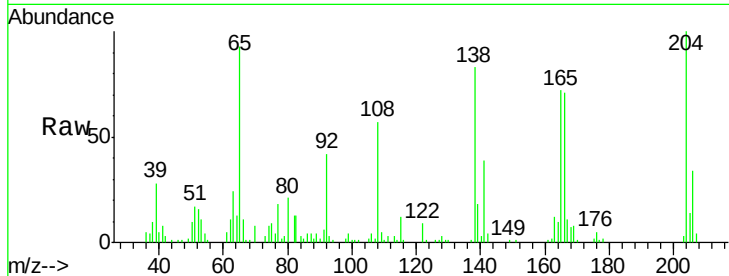




Abundance Ion 138.00 (137.70 to 138.70): E
Ion 92.00 (91.70 to 92.70): BF0
Ion 108.00 (107.70 to 108.70): E

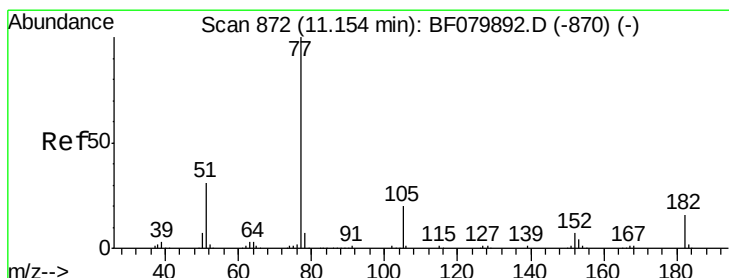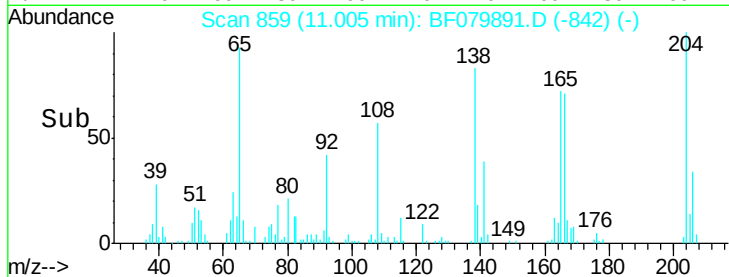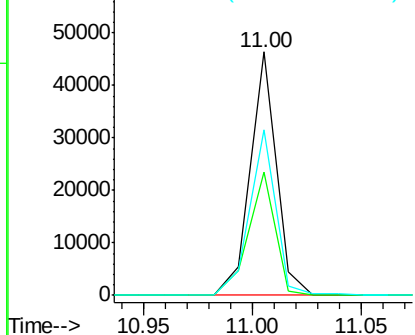


#62
Azobenzene
Concen: 24.57 ng
RT: 11.15 min Scan# 872
Delta R.T. -0.00 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion: 77 Resp: 174110
Ion Ratio Lower Upper
77 100
182 13.4 0.0 35.9
105 18.7 0.1 40.1
51 32.0 11.5 51.5

Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 182.00 (181.70 to 182.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 51.00 (50.70 to 51.70): BF0

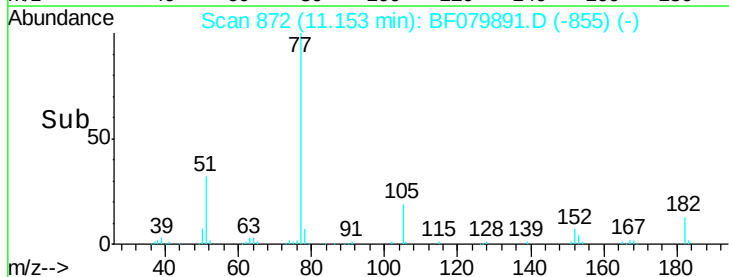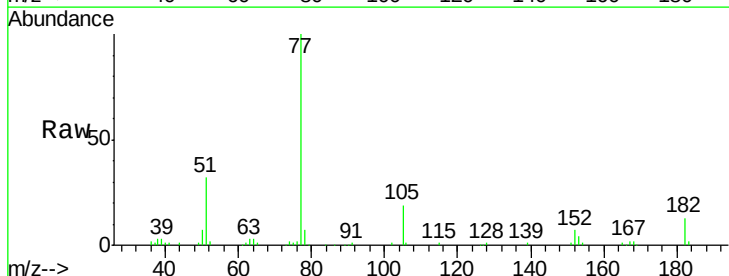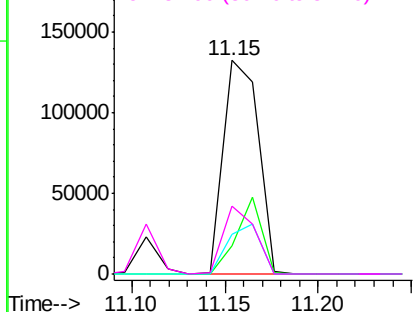

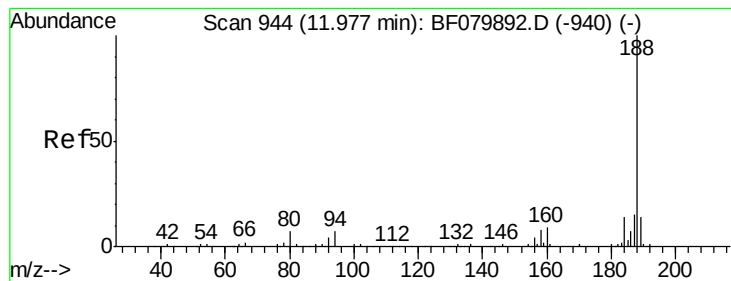

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.99 min Scan# 945

Delta R.T. 0.01 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09

Instrument :

BNA_F

ClientSampleId :

SSTDICC025


Tgt Ion:188 Resp: 196130

Ion Ratio Lower Upper

188 100

94 10.5 5.8 8.8#




80 11.9 5.9 8.9#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

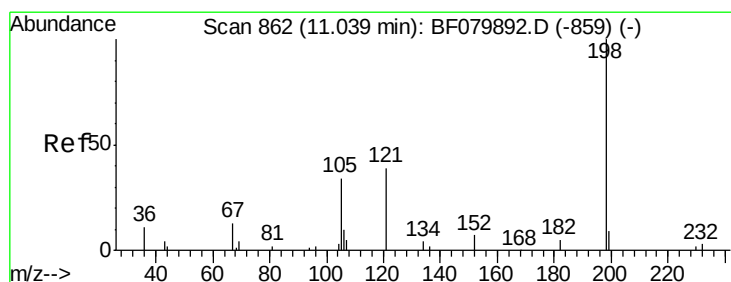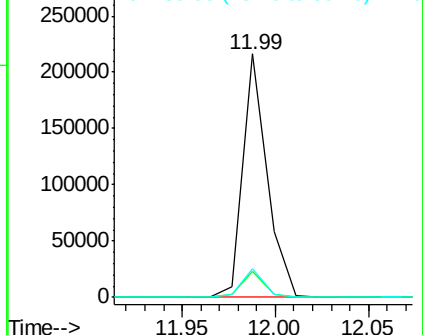

#64

4,6-Dinitro-2-methylphenol

Concen: 12.64 ng

RT: 11.04 min Scan# 862

Delta R.T. -0.00 min

Lab File: BF079891.D

Acq: 11 Jun 2015 13:09


Tgt Ion:198 Resp: 6682

Ion Ratio Lower Upper

198 100

51 51.0 22.1 62.1



105 44.5 22.7 62.7




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF0

Ion 105.00 (104.70 to 105.70): E

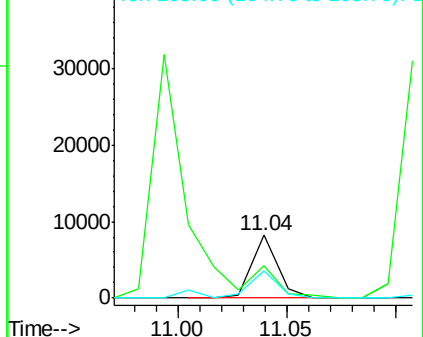







#65
 n-Nitrosodiphenylamine
 Concen: 24.36 ng
 RT: 11.11 min Scan# 868
 Delta R.T. -0.00 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC025

Tgt Ion:169 Resp: 159797
 Ion Ratio Lower Upper
 169 100
 168 68.1 54.2 81.4
 167 37.5 29.7 44.5




Abundance Ion 169.00 (168.70 to 169.70): E
 Ion 168.00 (167.70 to 168.70): E
 Ion 167.00 (166.70 to 167.70): E


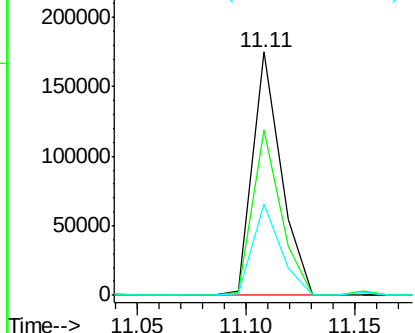



#66
 4-Bromophenyl-phenylether
 Concen: 22.77 ng
 RT: 11.51 min Scan# 903
 Delta R.T. 0.01 min
 Lab File: BF079891.D
 Acq: 11 Jun 2015 13:09

Tgt Ion:248 Resp: 52227
 Ion Ratio Lower Upper
 248 100
 250 95.8 80.2 120.2
 141 39.2 46.9 70.3#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

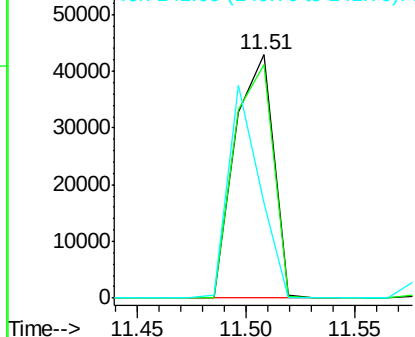







#67
Hexachlorobenzene
Concen: 25.50 ng
RT: 11.59 min Scan# 910
Delta R.T. 0.01 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Instrument :
BNA_F
ClientSampleId :
SSTDIC025

Tgt Ion:284 Resp: 60900
Ion Ratio Lower Upper
284 100
142 19.7 23.5 35.3#
249 29.7 25.3 37.9




Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

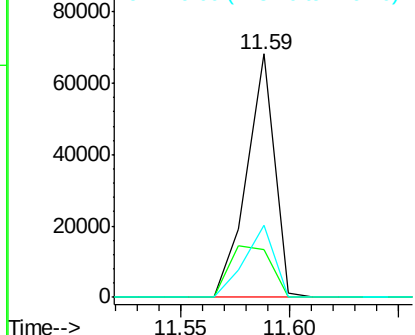

#68
Atrazine
Concen: 24.04 ng
RT: 11.64 min Scan# 915
Delta R.T. 0.01 min
Lab File: BF079891.D
Acq: 11 Jun 2015 13:09

Tgt Ion:200 Resp: 45351
Ion Ratio Lower Upper
200 100
173 23.7 4.1 44.1
215 51.3 29.2 69.2



Abundance Ion 200.00 (199.70 to 200.70): E
Ion 173.00 (172.70 to 173.70): E
Ion 215.00 (214.70 to 215.70): E

