

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
 Data File : BF079897.D
 Acq On : 11 Jun 2015 16:06
 Operator : TP/IZ
 Sample : PB83888BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83888BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.170	84	86	93	rVV	240557	388770	14.11%	2.156%
2	2.284	93	96	100	rVB	1825905	2755347	100.00%	15.284%
3	2.353	100	102	133	rVB	398912	1057209	38.37%	5.864%
4	6.010	419	422	424	rBV	1157467	1285324	46.65%	7.130%
5	6.993	505	508	510	rBV	1624025	1416302	51.40%	7.856%
6	7.165	520	523	525	rBV	1011356	1321073	47.95%	7.328%
7	7.393	541	543	546	rVB	369019	294935	10.70%	1.636%
8	7.553	555	557	559	rBV	1371073	1090111	39.56%	6.047%
9	7.953	589	592	594	rBV	613414	697862	25.33%	3.871%
10	8.685	654	656	658	rBV	520171	410941	14.91%	2.279%
11	9.759	748	750	753	rBV	2147544	1763887	64.02%	9.784%
12	10.456	809	811	814	rBV	514313	479195	17.39%	2.658%
13	11.257	878	881	883	rBV	837626	930301	33.76%	5.160%
14	11.965	941	943	946	rBV	549462	546969	19.85%	3.034%
15	13.668	1090	1092	1095	rBV	1992150	2376733	86.26%	13.184%
16	14.960	1203	1205	1208	rBV	454455	626259	22.73%	3.474%
17	16.891	1371	1374	1383	rBV	363452	586708	21.29%	3.254%


Sum of corrected areas: 18027926

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
Data File : BF079897.D
Acq On : 11 Jun 2015 16:06
Operator : TP/IZ
Sample : PB83888BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83888BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

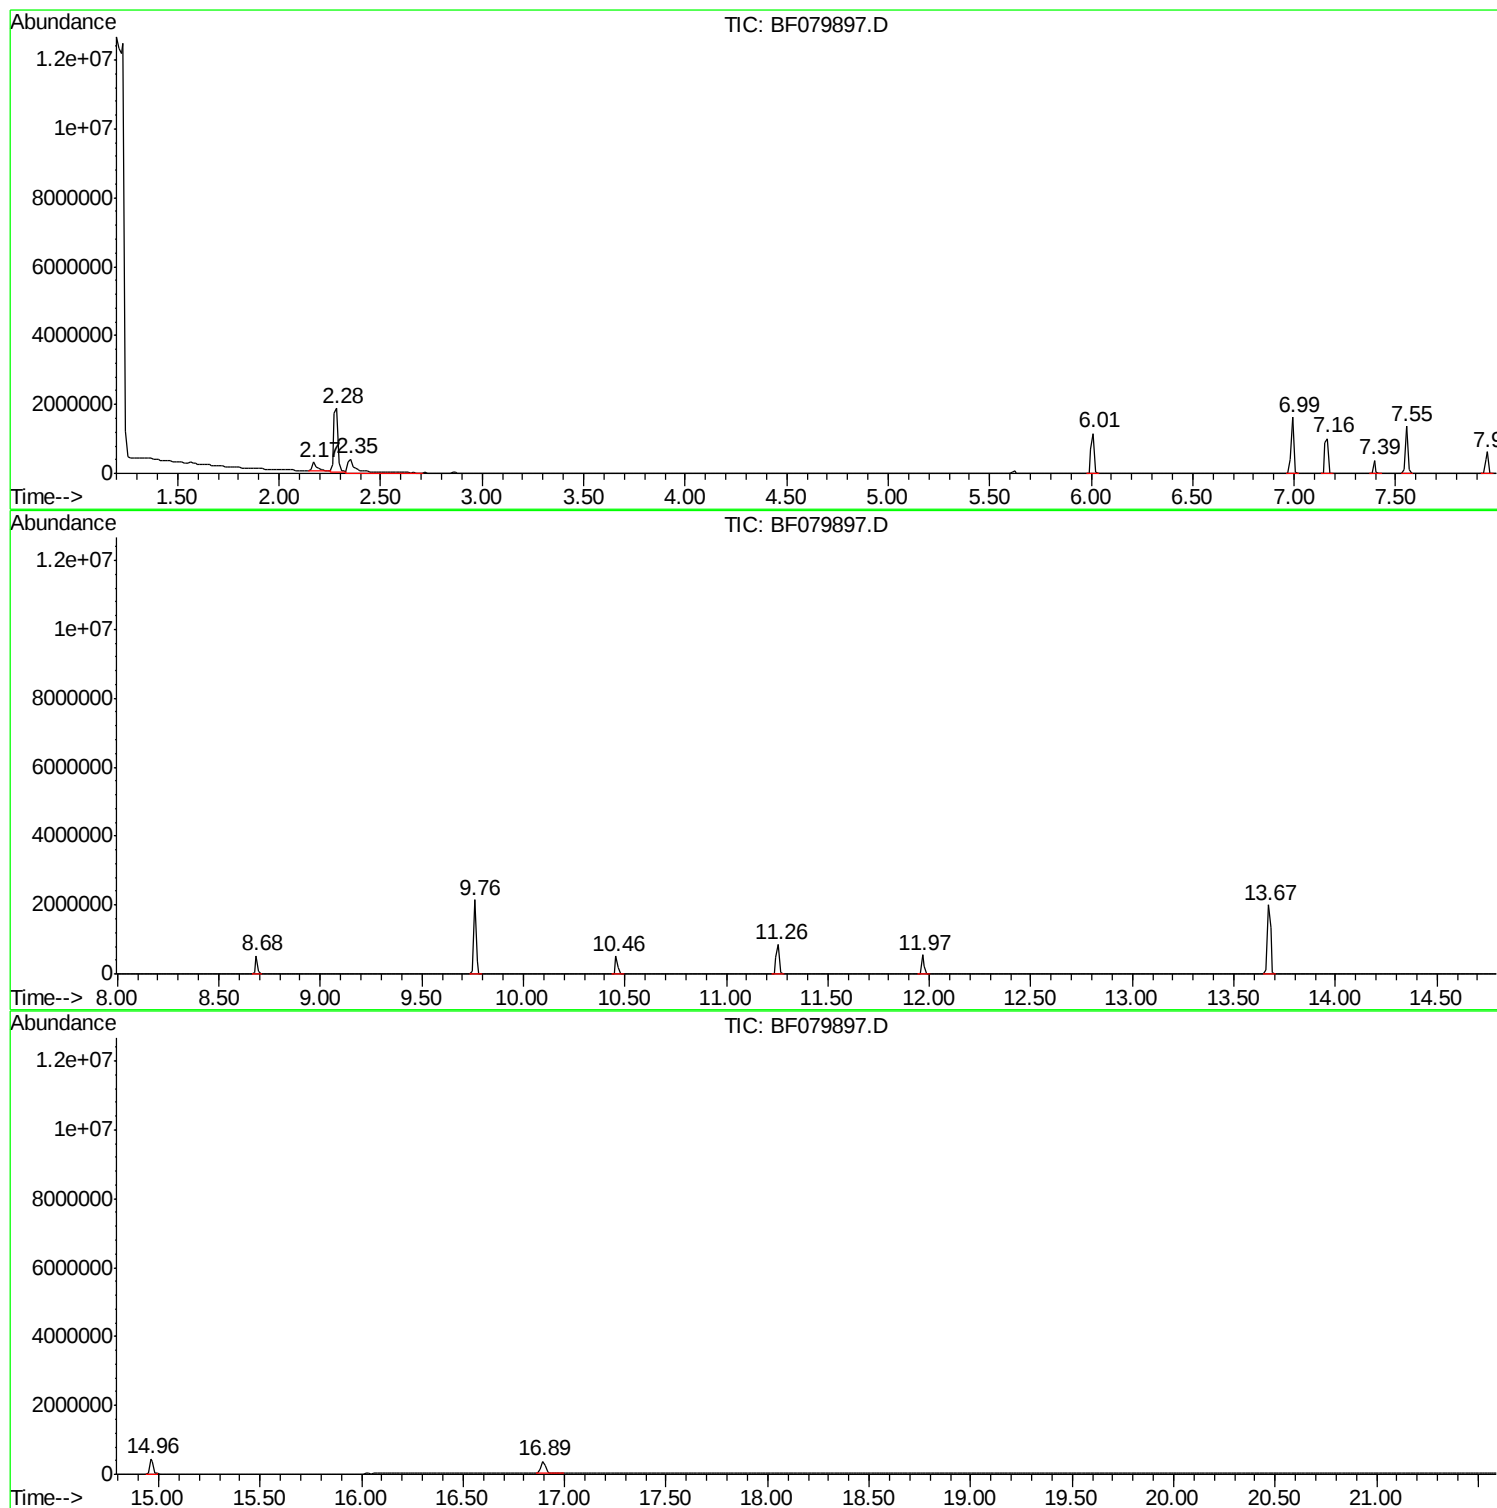

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
Data File : BF079897.D
Acq On : 11 Jun 2015 16:06
Operator : TP/IZ
Sample : PB83888BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83888BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown2.28 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.28	186.84 ng	2755350	1,4-Dichlorobenzene-d4	7.39

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	39
2		2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
3		Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
4		1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9
5		Borane, dimethoxy-	74	C2H7BO2	004542-61-4	7

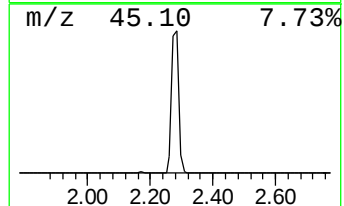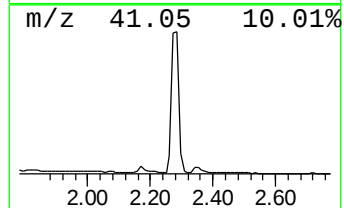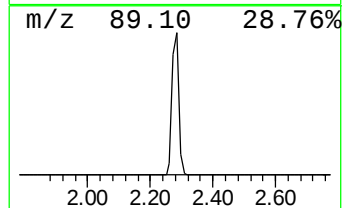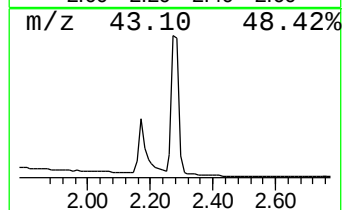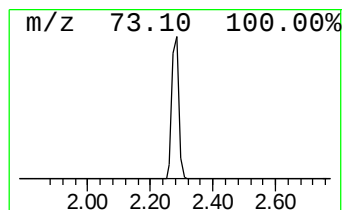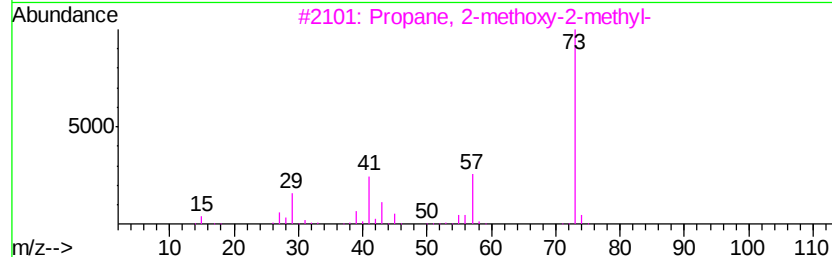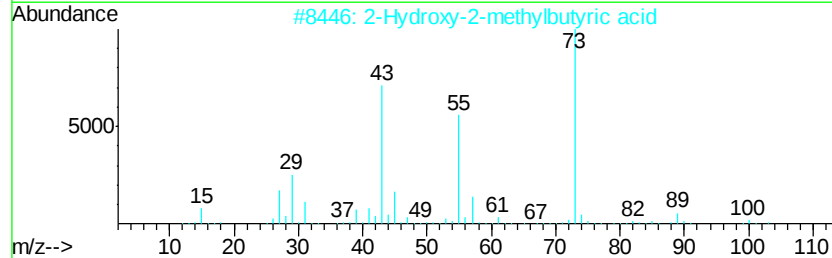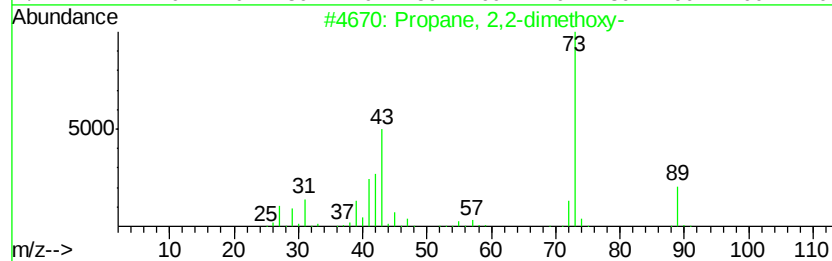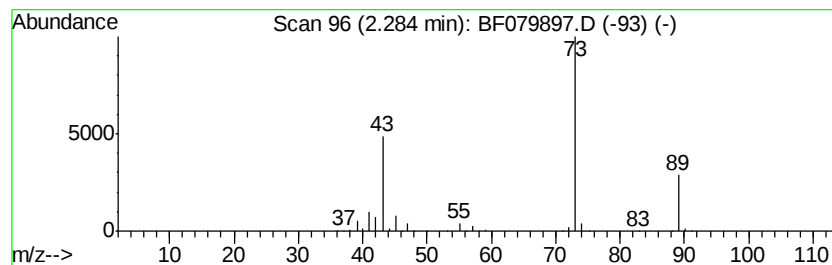

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061115\
Data File : BF079897.D
Acq On : 11 Jun 2015 16:06
Operator : TP/IZ
Sample : PB83888BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83888BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.16 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.16	89.58 ng	1321070	1,4-Dichlorobenzene-d4	7.39

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

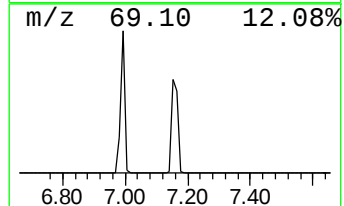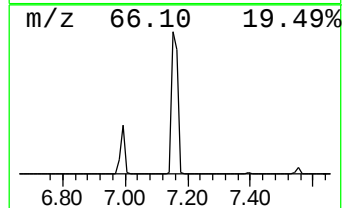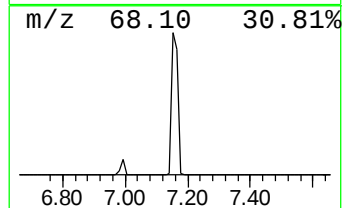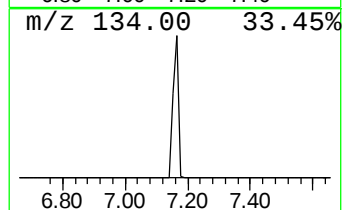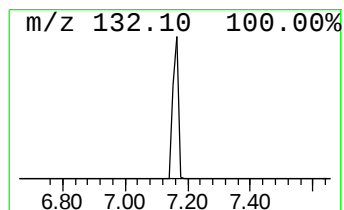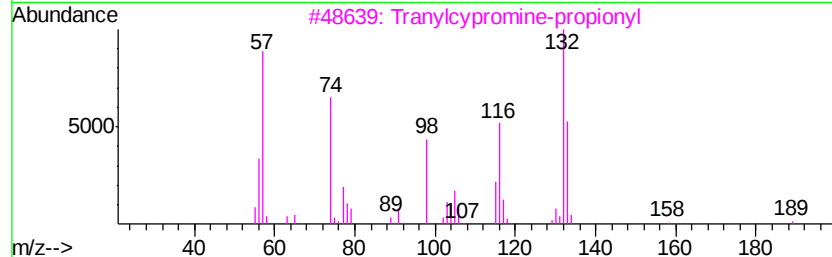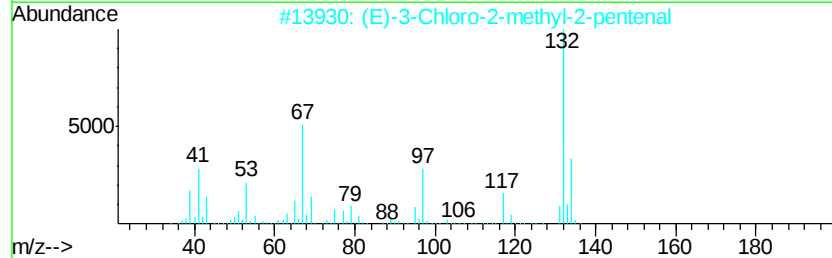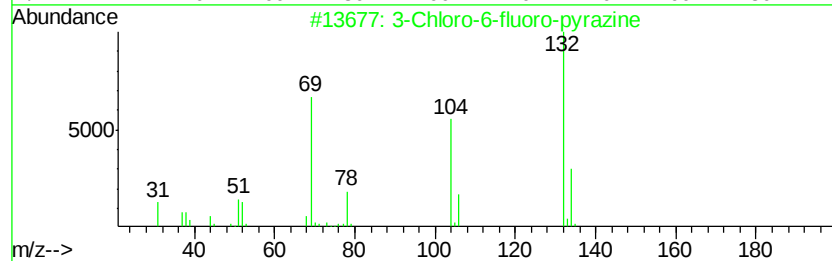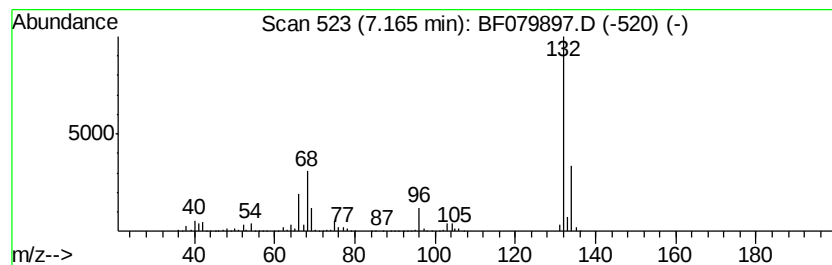

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061115\
Data File : BF079897.D
Acq On : 11 Jun 2015 16:06
Operator : TP/IZ
Sample : PB83888BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83888BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.28	2.28	186.8	ng	2755350	1	7.39	294935	20.0
unknown7.16	7.16	89.6	ng	1321070	1	7.39	294935	20.0