


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061115\
 Data File : BF079909.D
 Acq On : 11 Jun 2015 23:01
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 12 12:05:26 2015

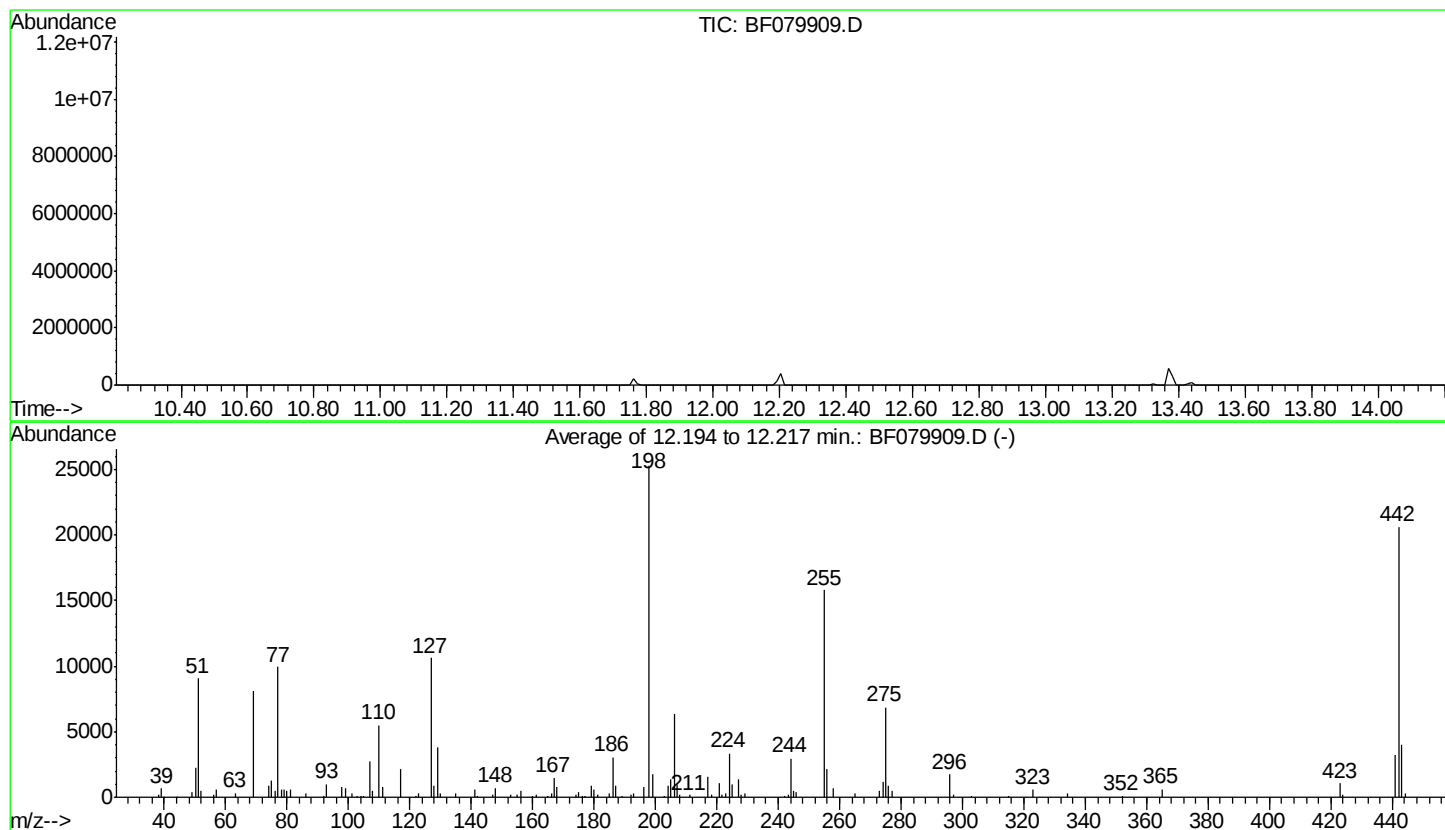

AutoFind: Scans 963, 964, 965; Background Corrected with Scan 960

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	9037	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	8116	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	10597	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25273	PASS
199	198	5	9	6.9	1735	PASS
275	198	10	60	27.1	6837	PASS
365	198	1	100	2.4	603	PASS
441	442	0.01	24	15.5	3191	PASS
442	198	50	100	81.5	20592	PASS
443	442	15	24	19.6	4028	PASS