
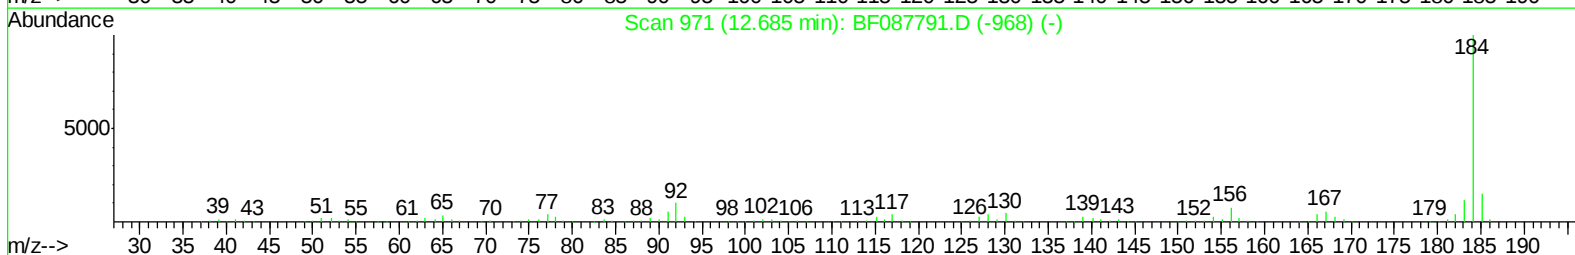
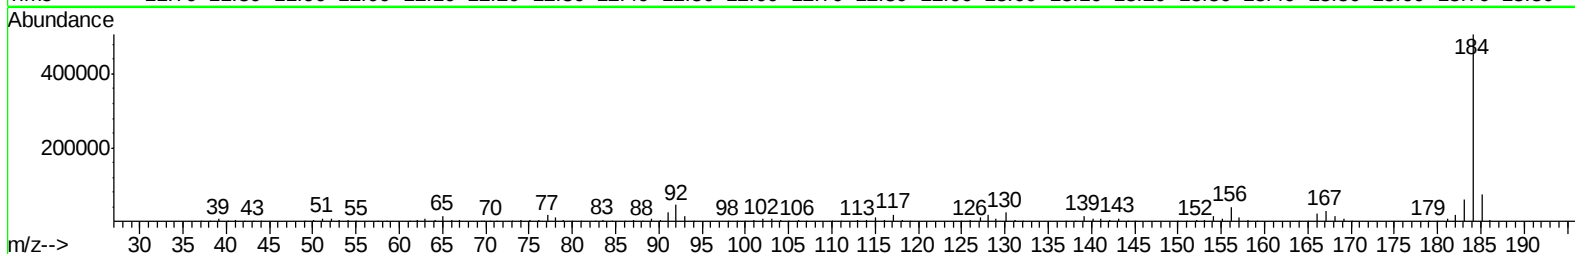


Data Path : Z:\HPCHEM1\BNA_F\Data\bf061116\
Data File : BF087899.D
Acq On : 11 Jun 2016 13:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 03:14:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 02:17:28 2016
Response via : Initial Calibration

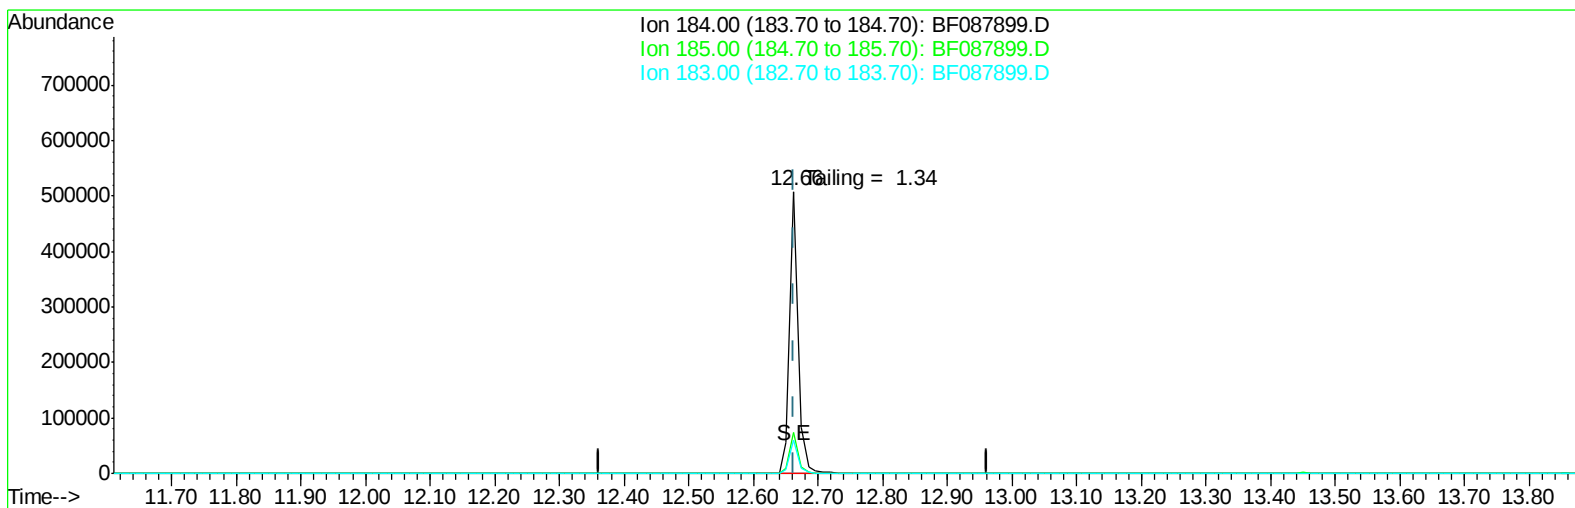

TIC: BF087899.D

(76) Benzidine




12.662min (-0.000) 57352.28ng

response 463704

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.43
183.00	11.60	11.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\bf061116\
Data File : BF087899.D
Acq On : 11 Jun 2016 13:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 03:14:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 02:17:28 2016
Response via : Initial Calibration

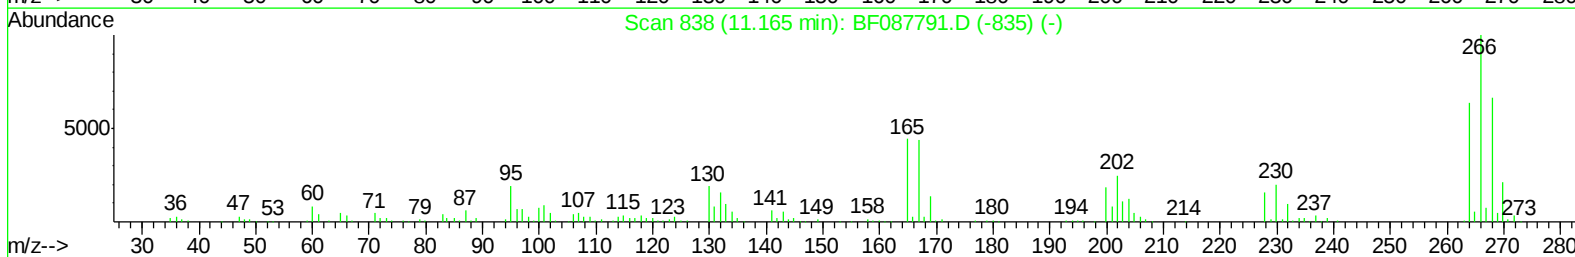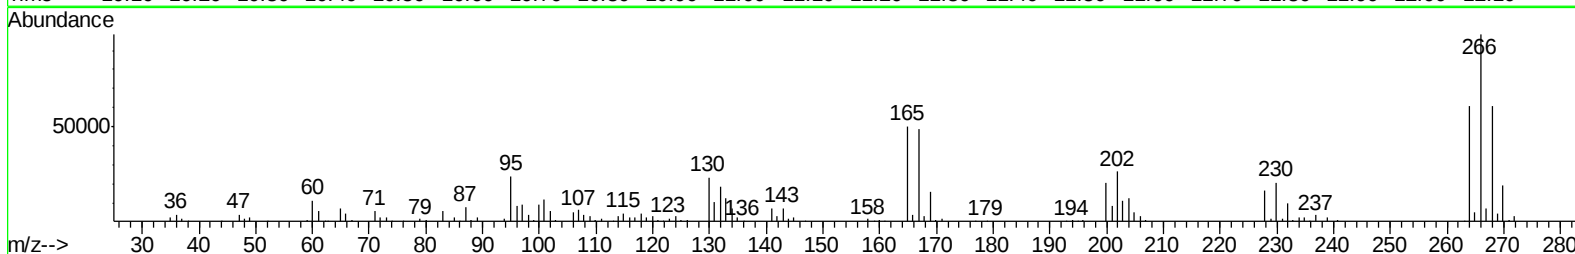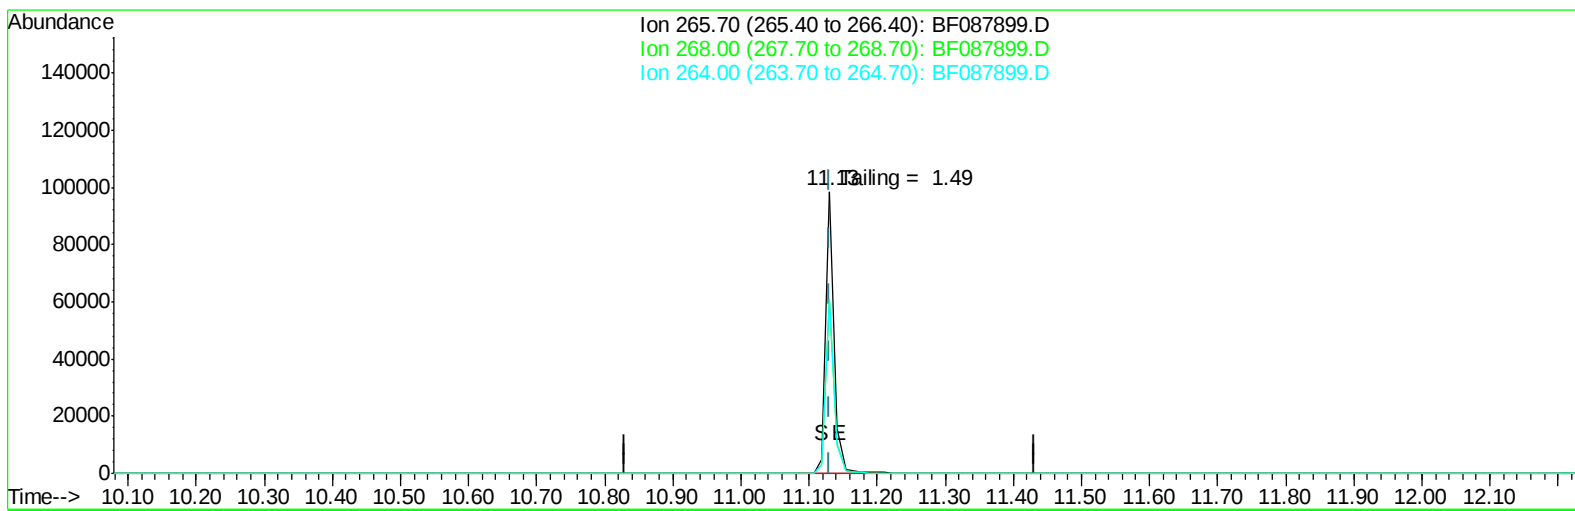

TIC: BF087899.D

(69) Pentachlorophenol (C)

11.131min (-0.000) 0.00ng

response 84440

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	61.72
264.00	62.00	61.97
0.00	0.00	0.00