

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061116\
 Data File : BF087925.D
 Acq On : 12 Jun 2016 3:24
 Operator : UM/SJ
 Sample : PB91213BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91213BL

Quant Time: Jun 12 06:05:08 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 18:51:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	108916	20.00	ng	-0.05
21) Naphthalene-d8	8.09	136	449339	20.00	ng	-0.03
38) Acenaphthene-d10	9.84	164	208256	20.00	ng	-0.05
63) Phenanthrene-d10	11.32	188	433340	20.00	ng	-0.03
75) Chrysene-d12	13.95	240	345868	20.00	ng	-0.03
86) Perylene-d12	15.37	264	263859	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	737530	115.76	ng	-0.03
7) Phenol-d6	6.43	99	812431	105.22	ng	-0.05
23) Nitrobenzene-d5	7.37	82	590563	76.75	ng	-0.05
41) 2,4,6-Tribromophenol	10.63	330	214422	97.51	ng	-0.05
44) 2-Fluorobiphenyl	9.16	172	1001272	74.87	ng	-0.05
78) Terphenyl-d14	12.91	244	940463	61.88	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061116\
Data File : BF087925.D
Acq On : 12 Jun 2016 3:24
Operator : UM/SJ
Sample : PB91213BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91213BL

Quant Time: Jun 12 06:05:08 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

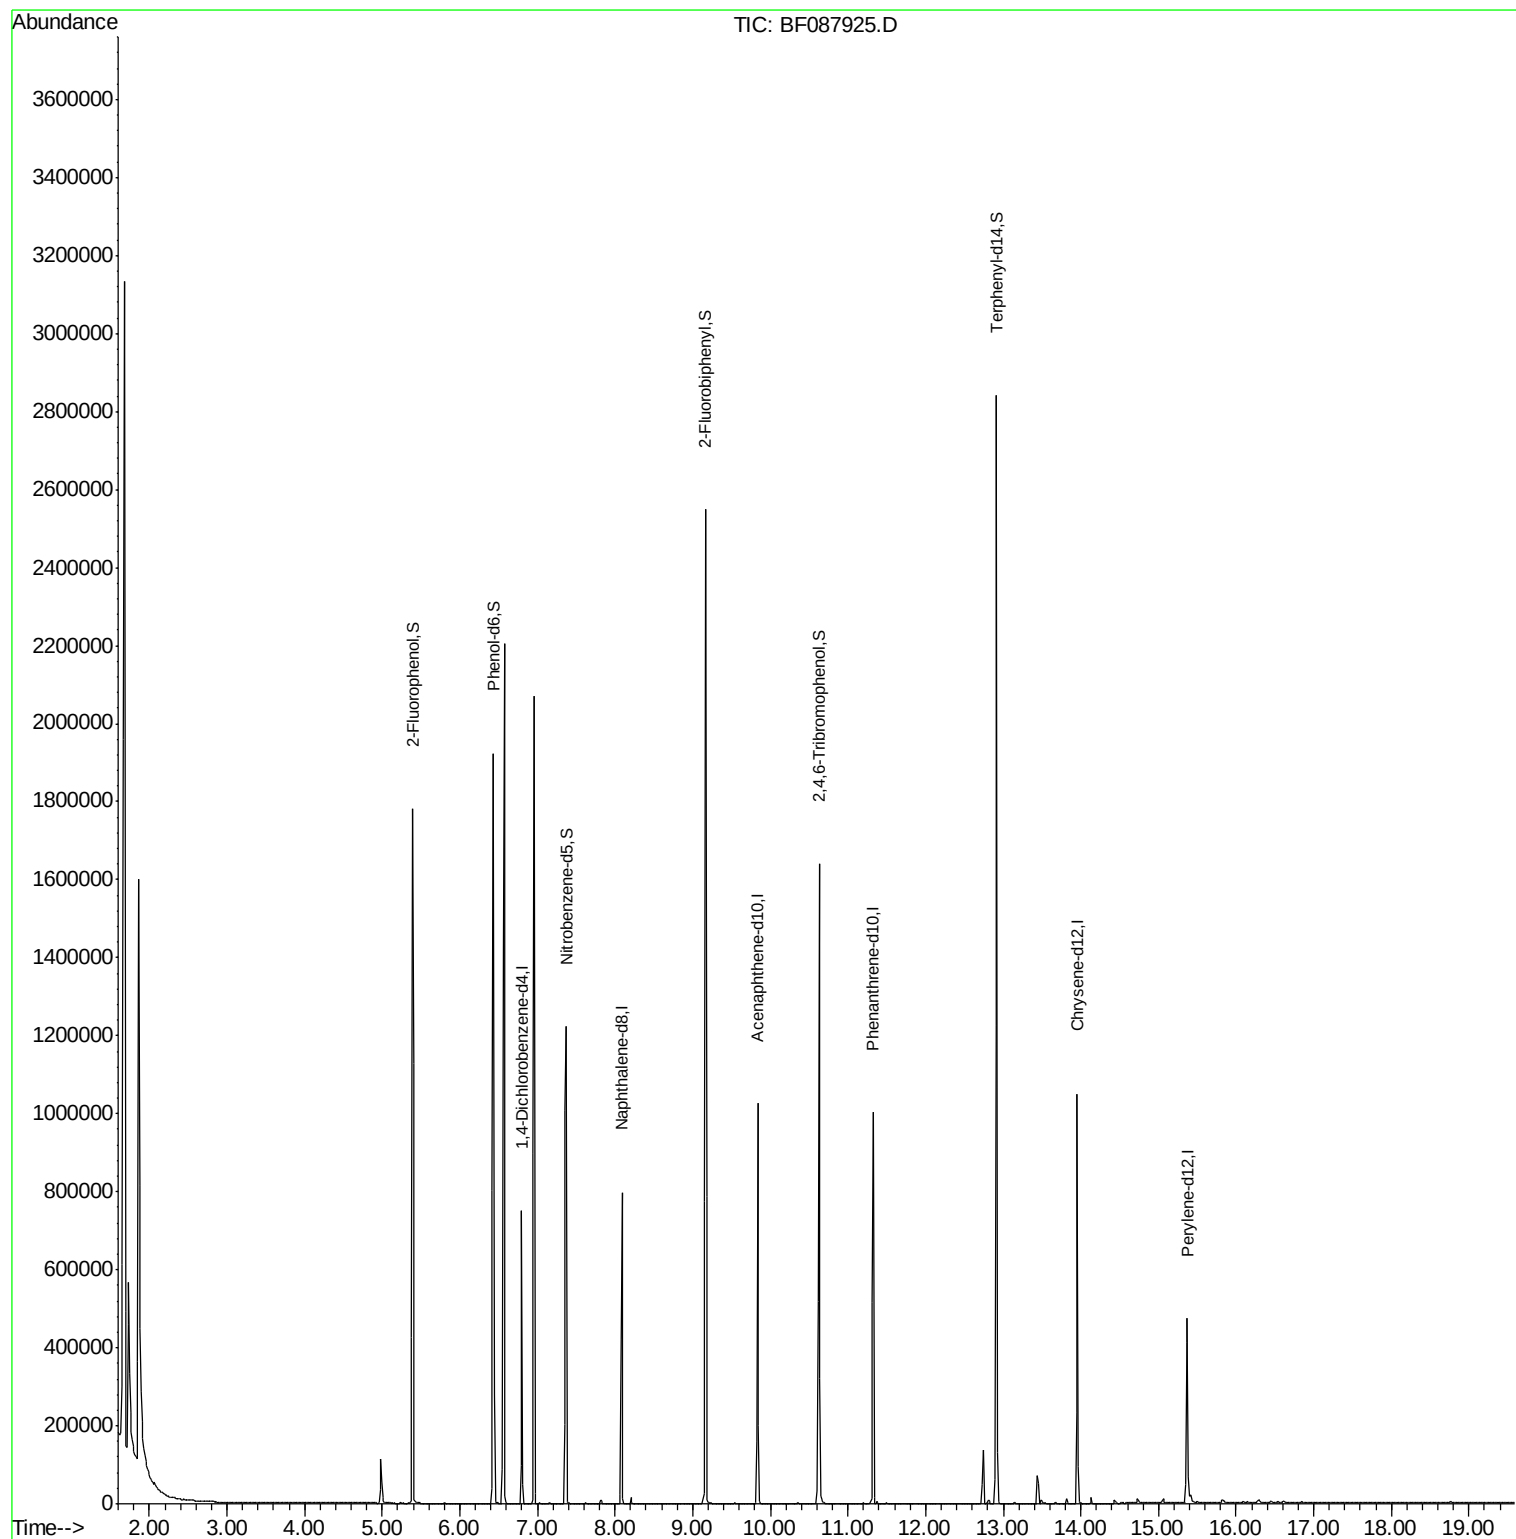

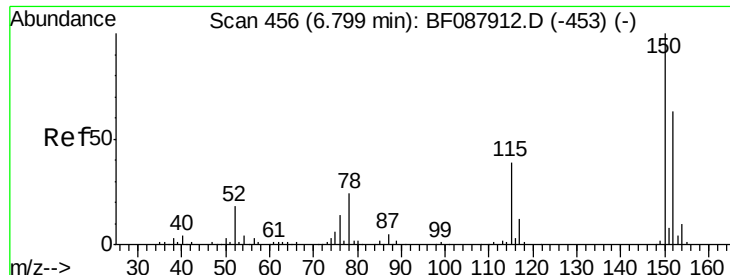

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.80 min Scan# 456

Delta R.T. -0.05 min

Lab File: BF087925.D

Acq: 12 Jun 2016 3:24

Instrument :

BNA_F

ClientSampled :

PB91213BL


Tot Ion:152 Resp: 108916

Ion Ratio Lower Upper

152 100

150 155.0 123.8 185.6




115 59.0 39.6 59.4

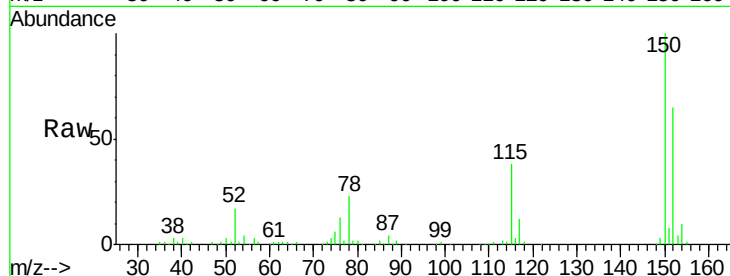

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

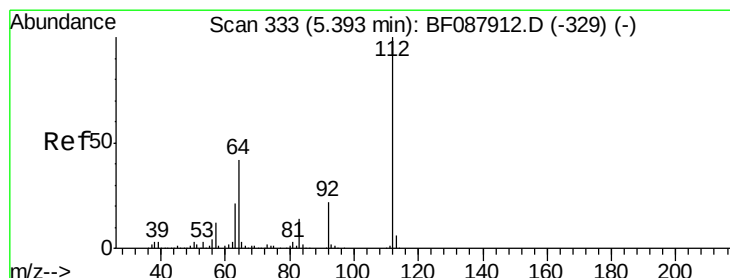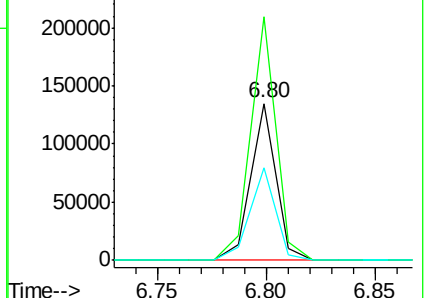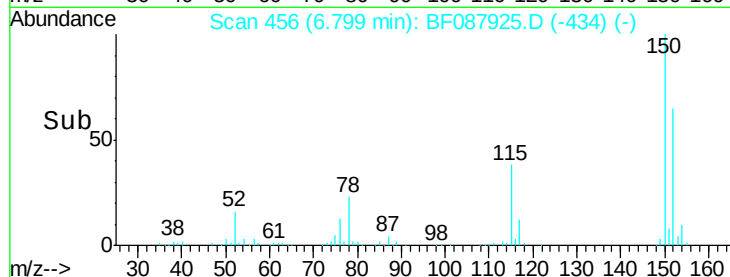

#5

2-Fluorophenol

Concen: 115.76 ng

RT: 5.39 min Scan# 333

Delta R.T. -0.03 min

Lab File: BF087925.D

Acq: 12 Jun 2016 3:24


Tgt Ion:112 Resp: 737530

Ion Ratio Lower Upper

112 100

64 57.5 42.2 63.2



63 29.3 21.8 32.8

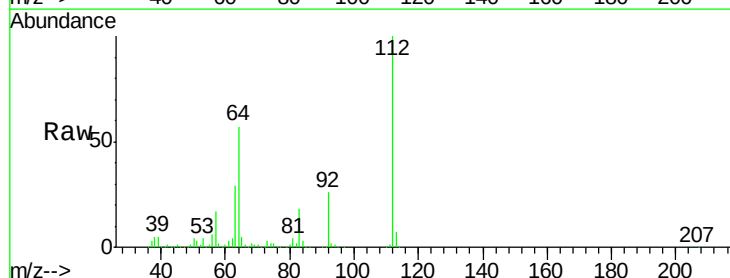


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

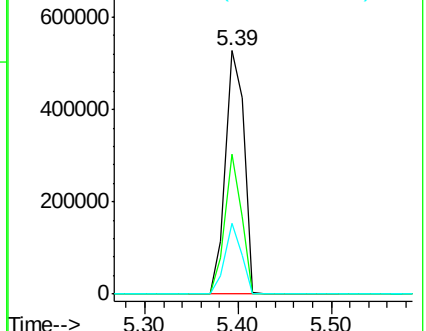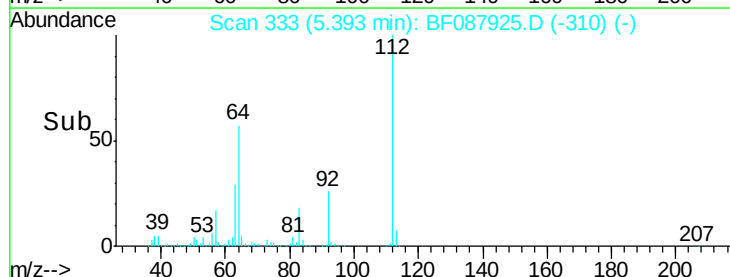

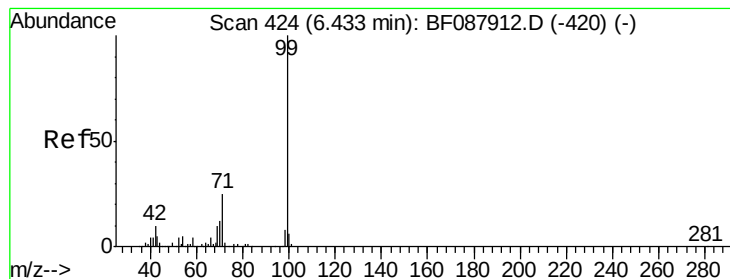

#7

Phenol-d6

Concen: 105.22 ng

RT: 6.43 min Scan# 424

Delta R.T. -0.05 min

Lab File: BF087925.D

Acq: 12 Jun 2016 3:24

Instrument :

BNA_F

ClientSampleId :

PB91213BL


Tot Ion: 99 Resp: 812431

Ion Ratio Lower Upper

99 100

42 16.0 12.2 18.2




71 32.8 23.4 35.0

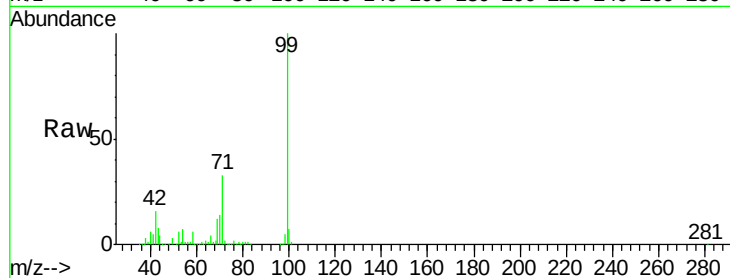

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

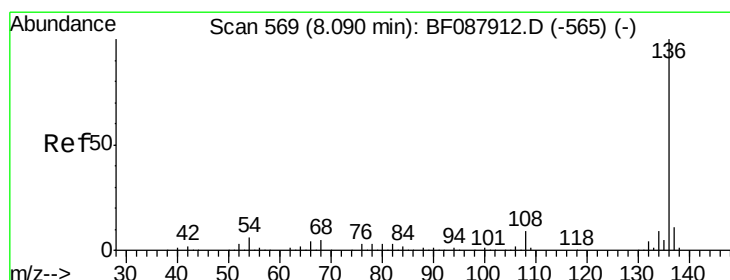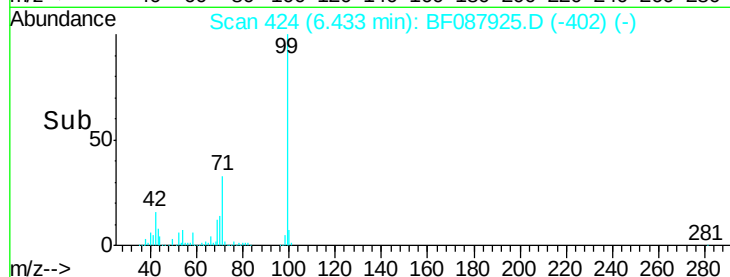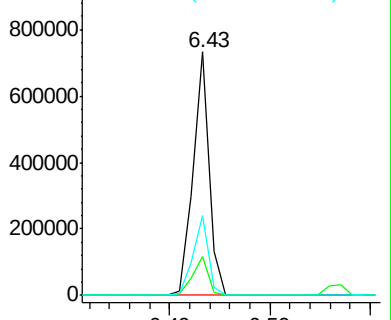

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.09 min Scan# 569

Delta R.T. -0.03 min

Lab File: BF087925.D

Acq: 12 Jun 2016 3:24

Tgt Ion: 136 Resp: 449339


Ion Ratio Lower Upper

136 100

137 10.8 9.1 13.7

54 5.5 6.6 10.0#

68 5.0 5.1 7.7#


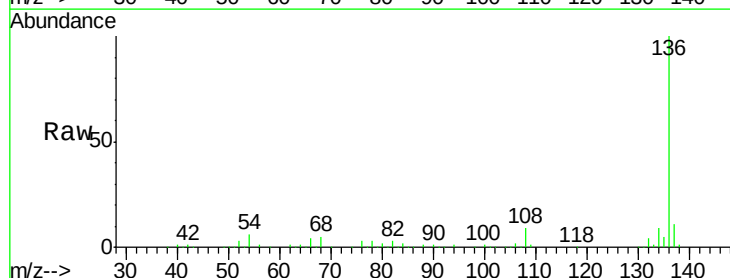



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



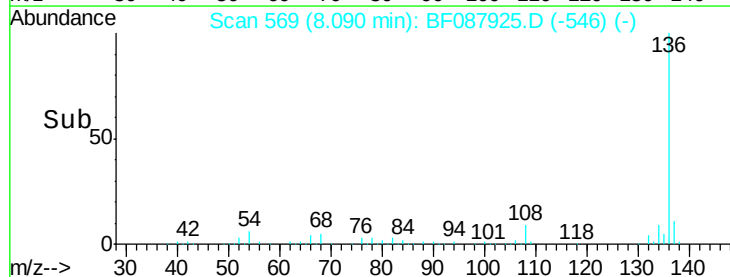
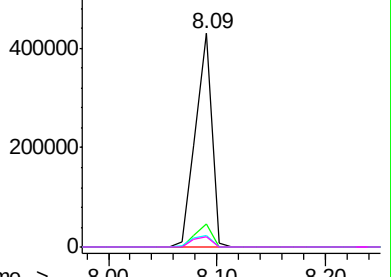


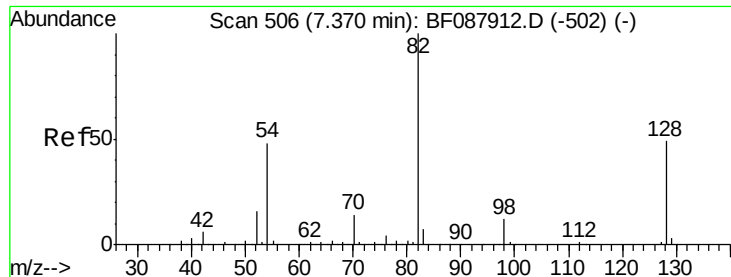

#23
 Nitrobenzene-d5
 Concen: 76.75 ng
 RT: 7.37 min Scan# 506
 Delta R.T. -0.05 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24




Instrument :
 BNA_F
 ClientSampleID :
 PB91213BL


Tot Ion	82	Resp	590563
Ion Ratio	100	Lower	Upper
128	56.4	35.9	53.9#
54	42.0	40.9	61.3

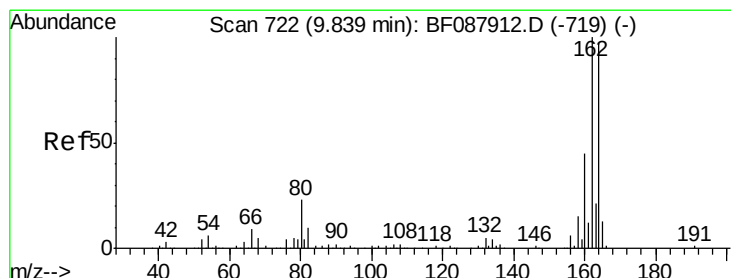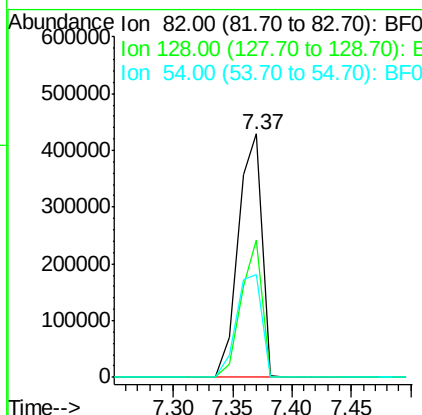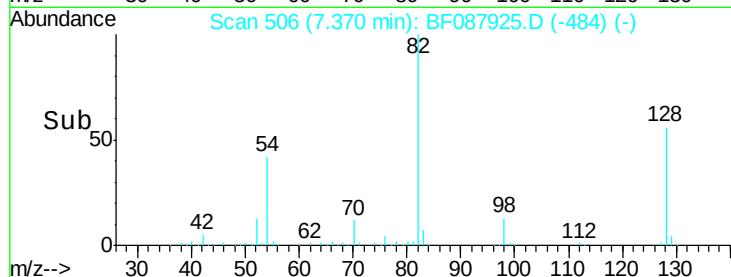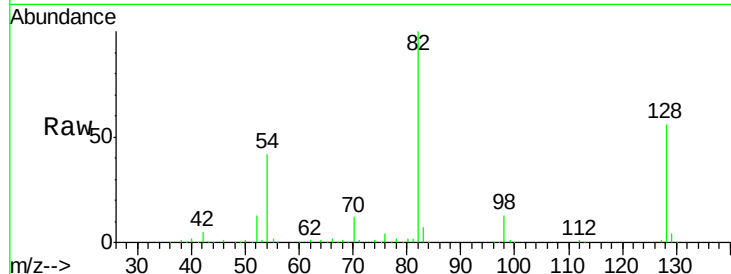

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.84 min Scan# 722
 Delta R.T. -0.05 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24

Tgt Ion	164	Resp	208256
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	104.1	85.4	128.2
160	46.7	39.5	59.3

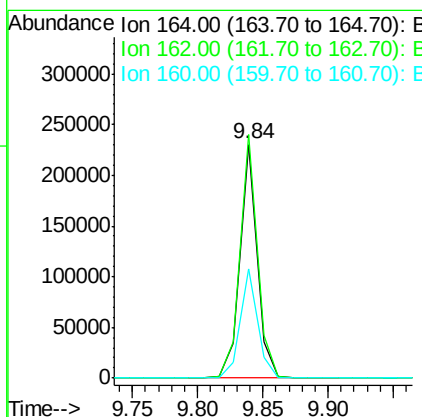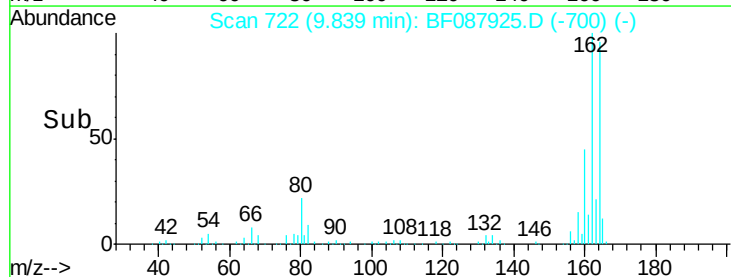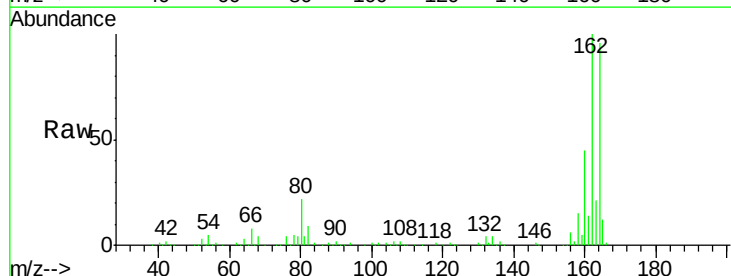


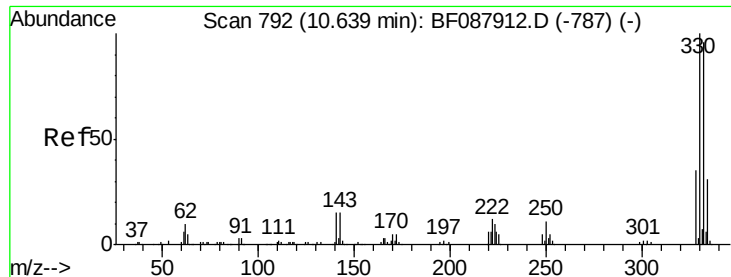




#41
 2,4,6-Tribromophenol
 Concen: 97.51 ng
 RT: 10.63 min Scan# 791
 Delta R.T. -0.05 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24

Instrument :
 BNA_F
 ClientSampleID :
 PB91213BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	0.0	0.0#
141	39.1	0.0	0.0#

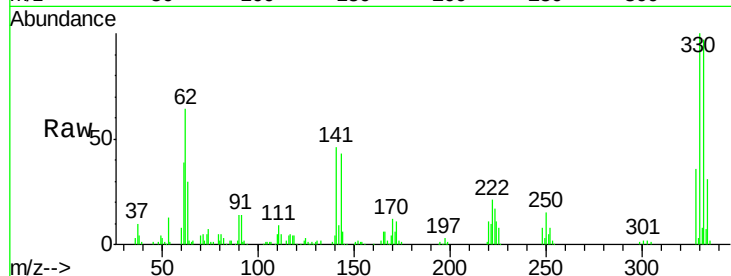


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

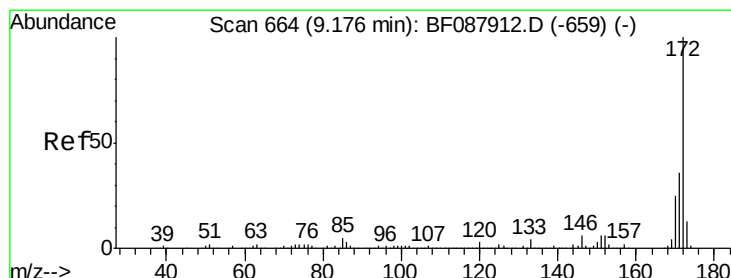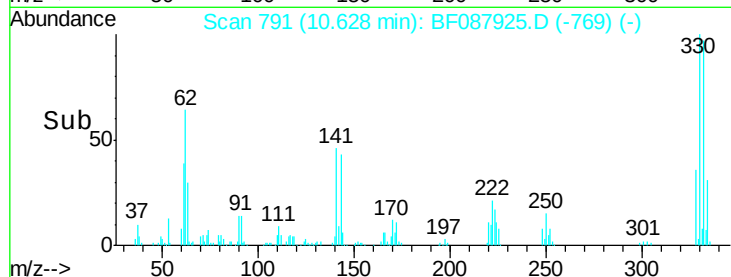
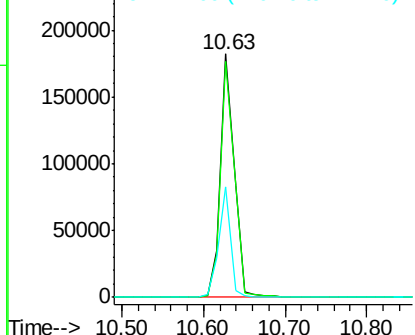



#44
 2-Fluorobiphenyl
 Concen: 74.87 ng
 RT: 9.16 min Scan# 663
 Delta R.T. -0.05 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.6	43.0
170	24.4	19.2	28.8

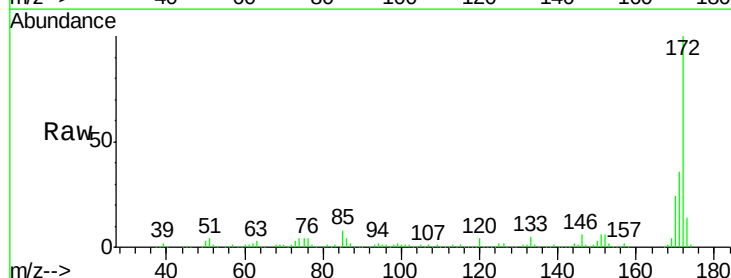

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

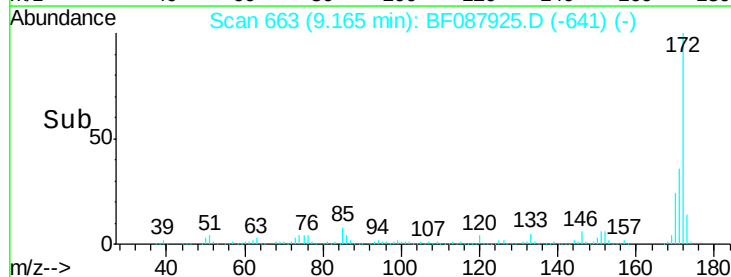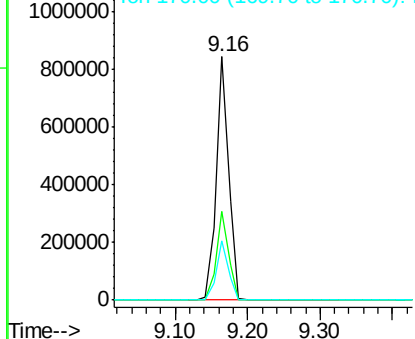


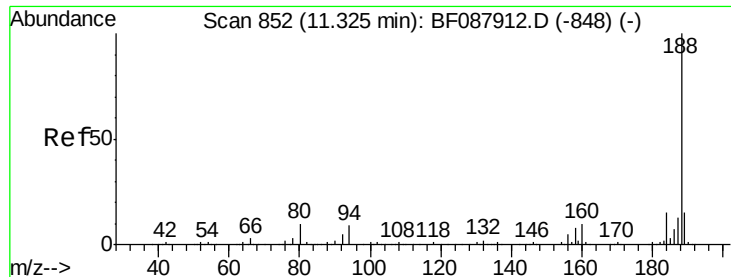




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.32 min Scan# 852
Delta R.T. -0.03 min
Lab File: BF087925.D
Acq: 12 Jun 2016 3:24

Instrument :
BNA_F
ClientSampleId :
PB91213BL

Tot Ion:188 Resp: 433340
Ion Ratio Lower Upper
188 100
94 7.2 9.0 13.6#
80 7.3 10.0 15.0#

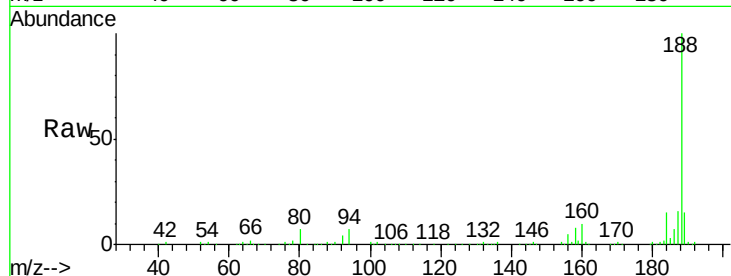


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

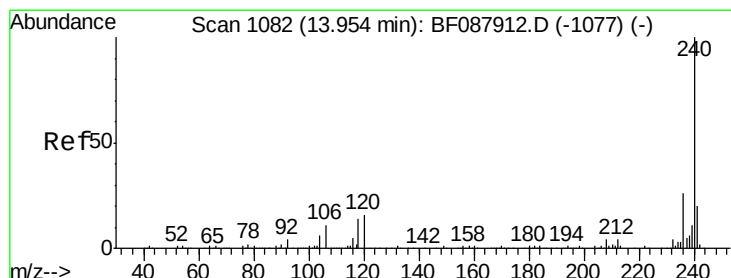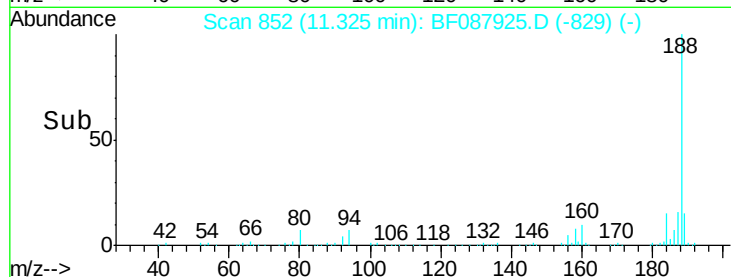
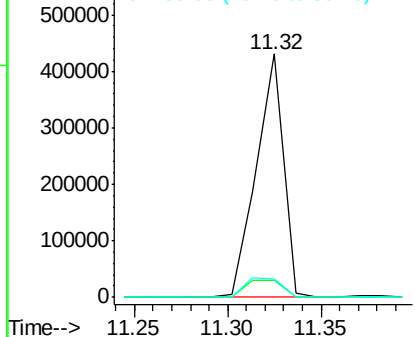



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.95 min Scan# 1082
Delta R.T. -0.03 min
Lab File: BF087925.D
Acq: 12 Jun 2016 3:24

Tgt Ion:240 Resp: 345868
Ion Ratio Lower Upper
240 100
120 12.8 6.8 10.2#
236 25.9 20.2 30.2

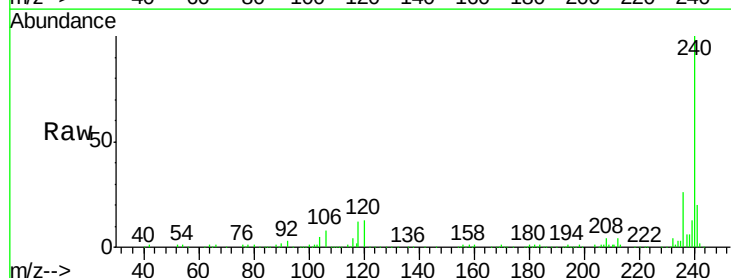

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



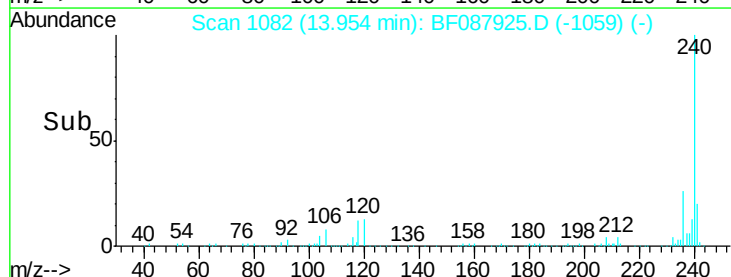
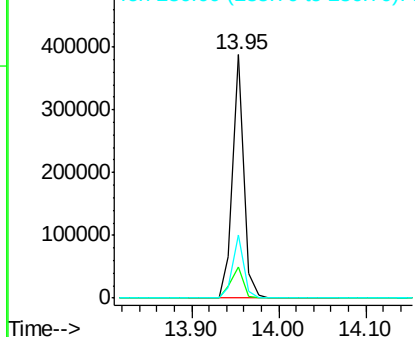


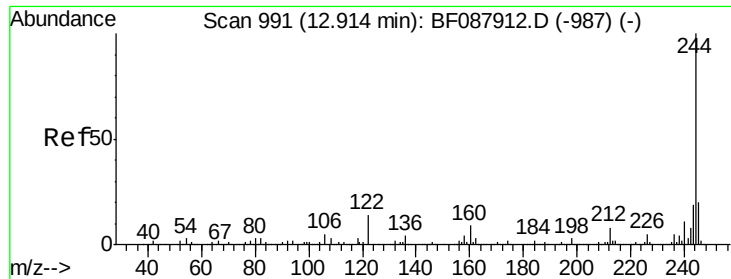

#78
 Terphenyl-d14
 Concen: 61.88 ng
 RT: 12.91 min Scan# 991
 Delta R.T. -0.03 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24

Instrument :
 BNA_F
 ClientSampleId :
 PB91213BL

Tot Ion:244 Resp: 940463
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.0 9.0
 122 12.8 11.2 16.8

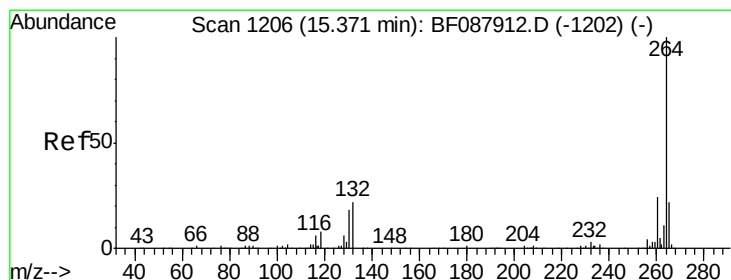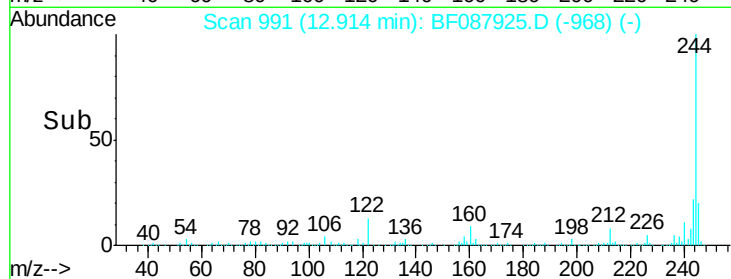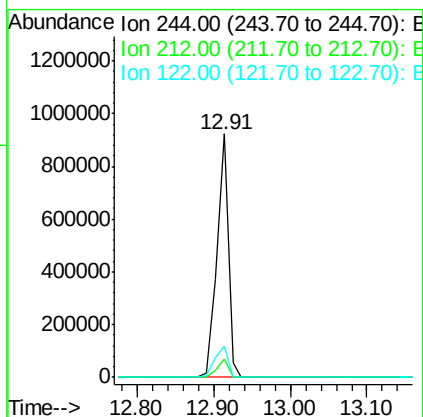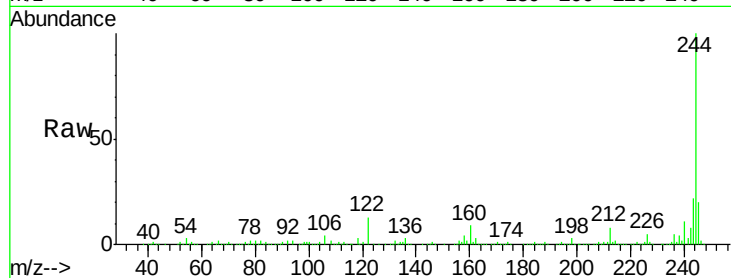

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.37 min Scan# 1206
 Delta R.T. -0.02 min
 Lab File: BF087925.D
 Acq: 12 Jun 2016 3:24

Tgt Ion:264 Resp: 263859
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.2 28.8
 265 20.9 16.9 25.3

