


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF061116\  
 Data File : BF087899.D  
 Acq On : 11 Jun 2016 13:42  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 13 14:10:49 2016

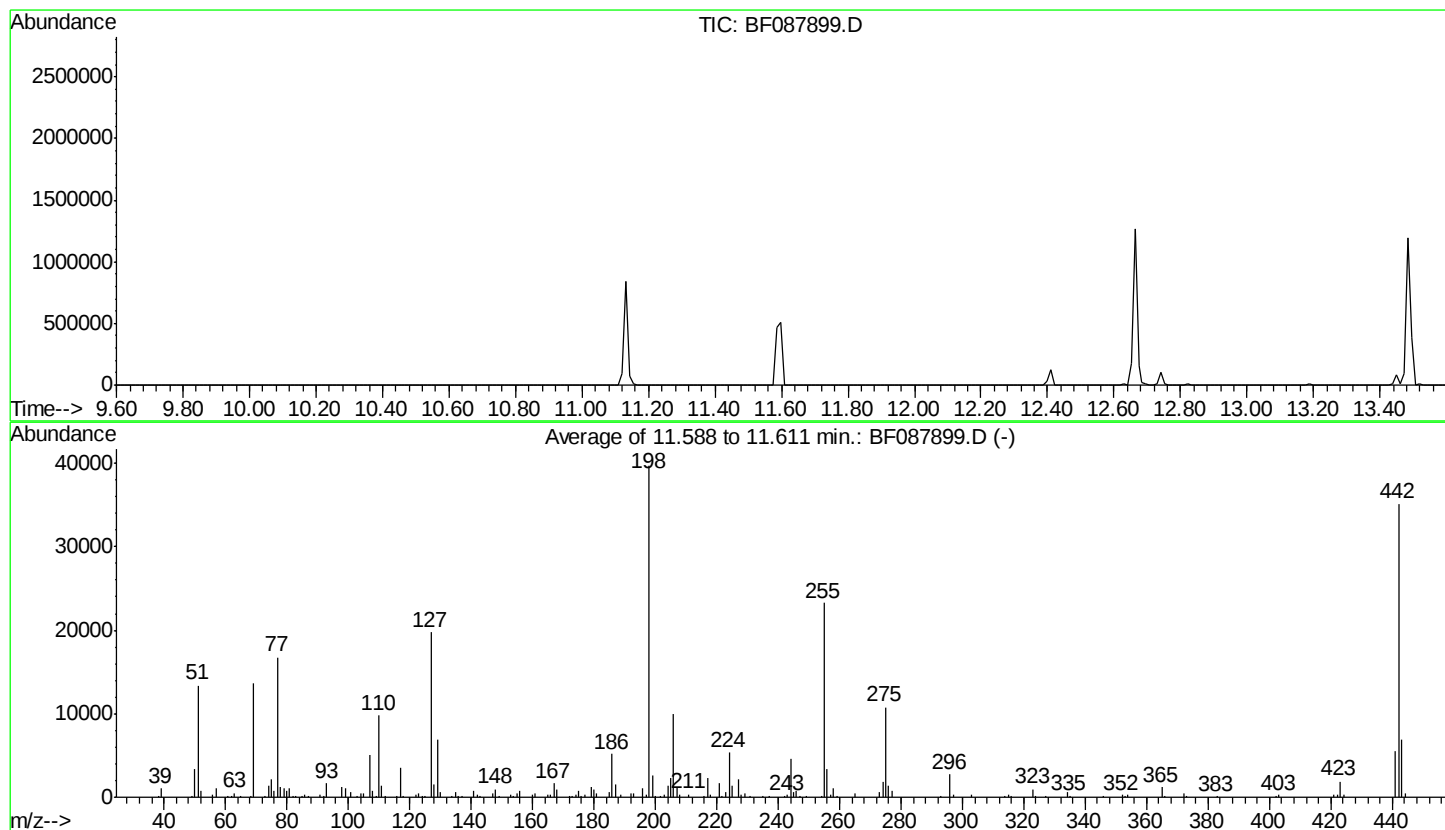

AutoFind: Scans 875, 876, 877; Background Corrected with Scan 871

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.6      | 13340   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 181     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.4      | 13672   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 49.7      | 19749   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.8       | 308     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 39714   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 2652    | PASS             |
| 275         | 198          | 10           | 60           | 27.1      | 10768   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 1221    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.8      | 5550    | PASS             |
| 442         | 198          | 50           | 100          | 88.5      | 35136   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 6852    | PASS             |