
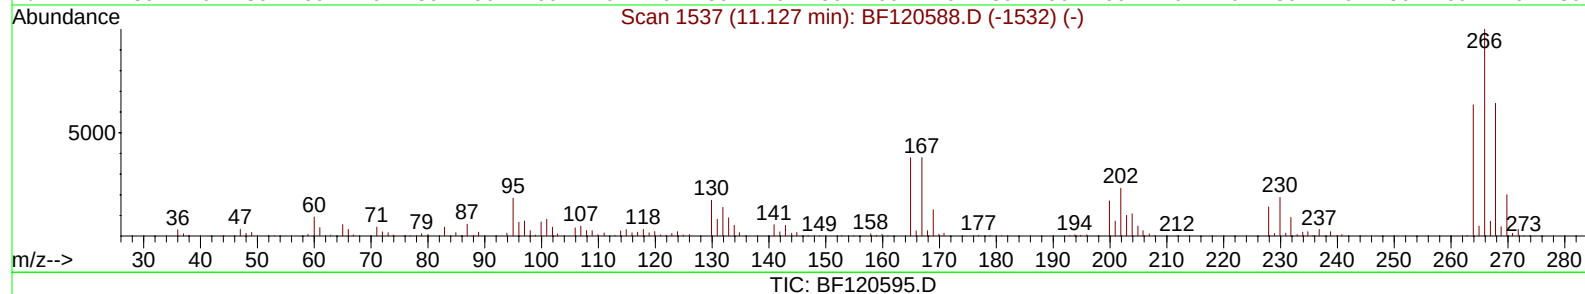
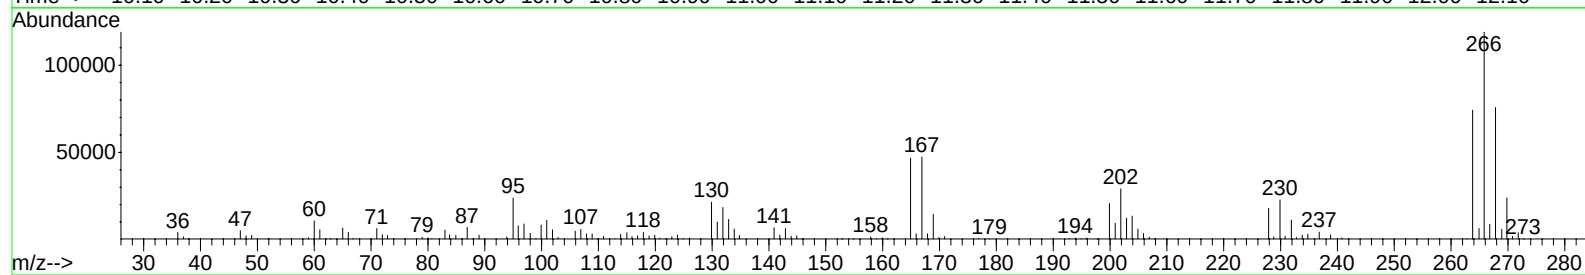


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061120\
 Data File : BF120595.D
 Acq On : 11 Jun 2020 8:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 17:57:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

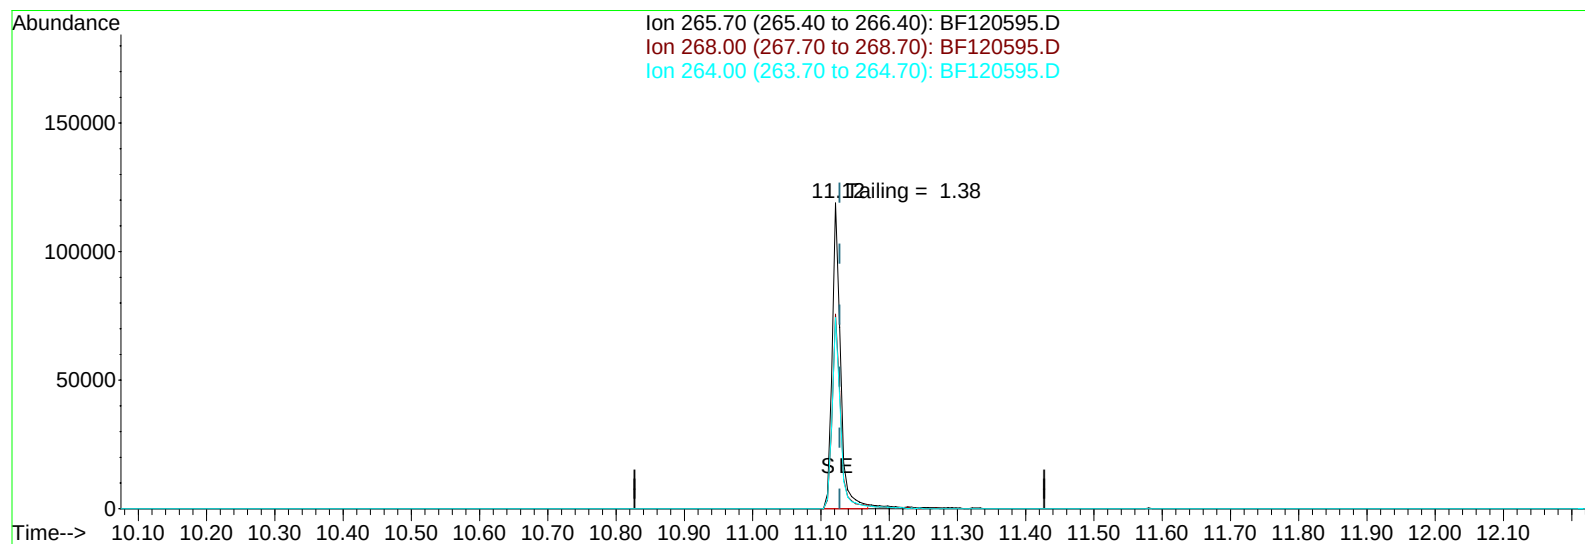

(70) Pentachlorophenol (C)




11.121min (-0.006) 126931.22ng

response 103331

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	63.61
264.00	63.50	62.40
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061120\
 Data File : BF120595.D
 Acq On : 11 Jun 2020 8:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 17:57:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

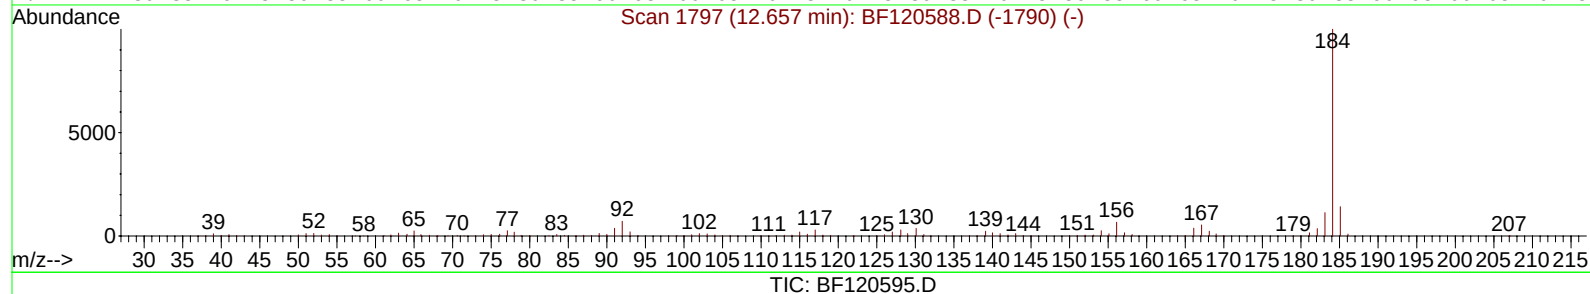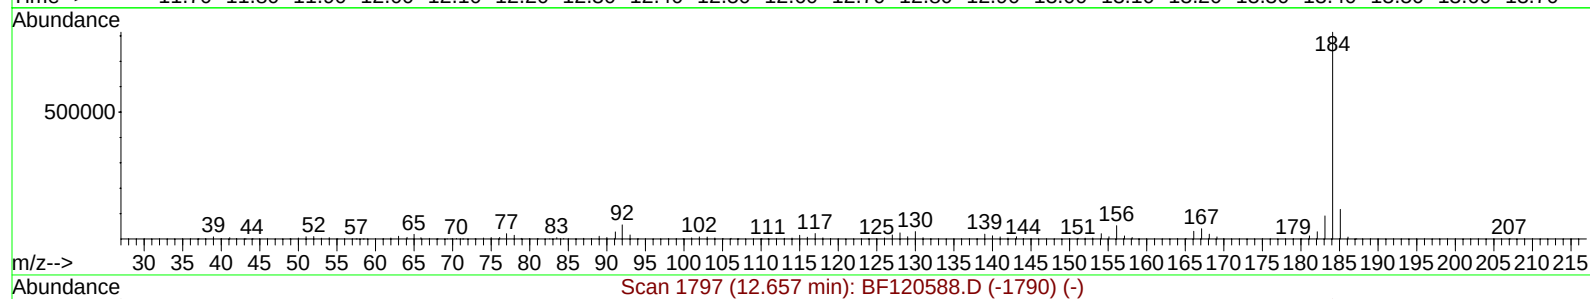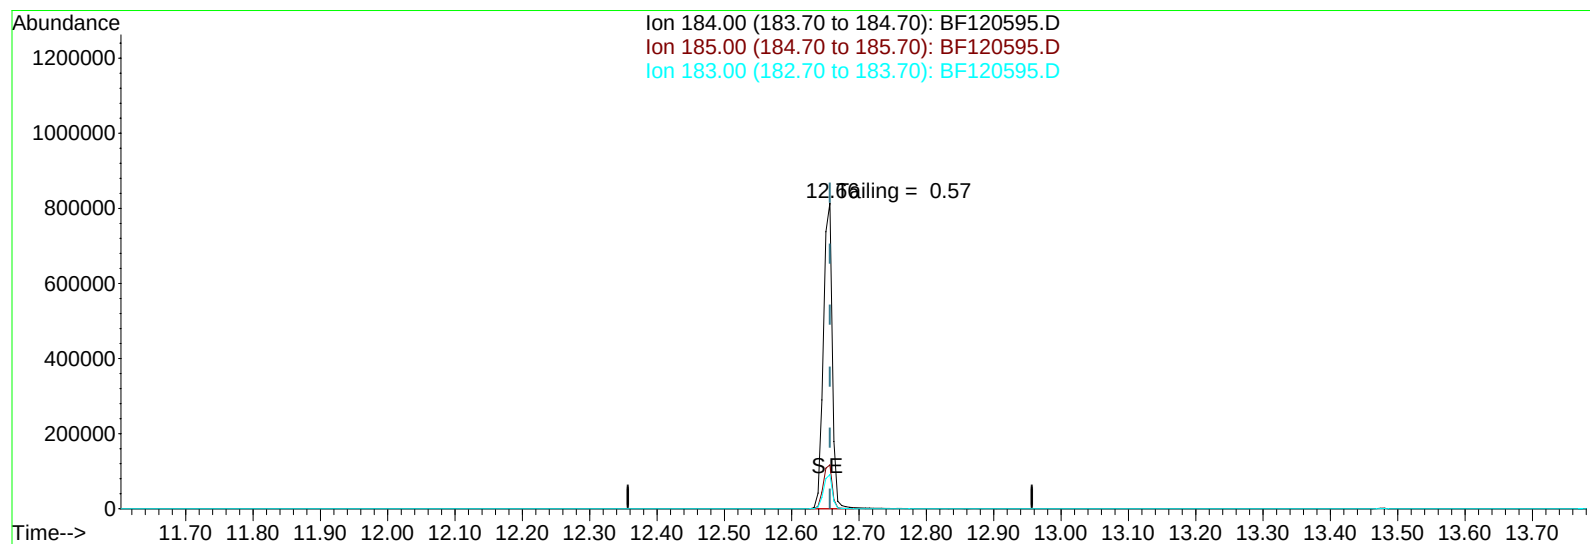

(77) Benzidine

12.657min (+0.000) 3474.41ng

response 750018

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.34
183.00	11.30	11.16
0.00	0.00	0.00