

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061120\  
 Data File : BF120598.D  
 Acq On : 11 Jun 2020 12:59  
 Operator : JU/CG  
 Sample : PB129457BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB129457BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.410       | 560           | 565         | 568          | rBV      | 3665929        | 3543386       | 76.65%          | 11.426%       |
| 2         | 6.434       | 733           | 739         | 742          | rBV      | 3504283        | 3593621       | 77.73%          | 11.588%       |
| 3         | 6.798       | 797           | 801         | 805          | rBV      | 1122817        | 864650        | 18.70%          | 2.788%        |
| 4         | 6.957       | 824           | 828         | 831          | rBV      | 3666069        | 3146174       | 68.06%          | 10.145%       |
| 5         | 7.363       | 892           | 897         | 900          | rBV      | 2704675        | 2485043       | 53.75%          | 8.013%        |
| 6         | 8.081       | 1015          | 1019        | 1022         | rBV      | 1421810        | 1120234       | 24.23%          | 3.612%        |
| 7         | 9.157       | 1198          | 1202        | 1205         | rBV      | 4881877        | 4622936       | 100.00%         | 14.907%       |
| 8         | 9.833       | 1313          | 1317        | 1320         | rBV      | 1624546        | 1314098       | 28.43%          | 4.237%        |
| 9         | 10.622      | 1447          | 1451        | 1455         | rBV      | 2845263        | 2839486       | 61.42%          | 9.156%        |
| 10        | 11.316      | 1566          | 1569        | 1573         | rBV      | 1010688        | 919684        | 19.89%          | 2.966%        |
| 11        | 12.910      | 1835          | 1840        | 1843         | rBV      | 3768921        | 3732761       | 80.74%          | 12.037%       |
| 12        | 13.957      | 2014          | 2018        | 2021         | rVB      | 1310272        | 1239446       | 26.81%          | 3.997%        |
| 13        | 14.733      | 2146          | 2150        | 2154         | rBV      | 47012          | 49373         | 1.07%           | 0.159%        |
| 14        | 15.062      | 2202          | 2206        | 2212         | rBV      | 52372          | 62359         | 1.35%           | 0.201%        |
| 15        | 15.398      | 2257          | 2263        | 2267         | rBV      | 1041149        | 1300383       | 28.13%          | 4.193%        |
| 16        | 15.427      | 2267          | 2268        | 2275         | rVB      | 58793          | 56248         | 1.22%           | 0.181%        |
| 17        | 15.851      | 2335          | 2340        | 2344         | rBV      | 45291          | 64857         | 1.40%           | 0.209%        |
| 18        | 16.345      | 2417          | 2424        | 2430         | rBV2     | 30199          | 57164         | 1.24%           | 0.184%        |


Sum of corrected areas: 31011903

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061120\  
Data File : BF120598.D  
Acq On : 11 Jun 2020 12:59  
Operator : JU/CG  
Sample : PB129457BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

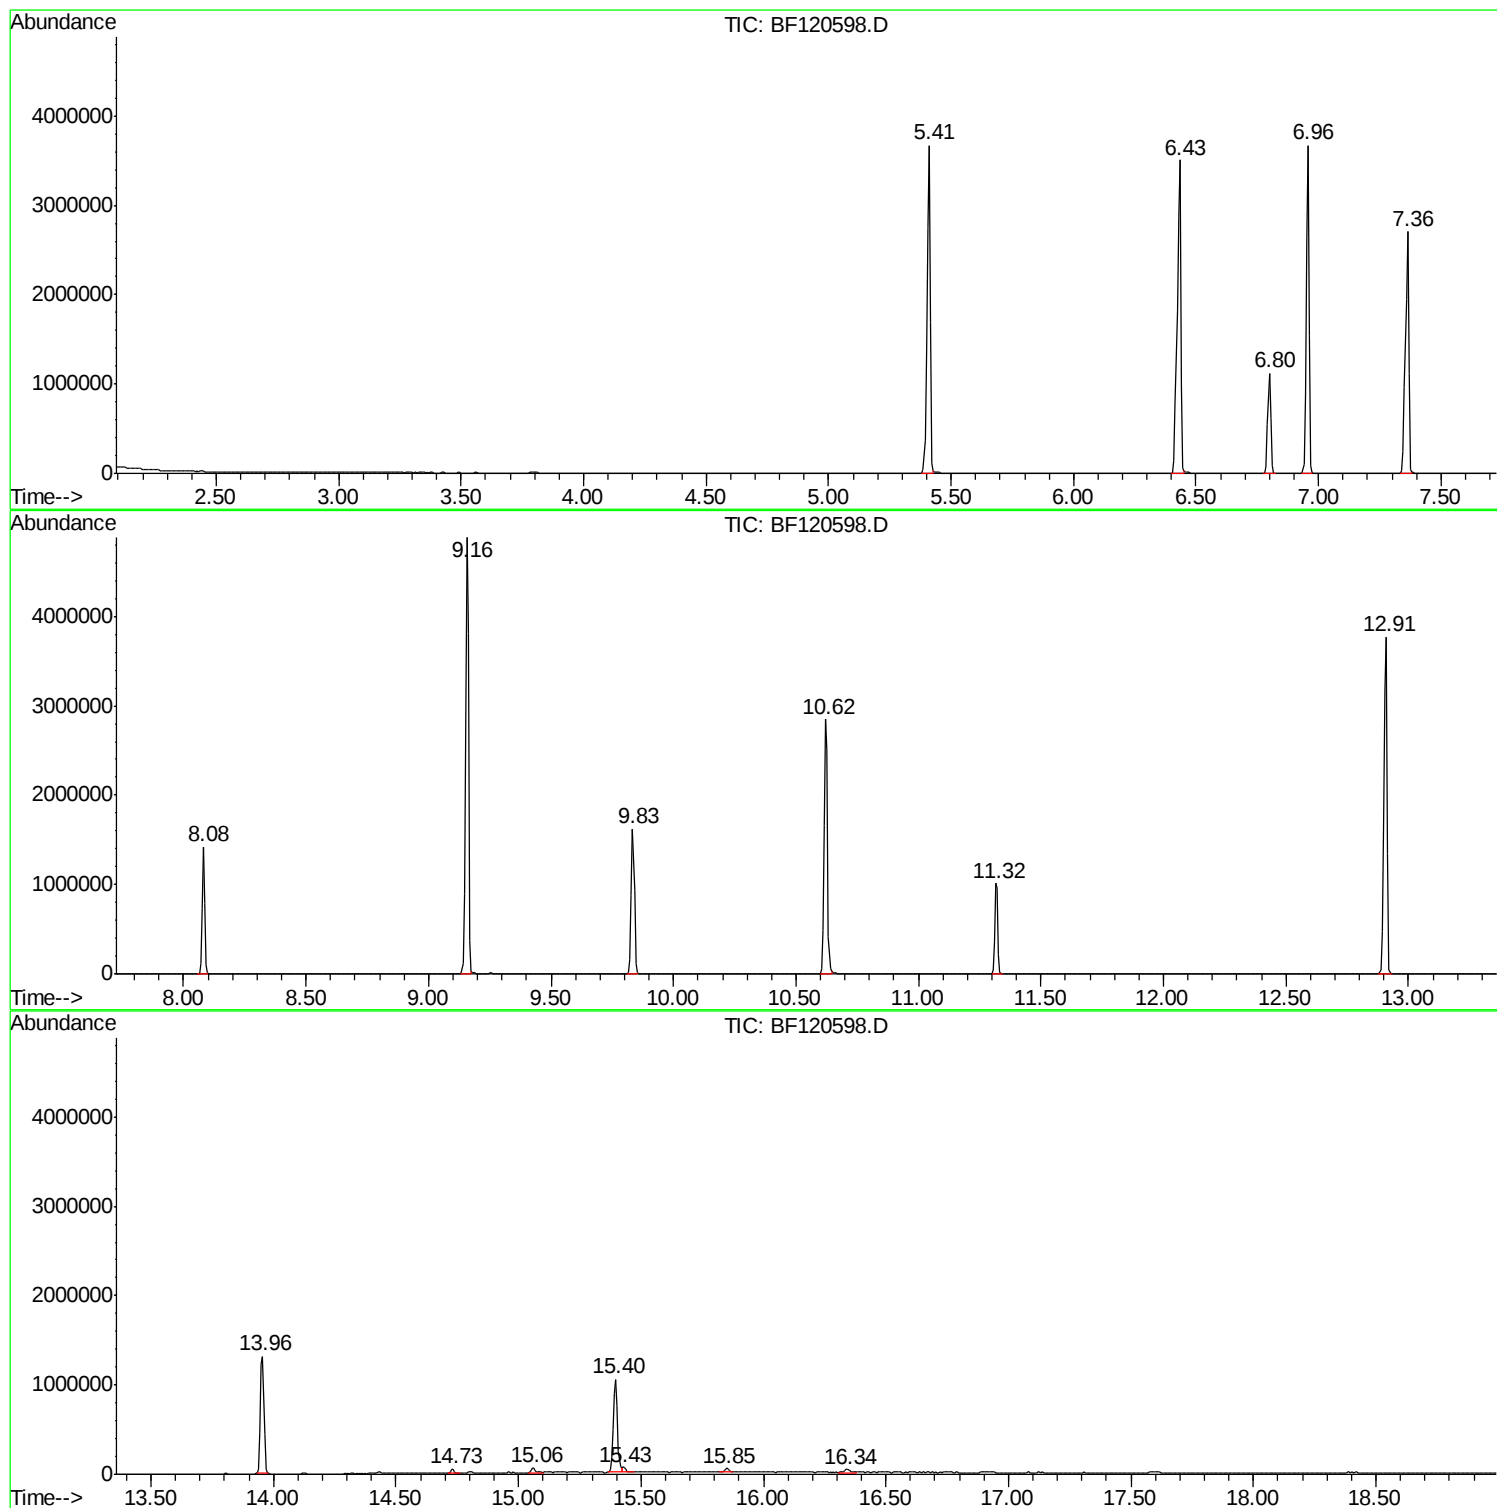

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061120\  
Data File : BF120598.D  
Acq On : 11 Jun 2020 12:59  
Operator : JU/CG  
Sample : PB129457BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061120\  
Data File : BF120598.D  
Acq On : 11 Jun 2020 12:59  
Operator : JU/CG  
Sample : PB129457BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |