
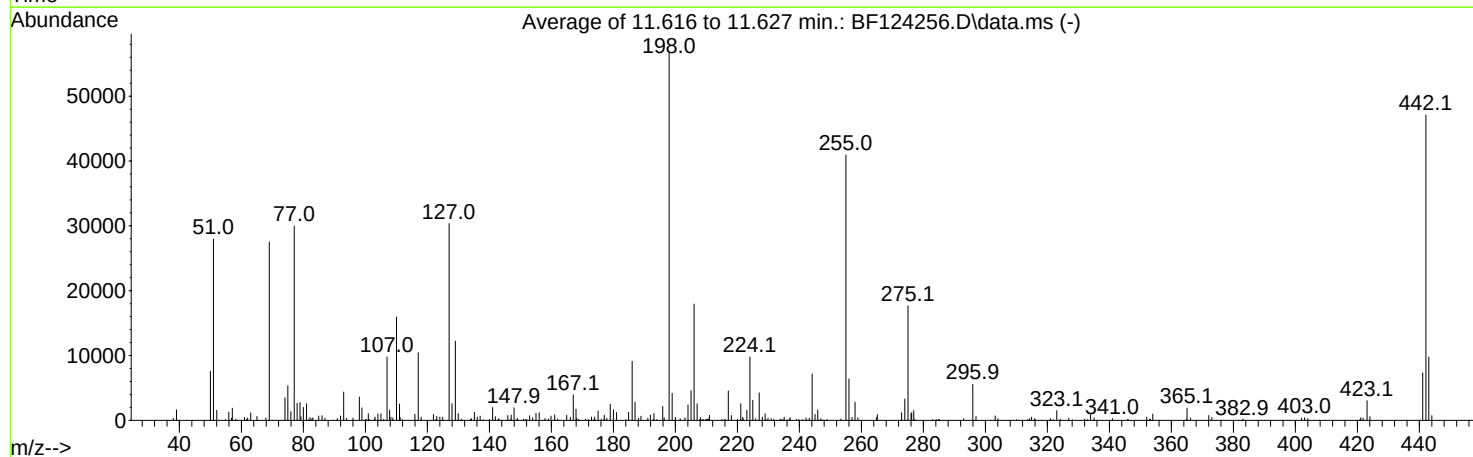


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061121\
 Data File : BF124256.D
 Acq On : 11 Jun 2021 11:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 10 01:53:56 2021

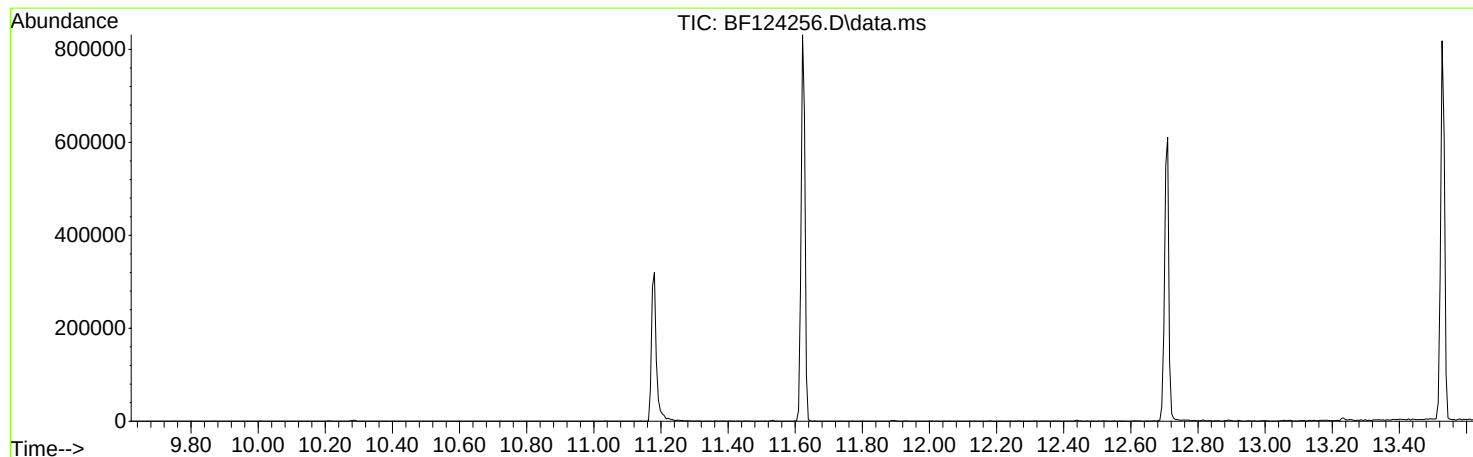

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	27968	PASS
68	69	0.00	2	1.4	377	PASS
69	198	0.00	100	48.5	27525	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	30355	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56736	PASS
199	198	5	9	7.3	4163	PASS
275	198	10	60	31.2	17683	PASS
365	198	1	100	3.4	1913	PASS
441	198	0.01	100	12.9	7312	PASS
442	442	50	100	100.0	47084	PASS
443	442	15	24	20.8	9777	PASS


	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
6/11/2021	BNA_F	<u>BF124256.D</u>
Compound Name	Response	Retention Time
DDT	118311	13.52
DDD	2650	13.22
DDE	0	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2650	120961	2.19

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061121\
Data File : BF124256.D
Acq On : 11 Jun 2021 11:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 13:55:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

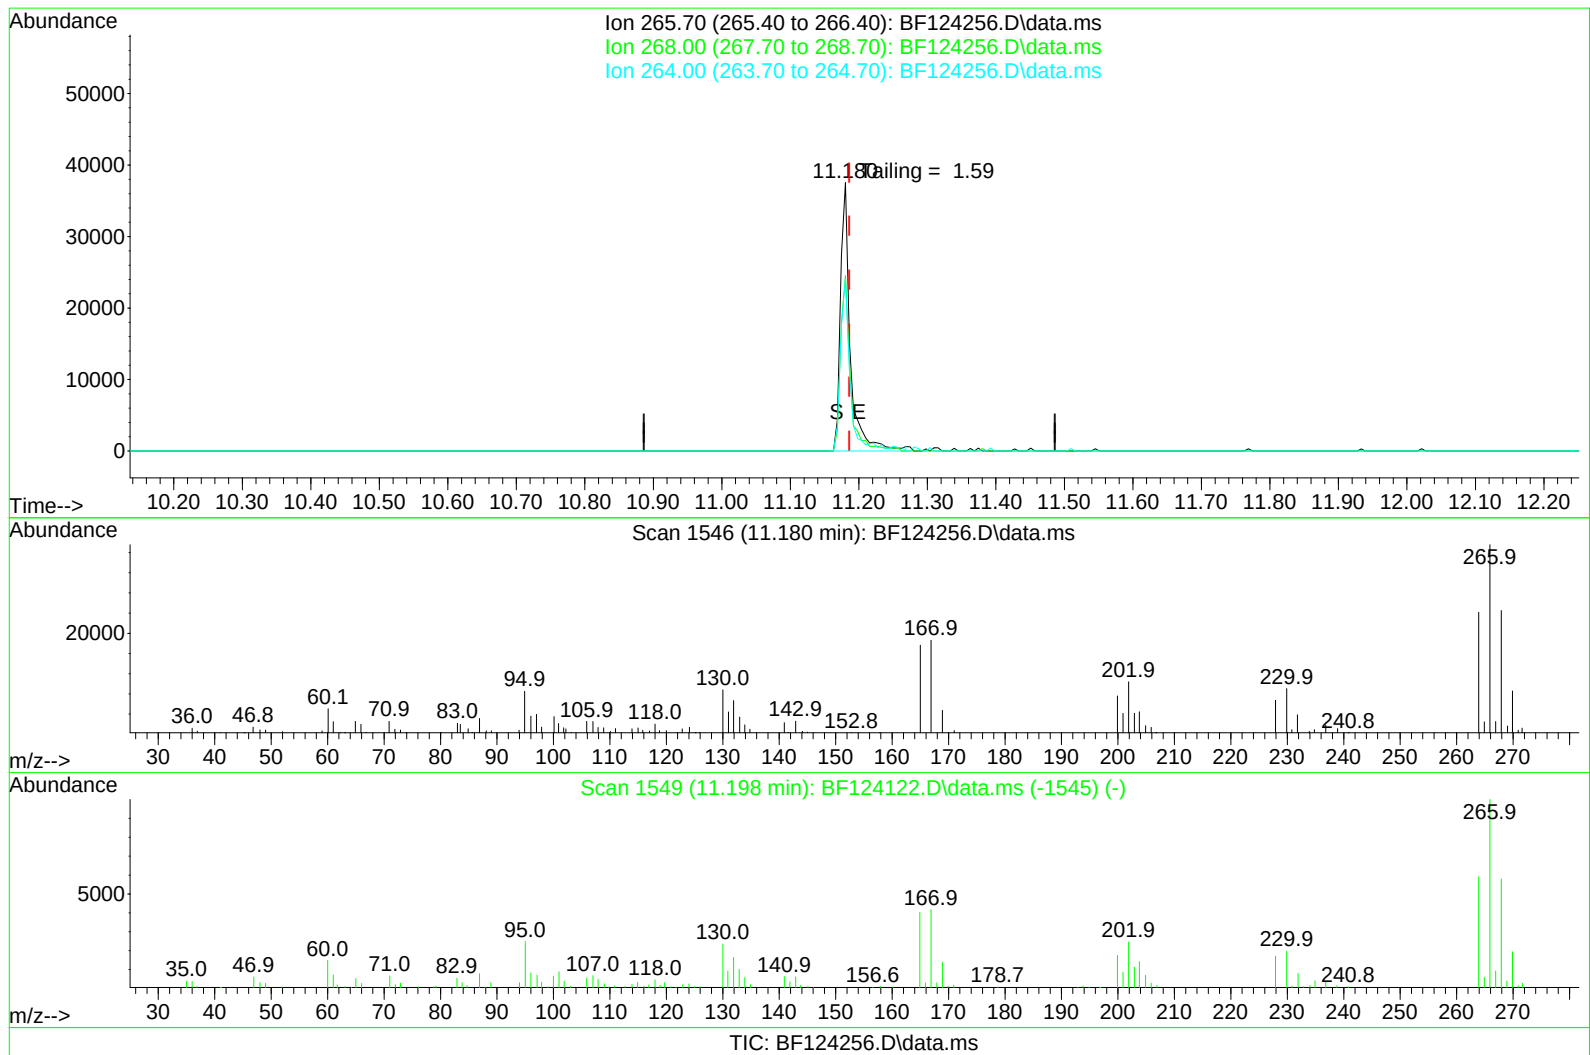

(70) Pentachlorophenol (C)

11.180min (-0.006) 11488.64 ng




response 37265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.29
264.00	65.70	64.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061121\
 Data File : BF124256.D
 Acq On : 11 Jun 2021 11:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 11 13:55:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

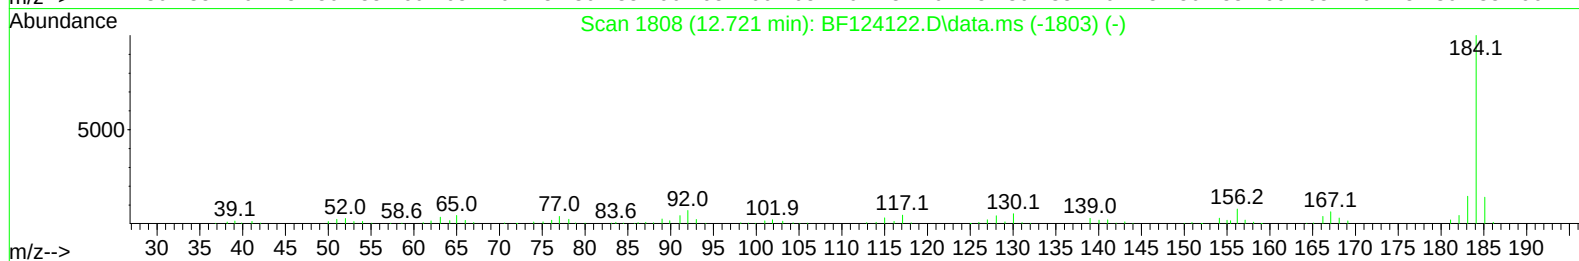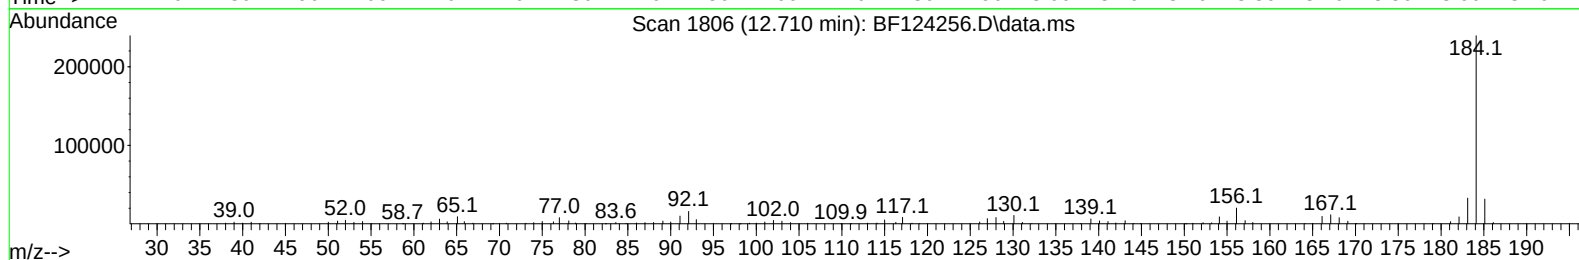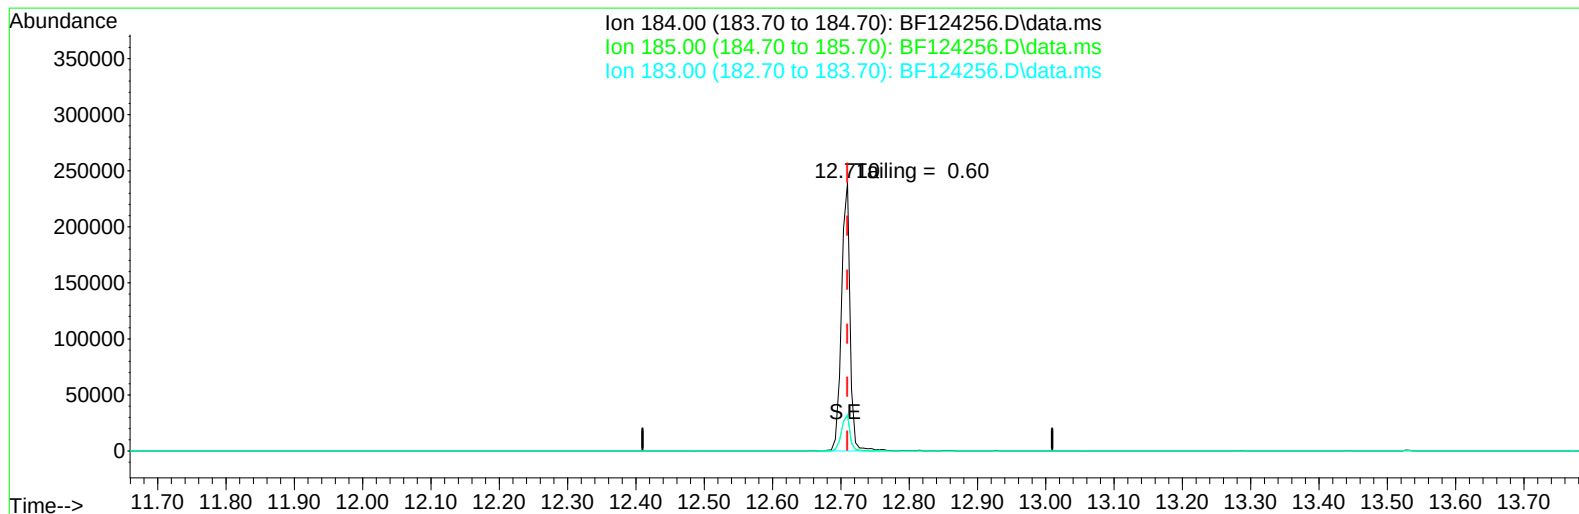

TIC: BF124256.D\data.ms

(77) Benzidine

12.710min (+ 0.000) 0.00 ng

response 209116

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.23
183.00	9.80	13.73#
0.00	0.00	0.00