
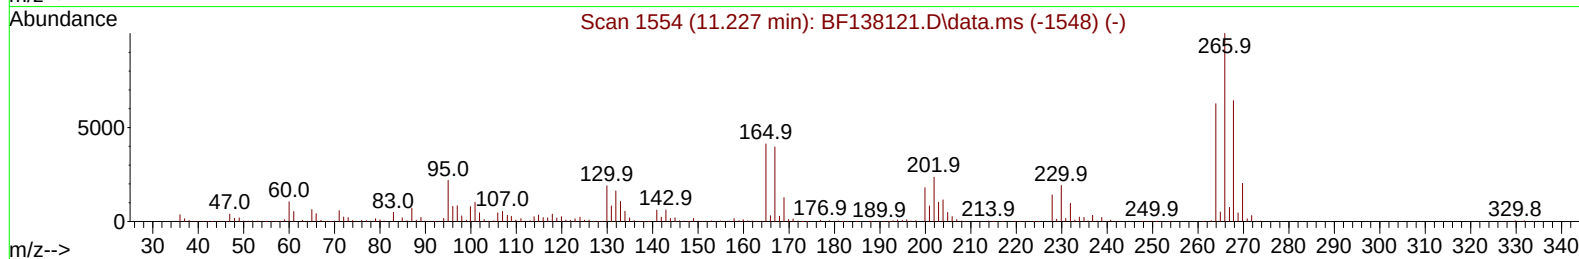
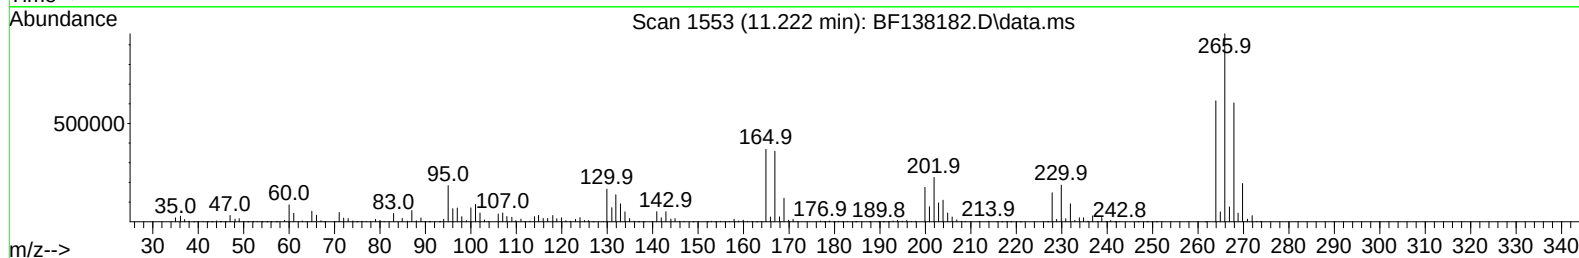


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138182.D
Acq On : 11 Jun 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 11:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

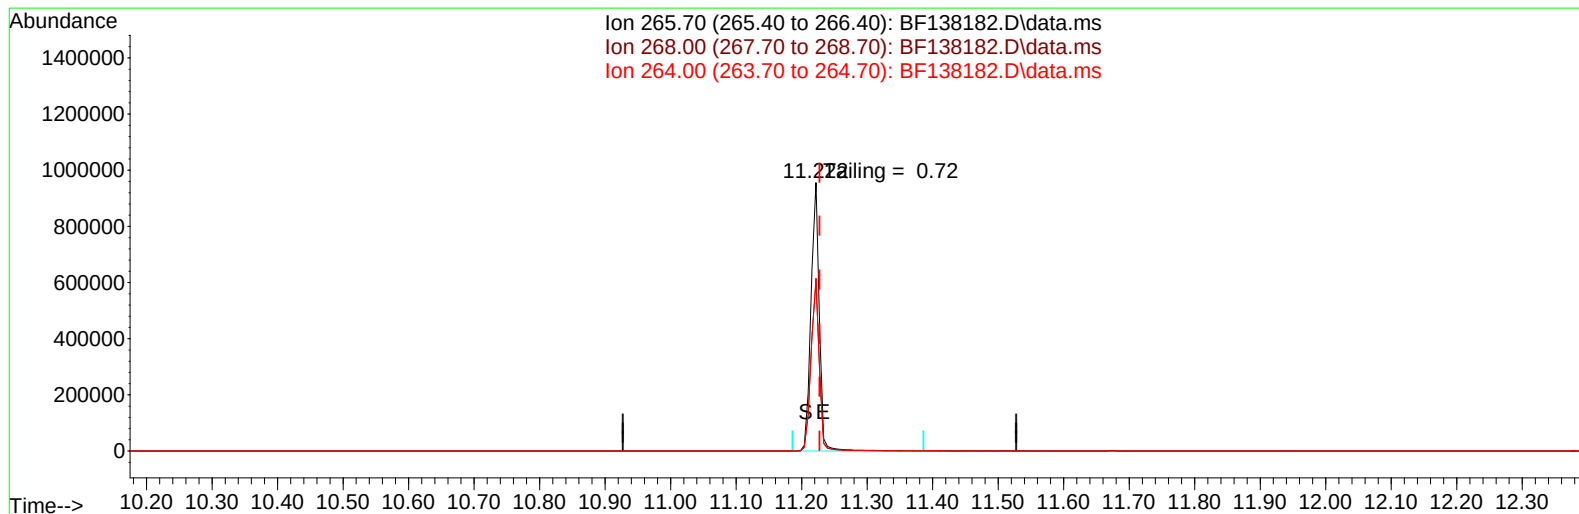

TIC: BF138182.D\data.ms




(70) Pentachlorophenol (C)

11.222min (-0.006) 750653.71 ng

response 840427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.23
264.00	62.60	64.35
0.00	0.00	0.00

Quant Time: Jun 11 11:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

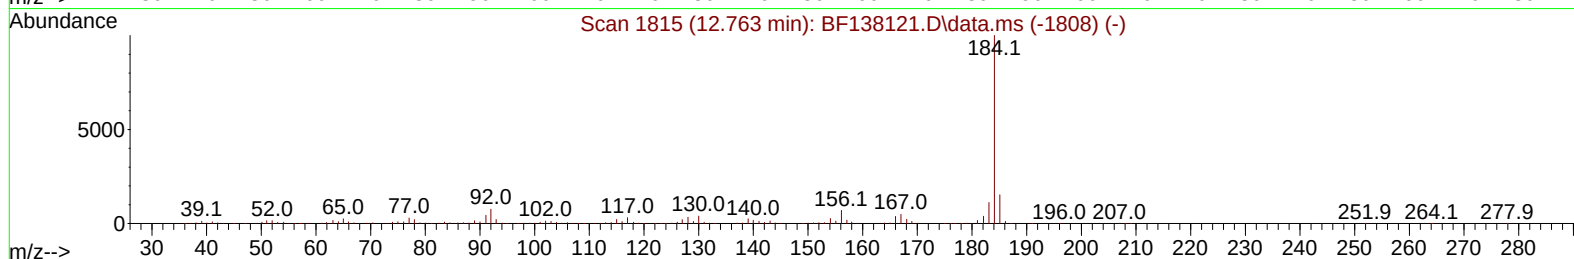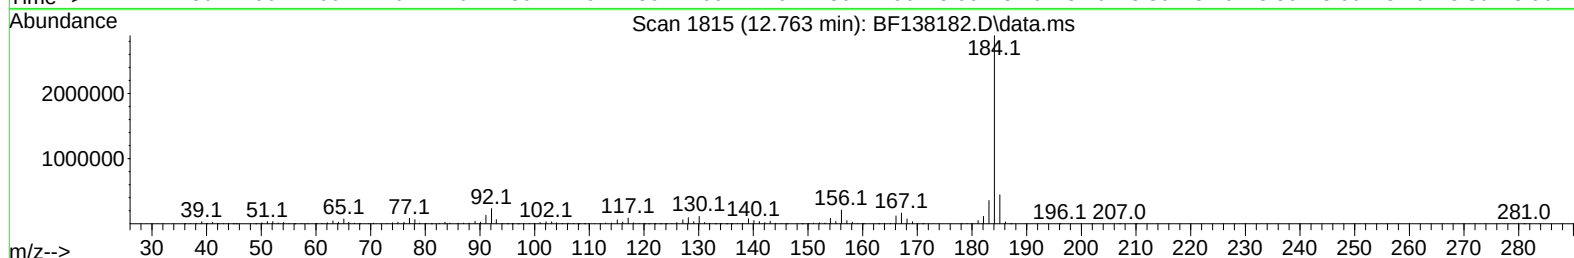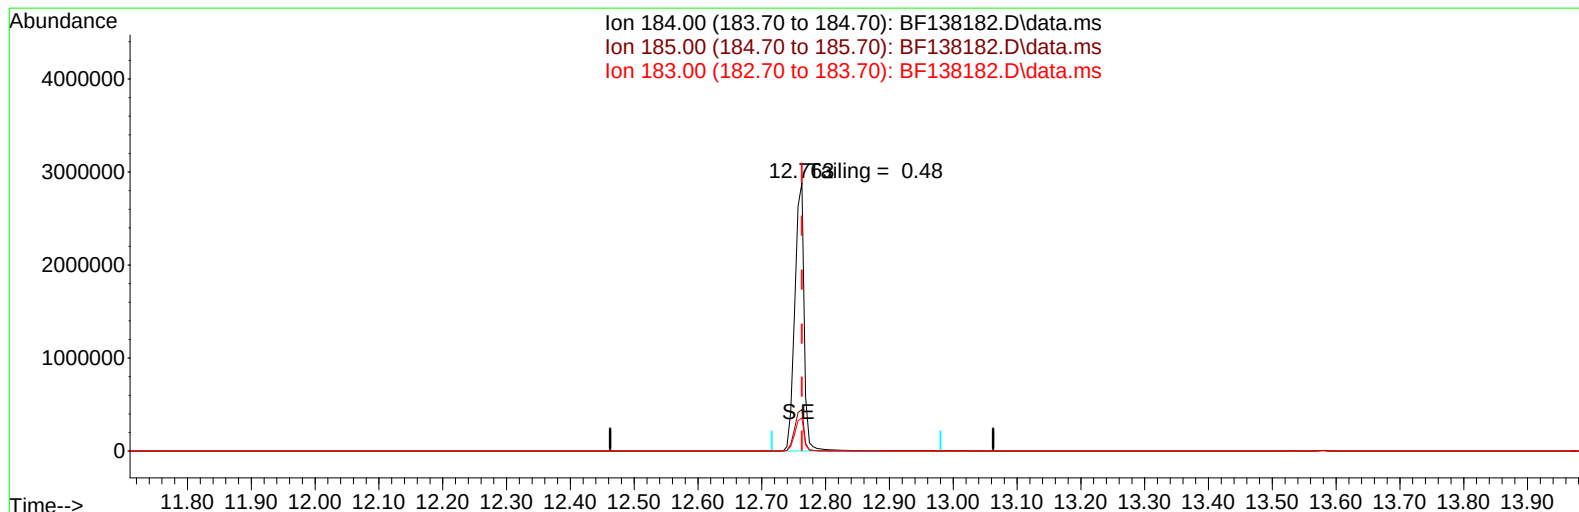

TIC: BF138182.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 1006630.00 ng

response **2952270**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.20	15.43
--------	-------	-------

183.00	11.20	12.37
--------	-------	-------

0.00 0.00 0.00