

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
 Data File : BF138184.D
 Acq On : 11 Jun 2024 13:07
 Operator : CG\JU
 Sample : PB161404BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB161404BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.275	18	32	38	rVB	231046	337045	2.42%	0.408%
2	5.145	512	520	533	rVB	422385	582805	4.18%	0.706%
3	5.528	579	585	588	rBV	8818136	9727757	69.78%	11.781%
4	6.528	748	755	757	rBV	7770835	9756141	69.99%	11.815%
5	6.898	814	818	821	rBV	2926564	2418663	17.35%	2.929%
6	7.457	908	913	916	rBV	5576207	6334986	45.44%	7.672%
7	8.175	1031	1035	1039	rBV	3345579	3259118	23.38%	3.947%
8	9.257	1213	1219	1222	rBV	12312227	12207765	87.57%	14.784%
9	9.933	1329	1334	1337	rBV	4737763	3834937	27.51%	4.644%
10	10.722	1462	1468	1472	rBV	7425246	7752592	55.61%	9.389%
11	11.421	1583	1587	1590	rBV	4956114	4056351	29.10%	4.912%
12	11.933	1669	1674	1692	rBV	234260	355632	2.55%	0.431%
13	12.716	1803	1807	1816	rBV	146801	215473	1.55%	0.261%
14	13.015	1852	1858	1861	rBV	12491751	13939900	100.00%	16.882%
15	14.057	2031	2035	2039	rBV	4447564	3931198	28.20%	4.761%
16	15.539	2281	2287	2292	rBV	3067233	3862818	27.71%	4.678%




Sum of corrected areas: 82573181

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138184.D
Acq On : 11 Jun 2024 13:07
Operator : CG\JU
Sample : PB161404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

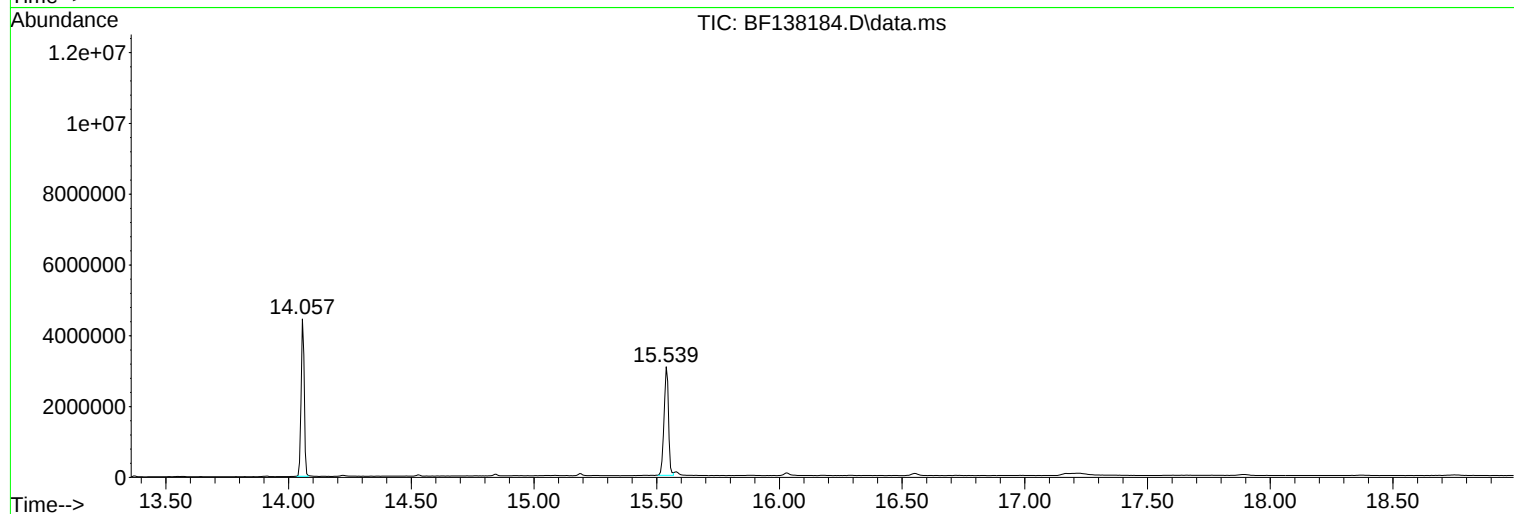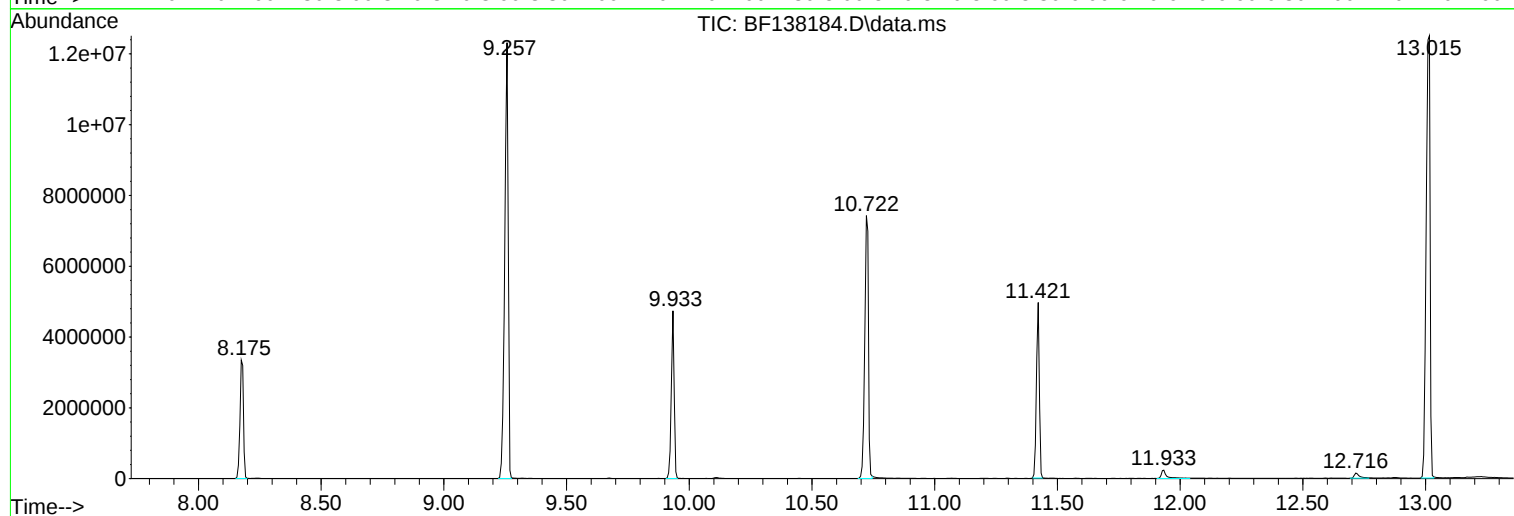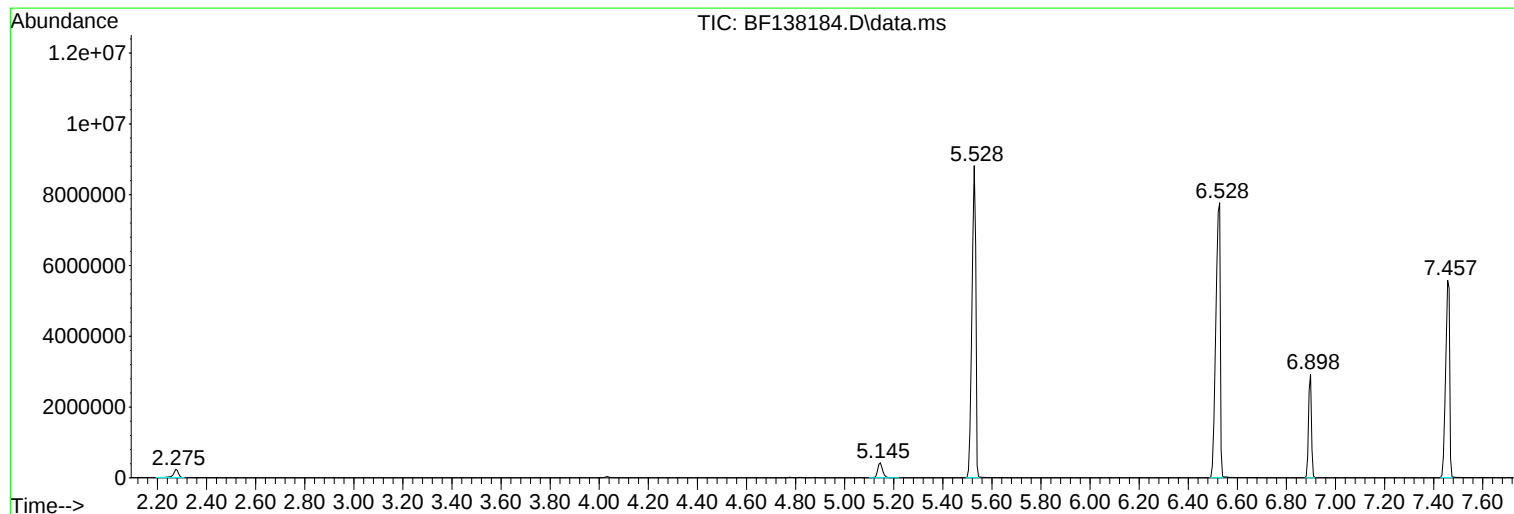

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138184.D
Acq On : 11 Jun 2024 13:07
Operator : CG\JU
Sample : PB161404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138184.D
Acq On : 11 Jun 2024 13:07
Operator : CG\JU
Sample : PB161404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------