
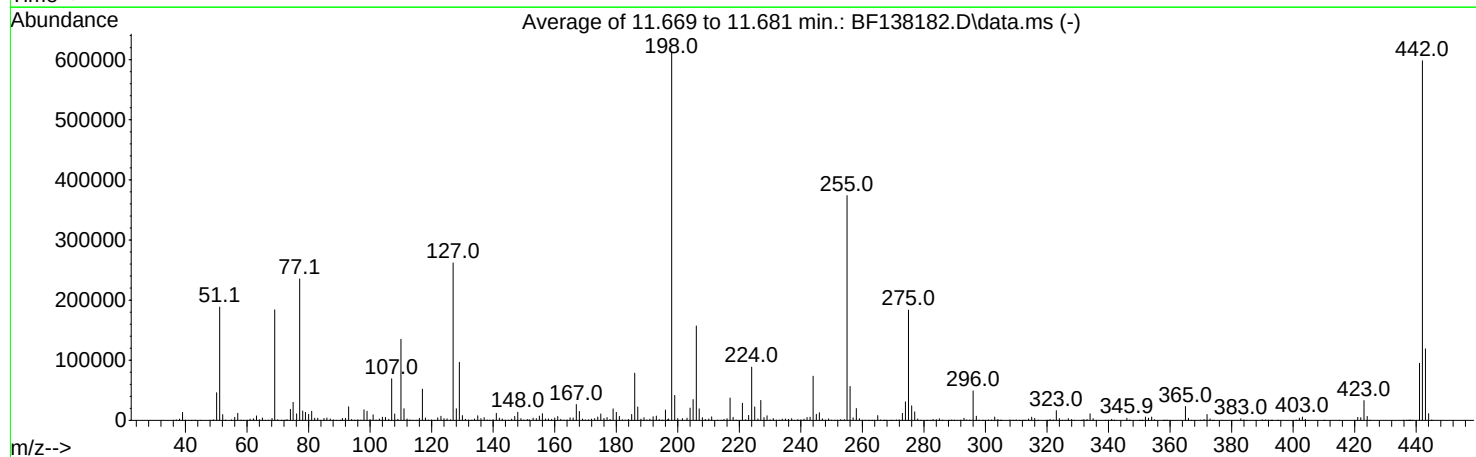


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138182.D
Acq On : 11 Jun 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 06 05:19:29 2024

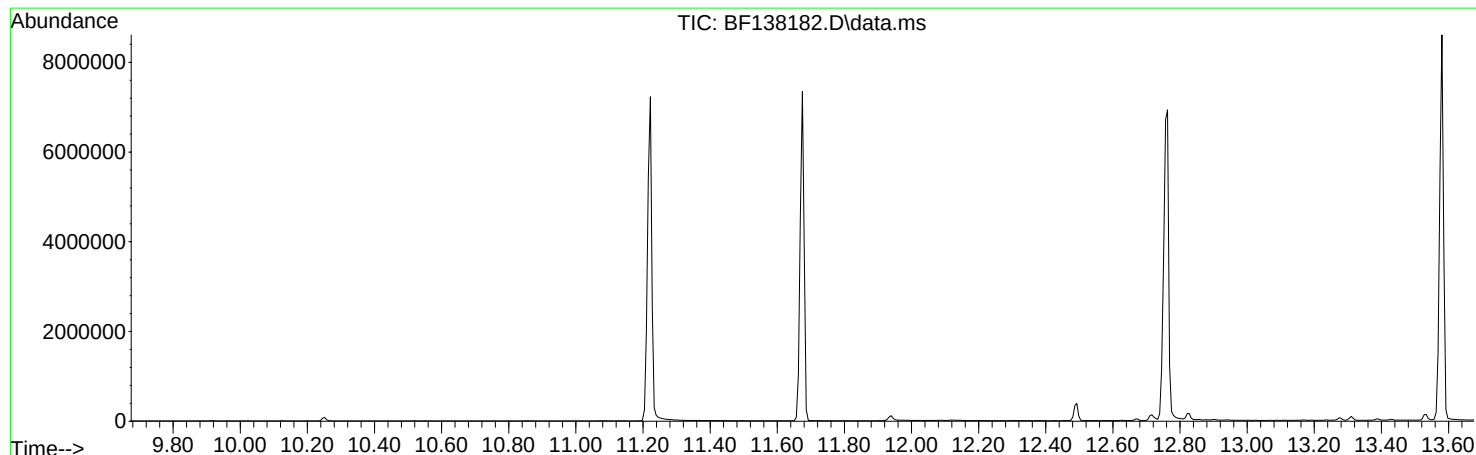




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	188517	PASS
68	69	0.00	2	1.7	3110	PASS
69	198	0.00	100	30.1	184000	PASS
70	69	0.00	2	0.6	1115	PASS
127	198	10	80	42.8	262037	PASS
197	198	0.00	2	0.4	2556	PASS
198	198	100	100	100.0	611925	PASS
199	198	5	9	6.8	41648	PASS
275	198	10	60	30.0	183467	PASS
365	198	1	100	3.8	23061	PASS
441	198	0.01	100	15.5	94917	PASS
442	442	50	100	100.0	598357	PASS
443	442	15	24	19.9	118885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\
Data File : BF138182.D
Acq On : 11 Jun 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

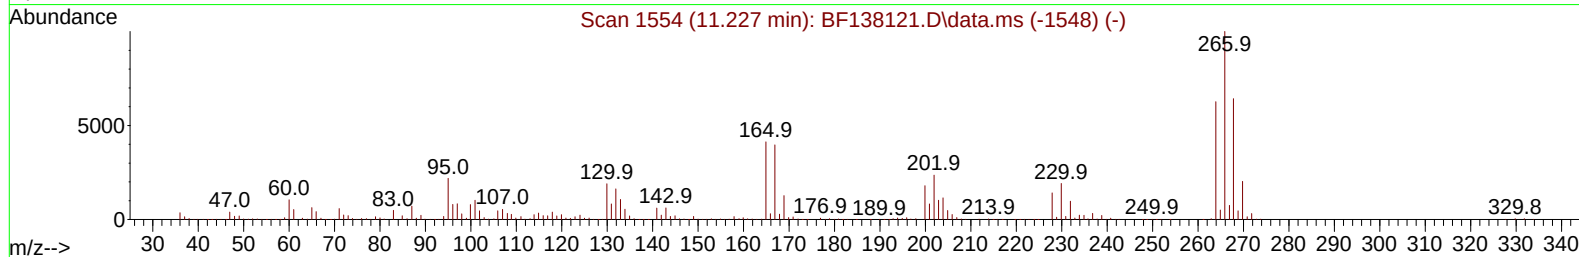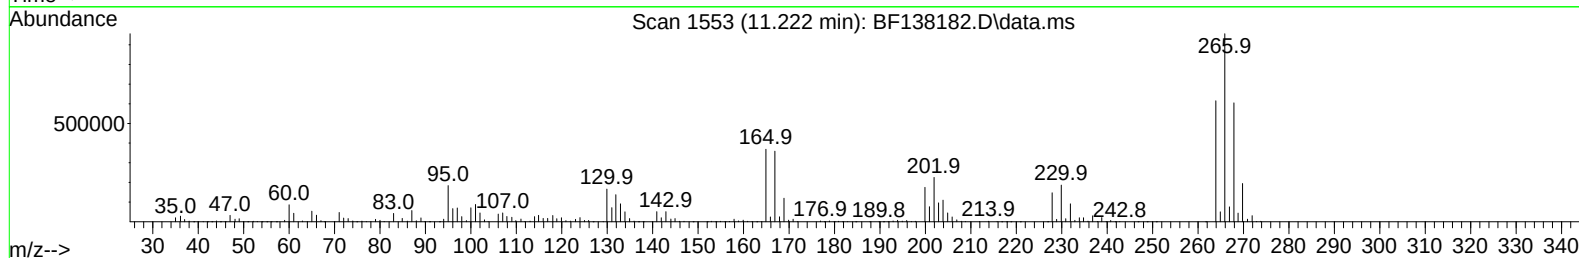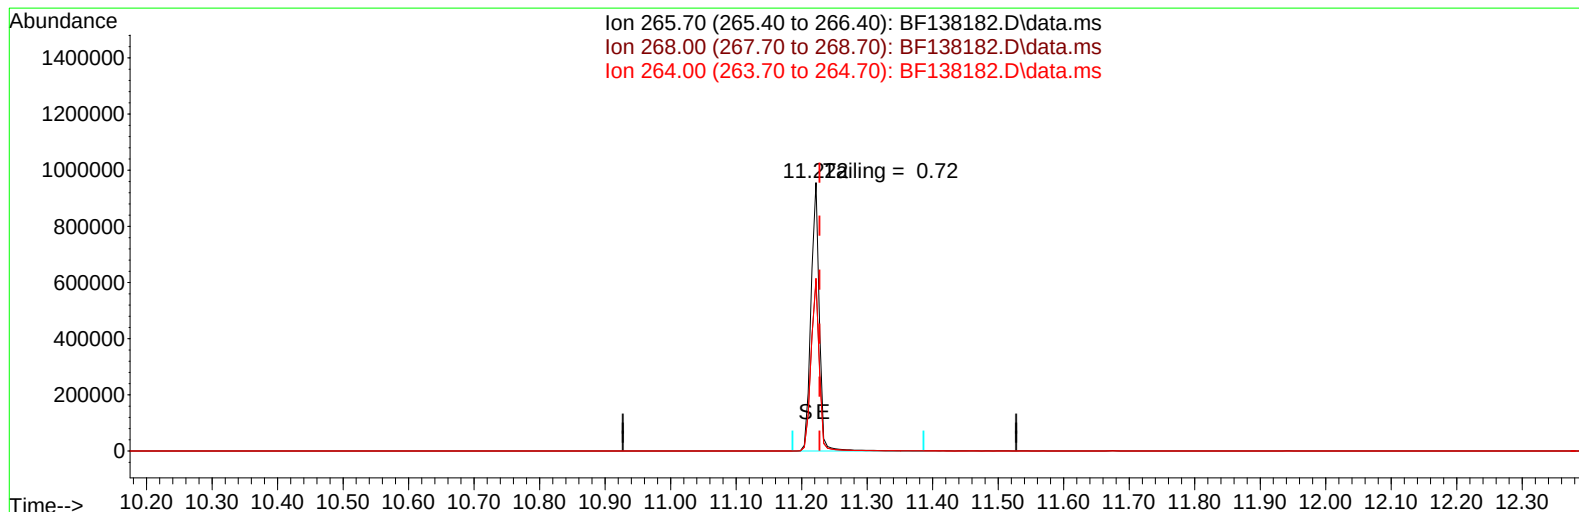

TIC: BF138182.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.006) 750653.71 ng




response 840427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.23
264.00	62.60	64.35
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061124\  
Data File : BF138182.D  
Acq On    : 11 Jun 2024  09:17  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

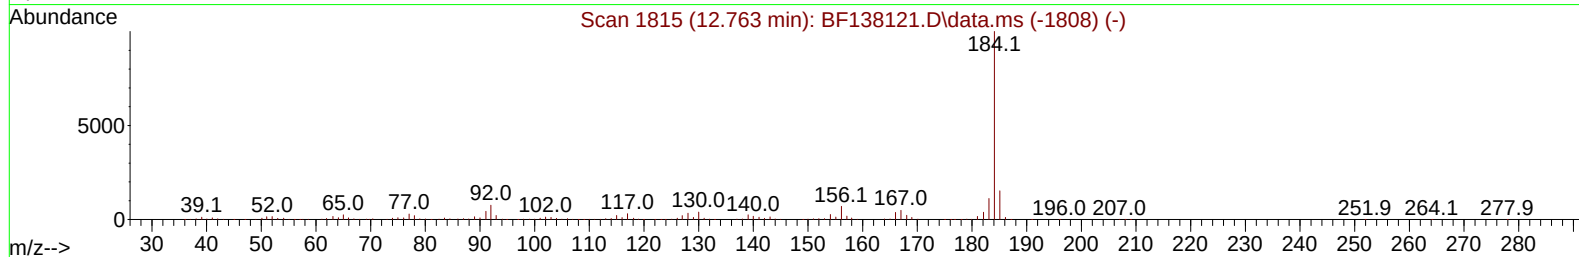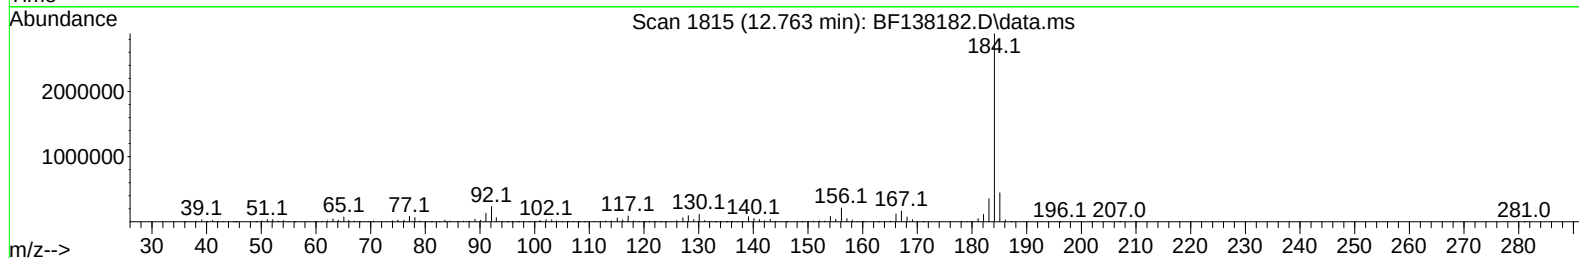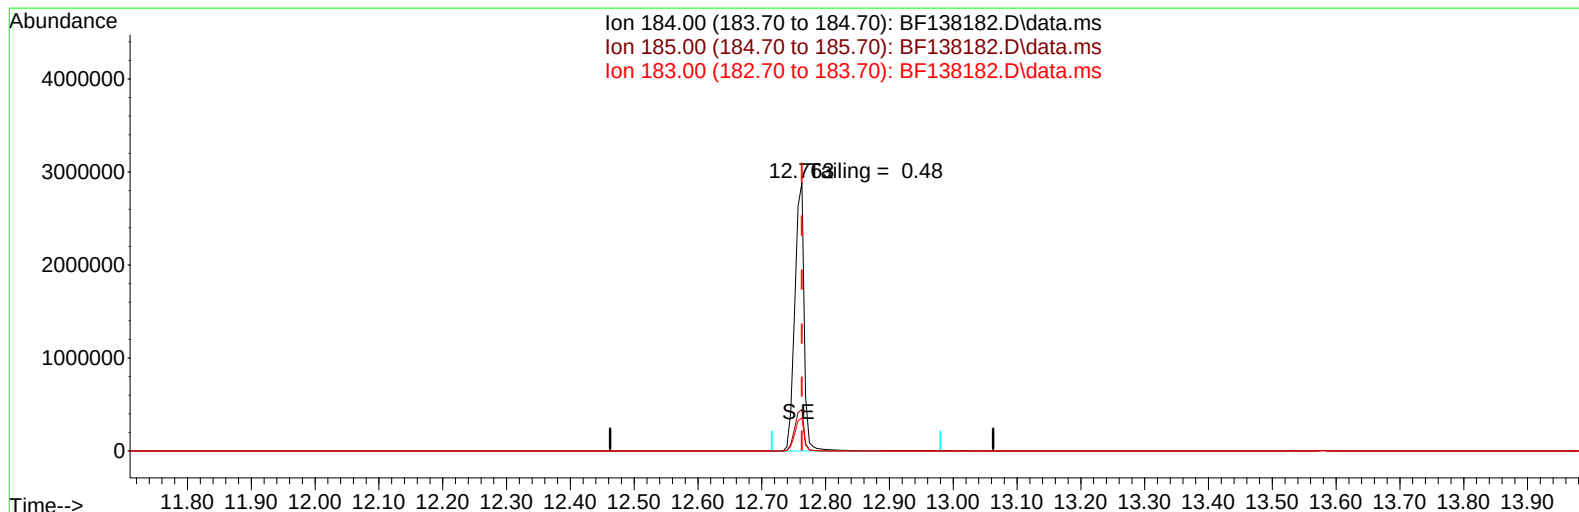

TIC: BF138182.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 1006630.00 ng

response **2952270**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.20	15.43
--------	-------	-------

183.00	11.20	12.37
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/11/2024	BNA_F	<u>BF138183.D</u>
Compound Name	Response	Retention Time
DDT	1356875	13.58
DDD	21194	13.31
DDE	1129	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22323	1379198	1.62

Instrument :
BNA_F
ClientSampleId :
DFTPP