
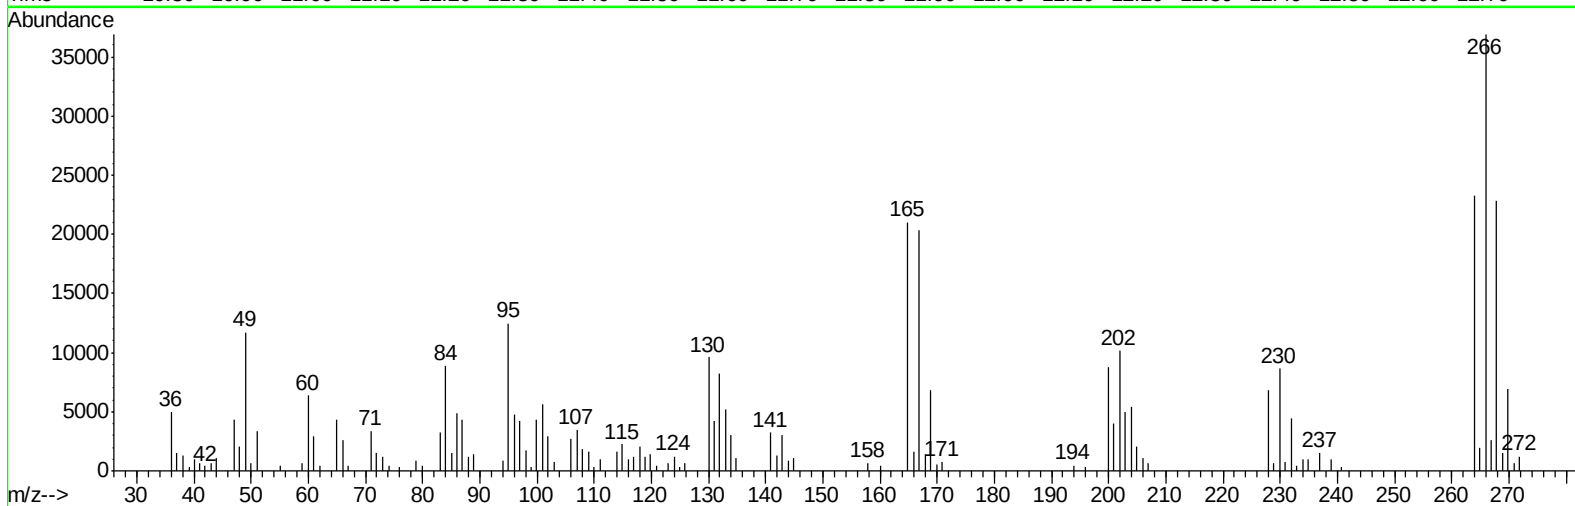


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061215\
Data File : BF079934.D
Acq On : 12 Jun 2015 14:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 06:44:58 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 22:57:49 2015
Response via : Initial Calibration

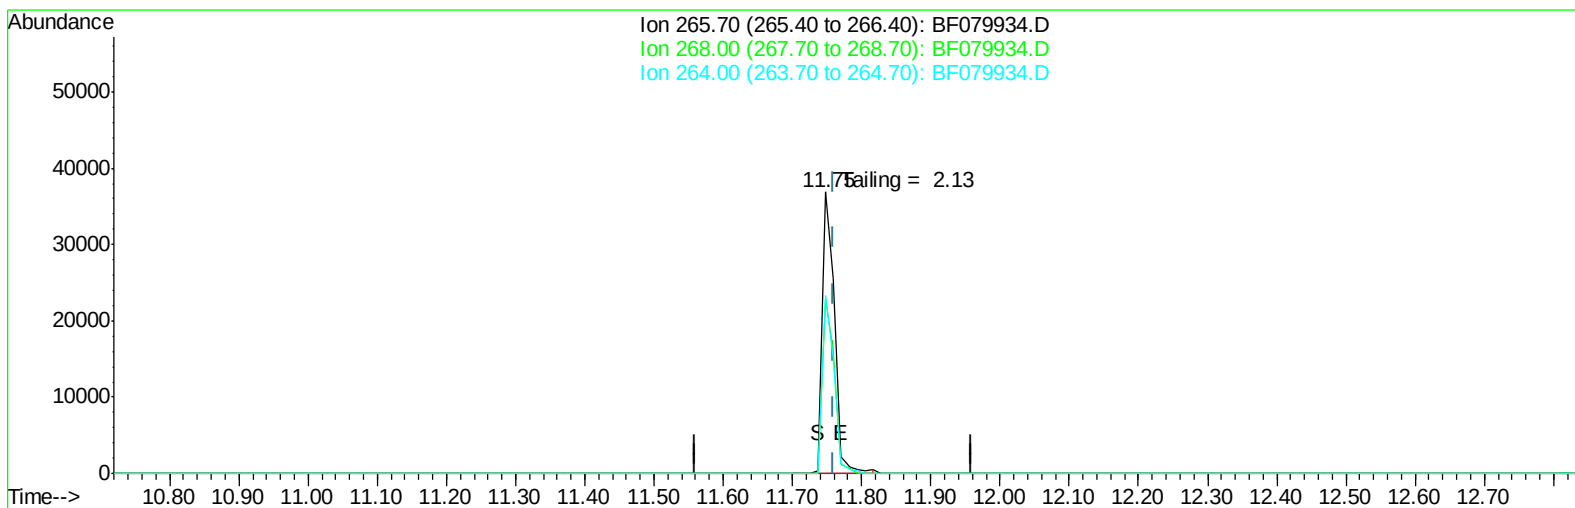

TIC: BF079934.D

(69) Pentachlorophenol (C)



11.748min (-0.011) 0.00ng

response 46164

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	61.94
264.00	59.60	63.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061215\
Data File : BF079934.D
Acq On : 12 Jun 2015 14:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 06:44:58 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 22:57:49 2015
Response via : Initial Calibration

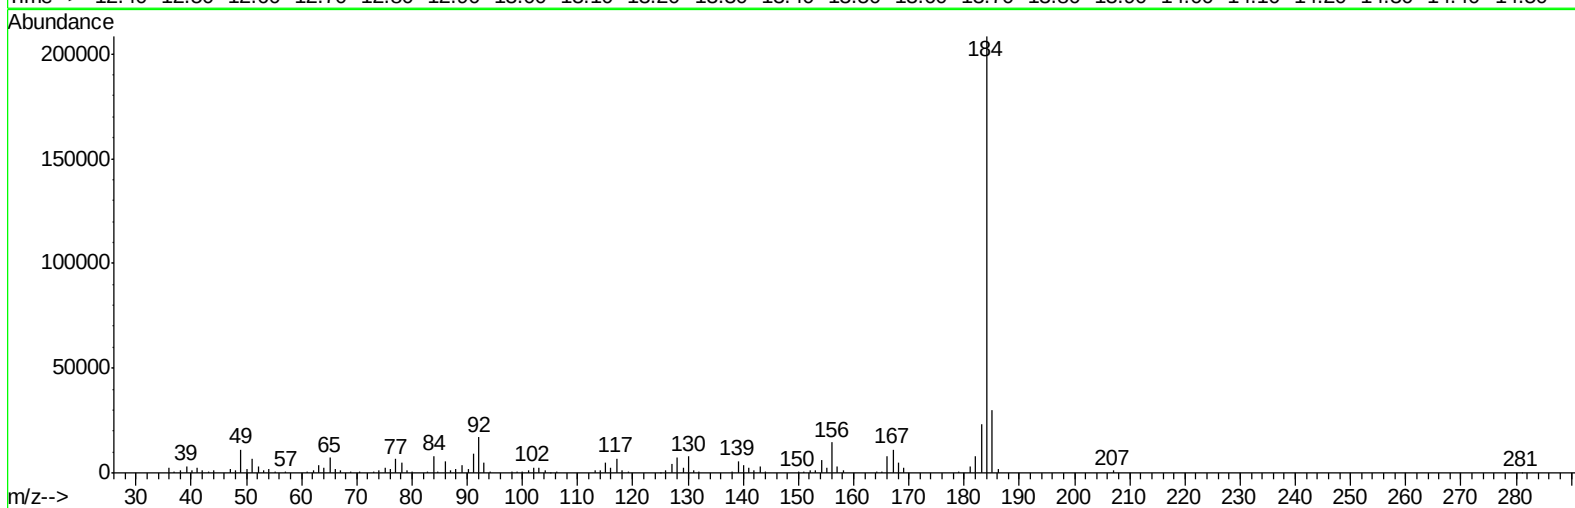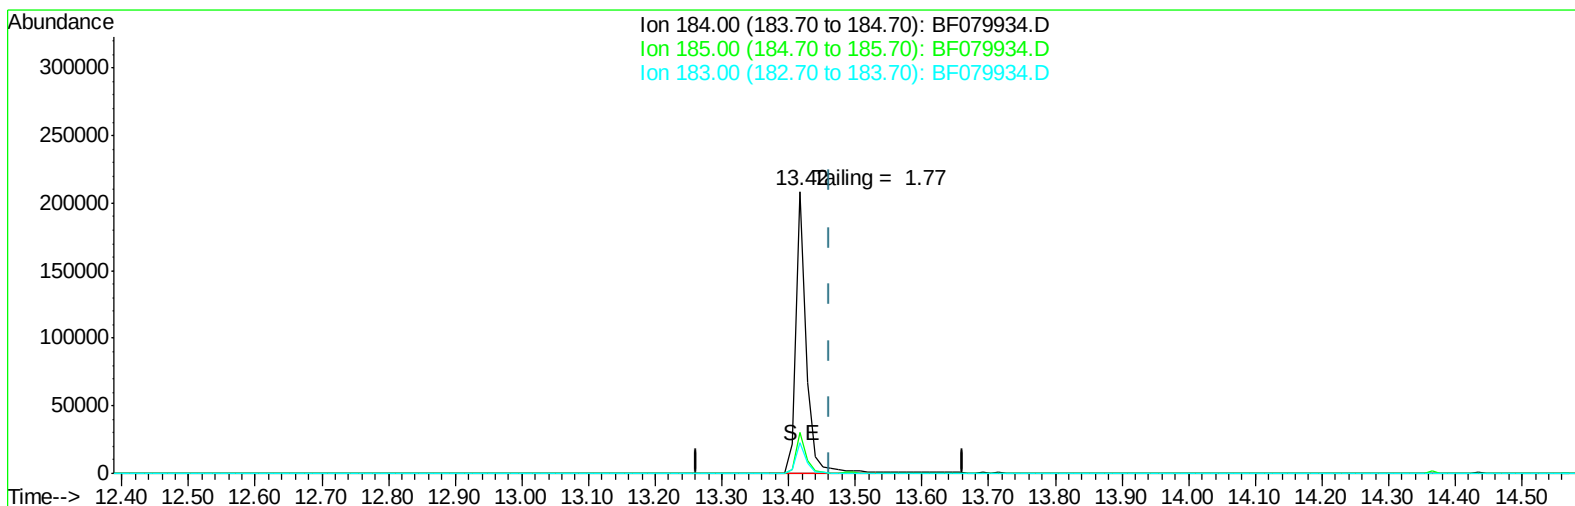

TIC: BF079934.D

(76) Benzidine

13.417min (-0.046) 0.00ng

response 228209

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.36
183.00	11.30	11.08
0.00	0.00	0.00