


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061215\
 Data File : BF079934.D
 Acq On : 12 Jun 2015 14:11
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 12 22:57:49 2015

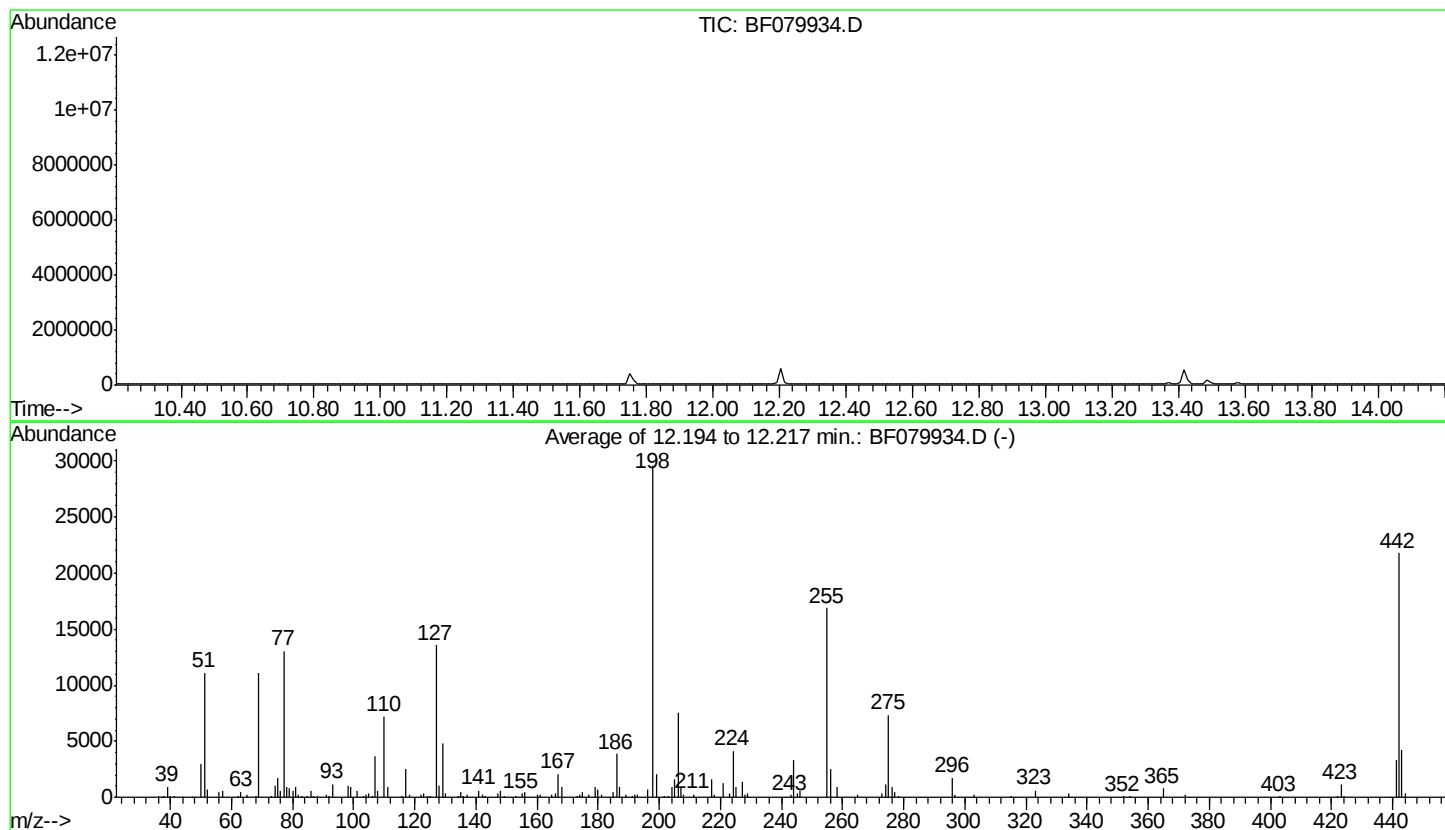

AutoFind: Scans 963, 964, 965; Background Corrected with Scan 960

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	11141	PASS
68	69	0.00	2	1.3	143	PASS
69	198	0.00	100	37.4	11065	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	13565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29596	PASS
199	198	5	9	6.9	2034	PASS
275	198	10	60	24.8	7334	PASS
365	198	1	100	2.6	775	PASS
441	442	0.01	24	15.2	3309	PASS
442	198	50	100	73.6	21776	PASS
443	442	15	24	19.7	4286	PASS