


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061215\
 Data File : BF079957.D
 Acq On : 13 Jun 2015 3:54
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 12 22:57:49 2015

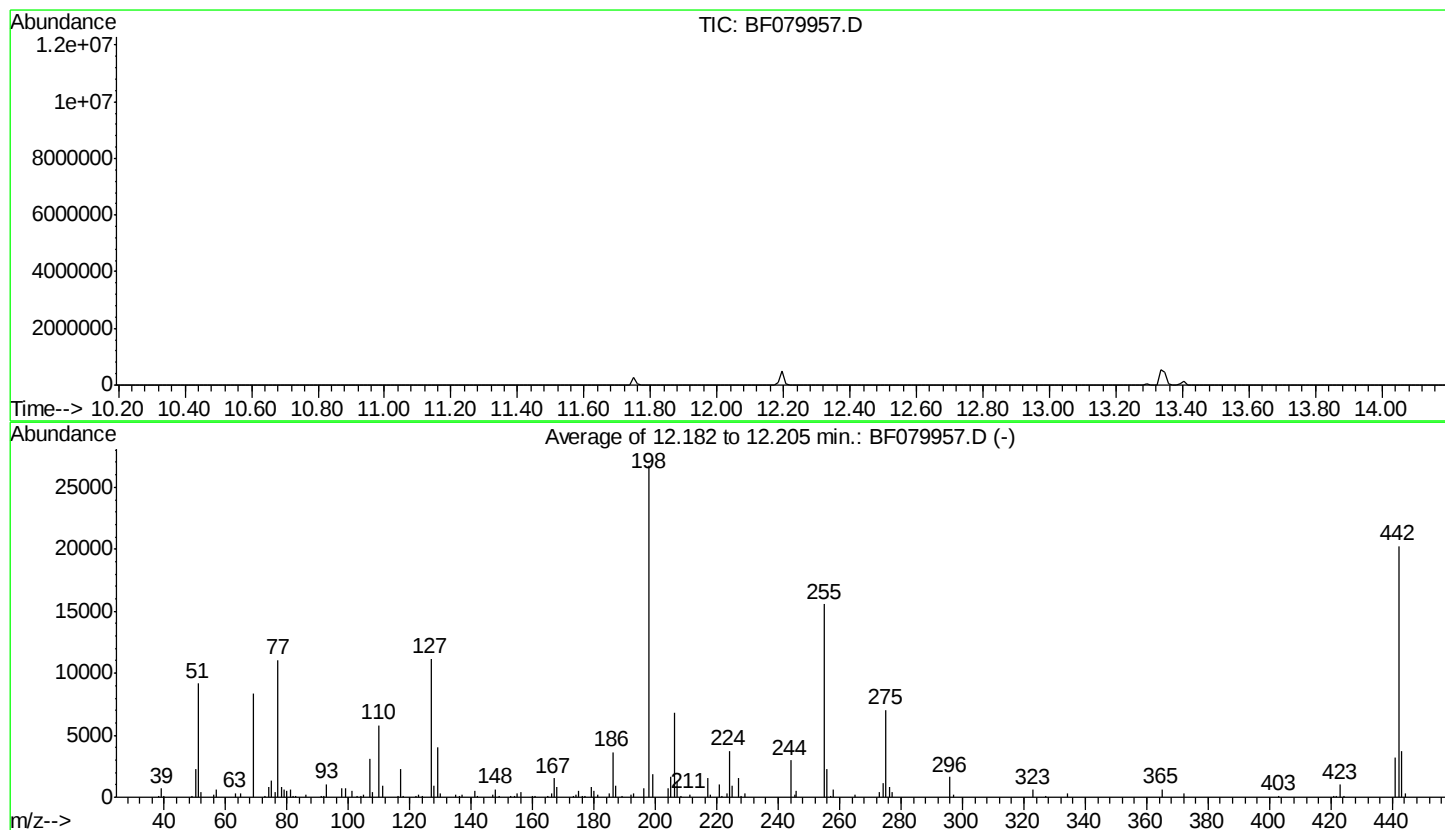

AutoFind: Scans 962, 963, 964; Background Corrected with Scan 959

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	9163	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.3	8375	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	11170	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26743	PASS
199	198	5	9	6.8	1828	PASS
275	198	10	60	26.4	7061	PASS
365	198	1	100	2.5	658	PASS
441	442	0.01	24	15.8	3207	PASS
442	198	50	100	75.8	20263	PASS
443	442	15	24	18.5	3739	PASS