

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061220\  
 Data File : BF120612.D  
 Acq On : 12 Jun 2020 14:44  
 Operator : JU/CG  
 Sample : PB129506BL  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB129506BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.410       | 560           | 565         | 568          | rBV      | 3909154        | 3910411       | 67.55%          | 10.538%       |
| 2         | 6.434       | 733           | 739         | 741          | rBV      | 3486926        | 4043102       | 69.84%          | 10.896%       |
| 3         | 6.798       | 797           | 801         | 804          | rBV      | 1184515        | 956392        | 16.52%          | 2.577%        |
| 4         | 6.957       | 823           | 828         | 831          | rBV      | 3913427        | 3486323       | 60.23%          | 9.395%        |
| 5         | 7.363       | 891           | 897         | 900          | rBV      | 2963737        | 2783806       | 48.09%          | 7.502%        |
| 6         | 8.080       | 1015          | 1019        | 1022         | rBV      | 1531782        | 1275606       | 22.04%          | 3.438%        |
| 7         | 9.157       | 1197          | 1202        | 1205         | rBV      | 5584152        | 5093959       | 88.00%          | 13.727%       |
| 8         | 9.833       | 1313          | 1317        | 1320         | rBV      | 1731545        | 1466494       | 25.33%          | 3.952%        |
| 9         | 10.621      | 1446          | 1451        | 1454         | rBV      | 3464182        | 3330660       | 57.54%          | 8.976%        |
| 10        | 11.316      | 1565          | 1569        | 1572         | rBV      | 1901148        | 1575797       | 27.22%          | 4.247%        |
| 11        | 12.904      | 1834          | 1839        | 1842         | rBV      | 5428810        | 5788681       | 100.00%         | 15.600%       |
| 12        | 13.951      | 2013          | 2017        | 2021         | rBV      | 1755510        | 1488956       | 25.72%          | 4.013%        |
| 13        | 15.051      | 2200          | 2204        | 2210         | rVB      | 55293          | 64867         | 1.12%           | 0.175%        |
| 14        | 15.392      | 2256          | 2262        | 2265         | rBV      | 1235101        | 1561246       | 26.97%          | 4.207%        |
| 15        | 15.421      | 2265          | 2267        | 2277         | rVB      | 77046          | 93430         | 1.61%           | 0.252%        |
| 16        | 15.839      | 2333          | 2338        | 2345         | rVB      | 61266          | 87731         | 1.52%           | 0.236%        |
| 17        | 16.333      | 2416          | 2422        | 2428         | rBV      | 51930          | 100242        | 1.73%           | 0.270%        |


Sum of corrected areas: 37107703

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061220\  
Data File : BF120612.D  
Acq On : 12 Jun 2020 14:44  
Operator : JU/CG  
Sample : PB129506BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

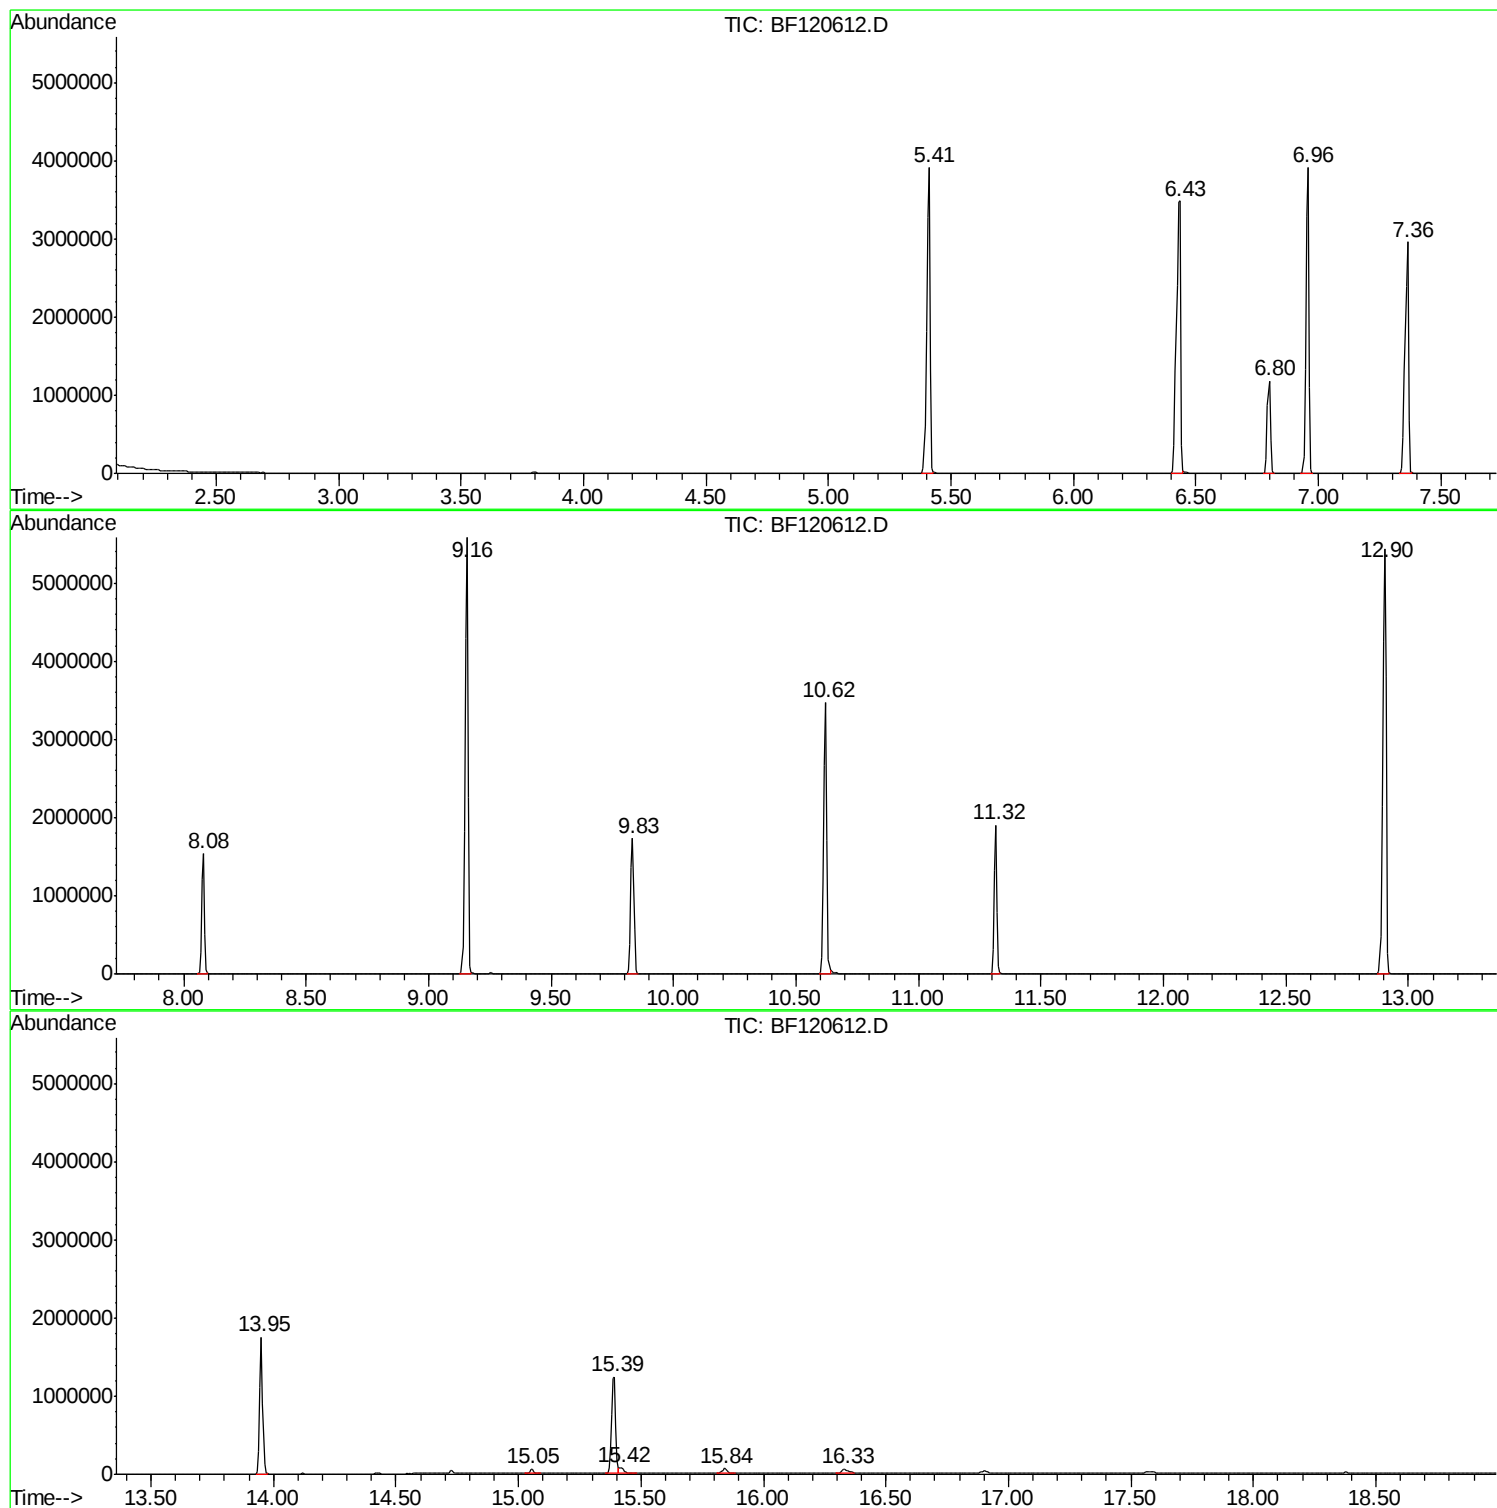

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061220\  
Data File : BF120612.D  
Acq On : 12 Jun 2020 14:44  
Operator : JU/CG  
Sample : PB129506BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061220\  
Data File : BF120612.D  
Acq On : 12 Jun 2020 14:44  
Operator : JU/CG  
Sample : PB129506BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |