


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061220\
 Data File : BF120606.D
 Acq On : 12 Jun 2020 7:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

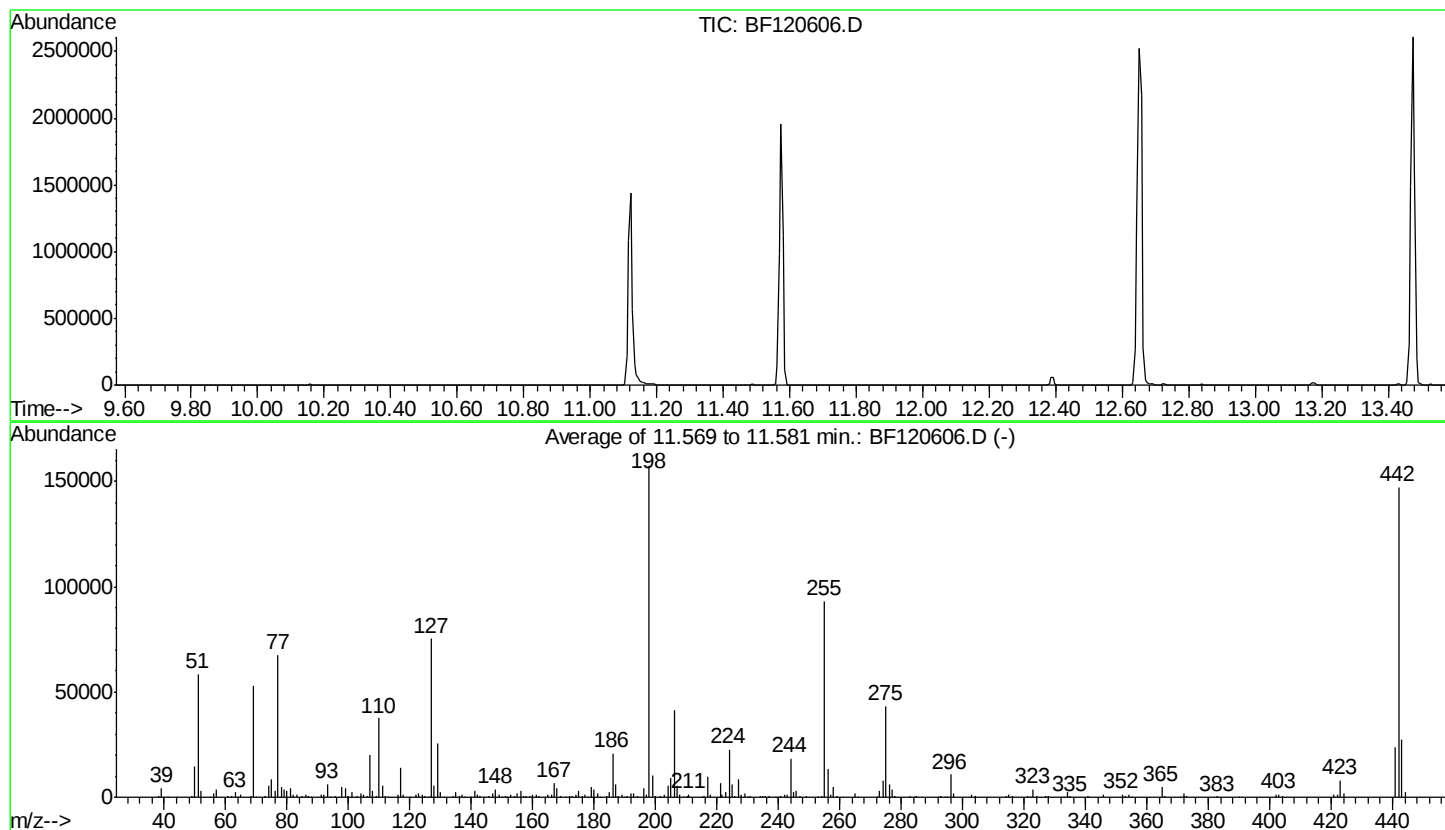

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	58693	PASS
68	69	0.00	2	1.7	880	PASS
69	198	0.00	100	33.6	52968	PASS
70	69	0.00	2	0.5	289	PASS
127	198	10	80	47.8	75312	PASS
197	198	0.00	2	0.6	981	PASS
198	198	100	100	100.0	157546	PASS
199	198	5	9	6.7	10585	PASS
275	198	10	60	27.6	43445	PASS
365	198	1	100	3.2	5113	PASS
441	198	0.01	100	14.9	23543	PASS
442	198	50	100	93.5	147333	PASS
443	442	15	24	18.4	27159	PASS