
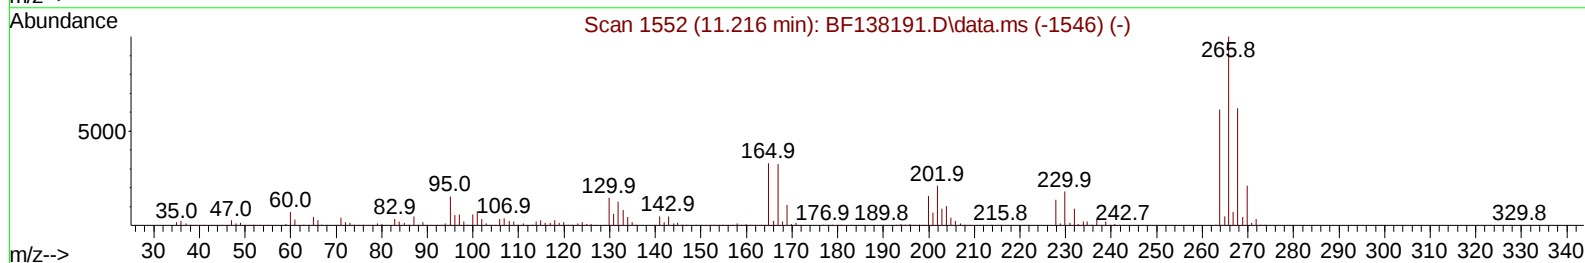
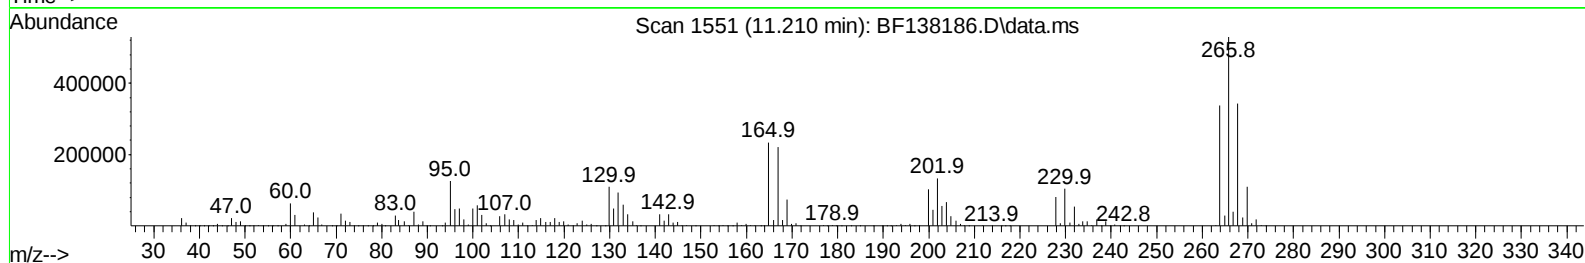


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061224\
Data File : BF138186.D
Acq On : 12 Jun 2024 11:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:05:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

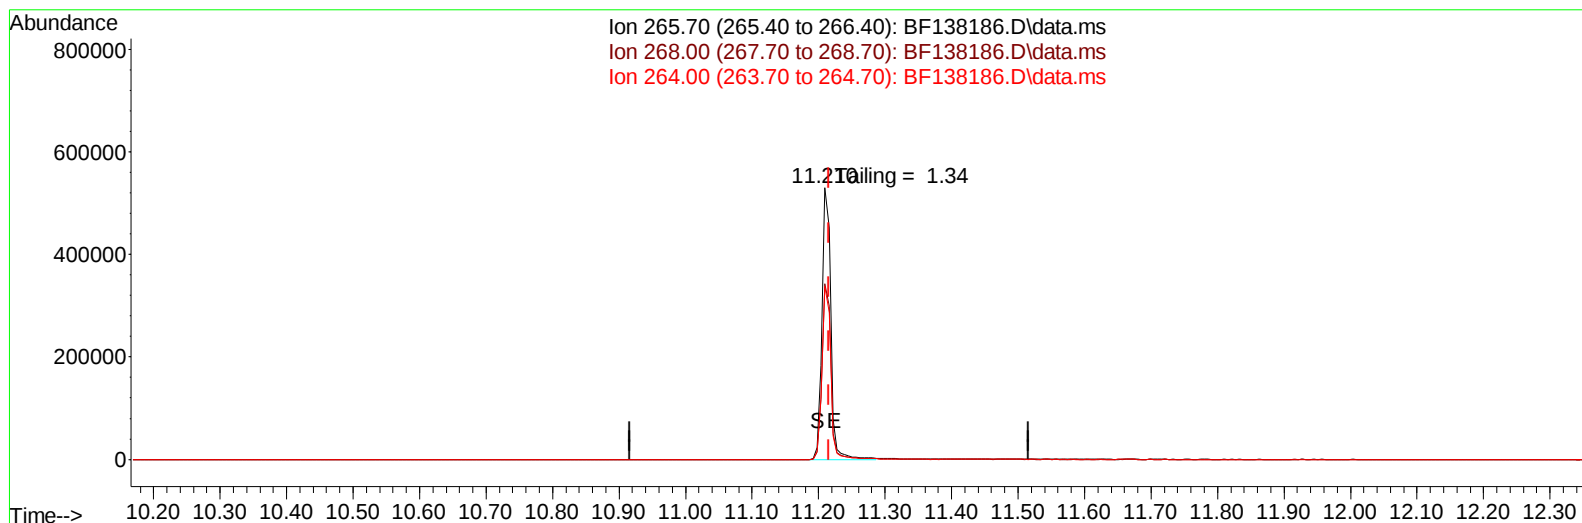

TIC: BF138186.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 165798.74 ng

response 478102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.64
264.00	61.50	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061224\
Data File : BF138186.D
Acq On : 12 Jun 2024 11:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:05:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

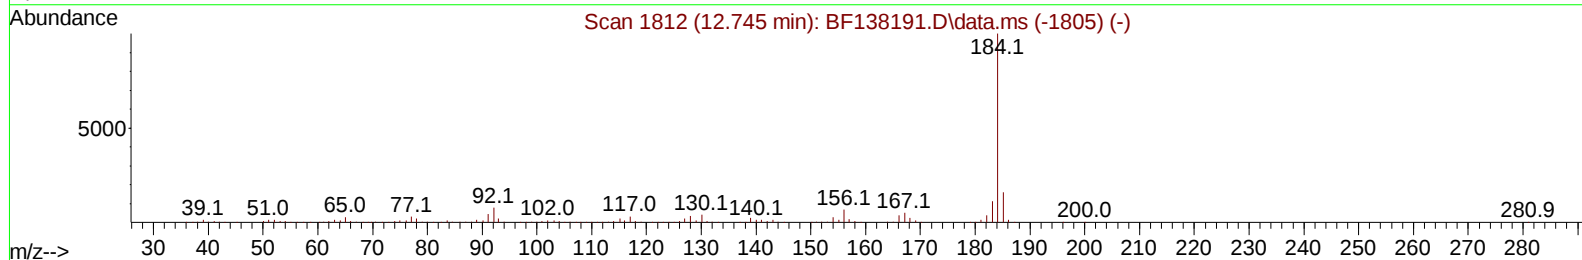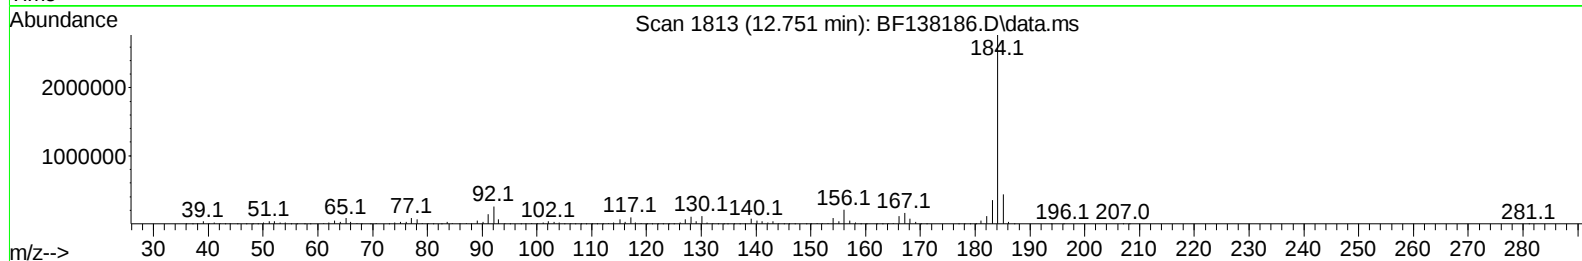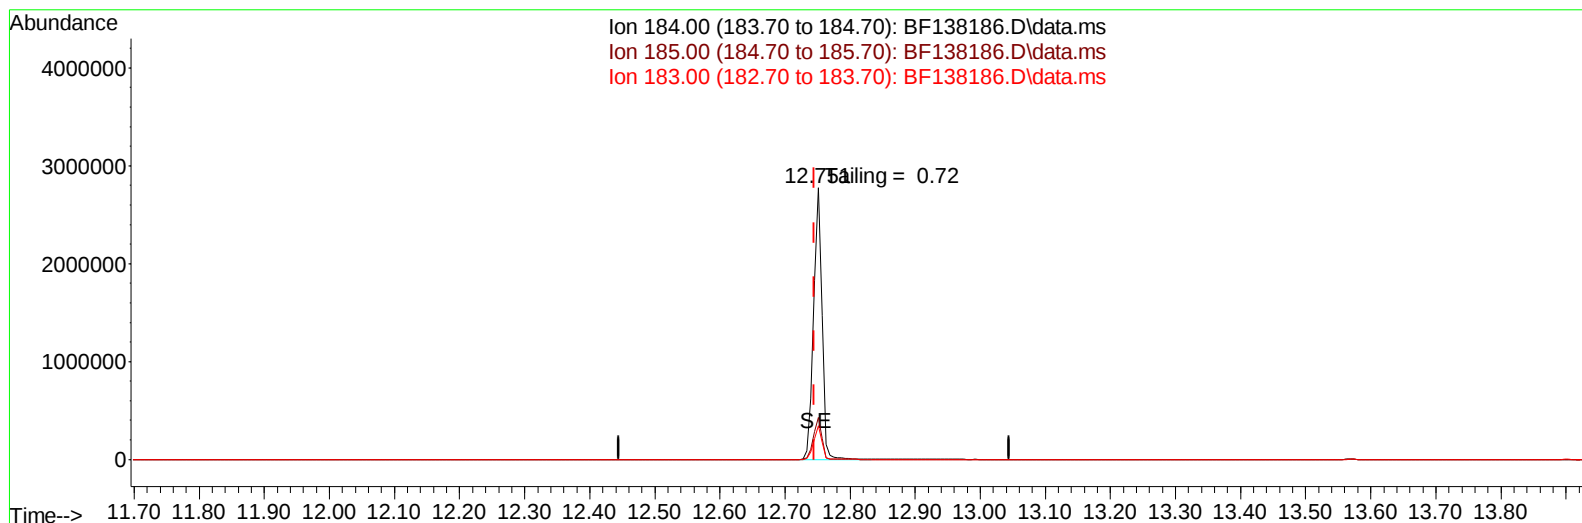

TIC: BF138186.D\data.ms

(77) Benzidine**12.751min (+ 0.006) 1634606.01 ng****response 2514633**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.45
183.00	11.30	12.46
0.00	0.00	0.00