


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061224\
Data File : BF138186.D
Acq On : 12 Jun 2024 11:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

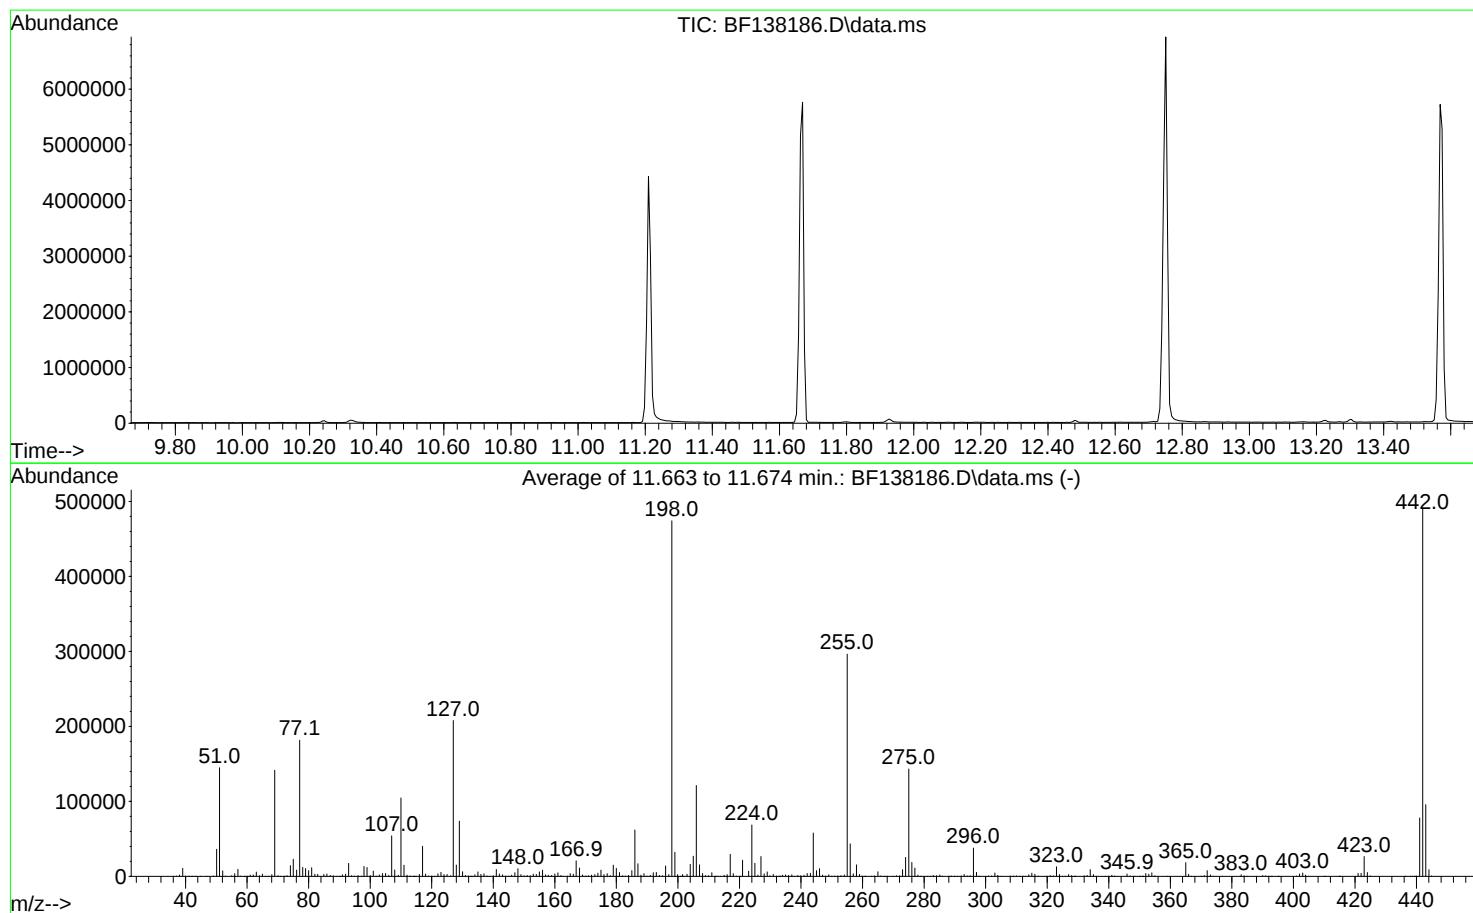




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	145003	PASS
68	69	0.00	2	1.7	2379	PASS
69	198	0.00	100	29.8	141424	PASS
70	69	0.00	2	0.6	843	PASS
127	198	10	80	43.9	207949	PASS
197	198	0.00	2	0.5	2302	PASS
198	198	100	100	100.0	474101	PASS
199	198	5	9	6.8	32319	PASS
275	198	10	60	30.2	143125	PASS
365	198	1	100	3.9	18415	PASS
441	198	0.01	100	16.4	77917	PASS
442	442	50	100	100.0	490560	PASS
443	442	15	24	19.5	95544	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061224\
Data File : BF138186.D
Acq On : 12 Jun 2024 11:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 02:05:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

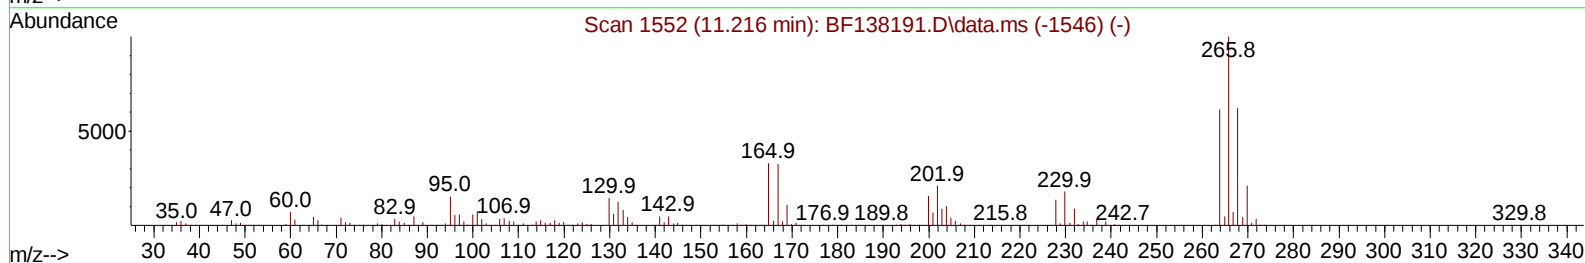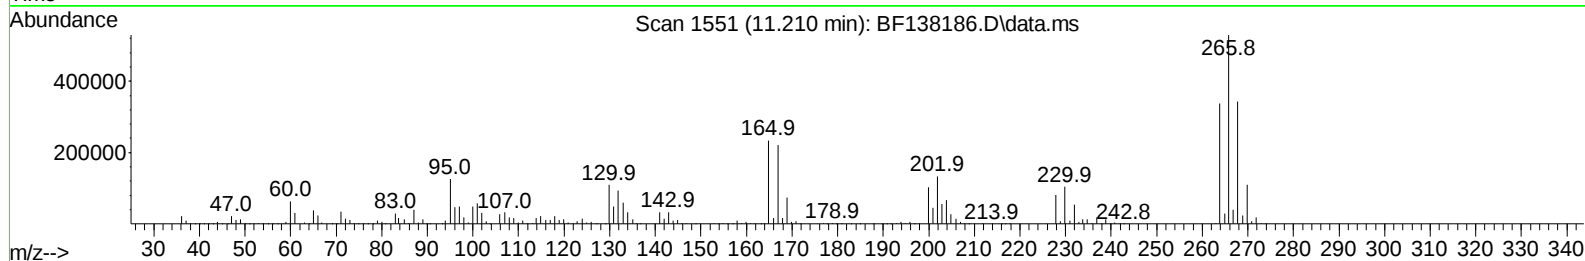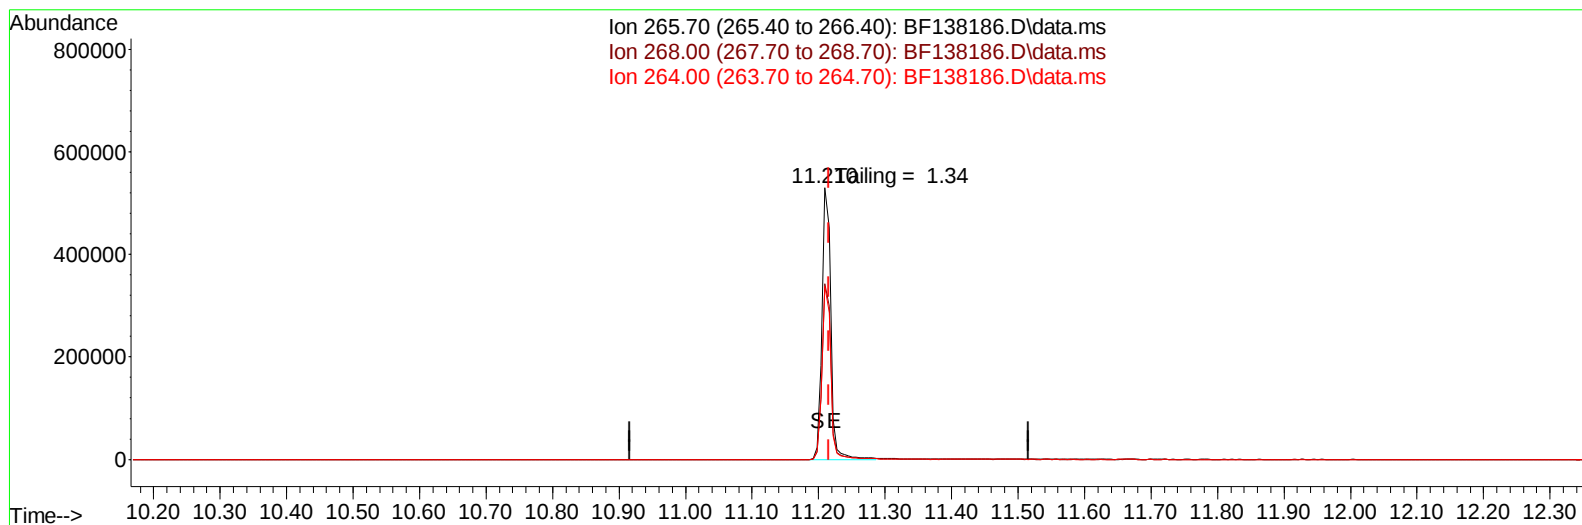

TIC: BF138186.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 165798.74 ng




response 478102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.64
264.00	61.50	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061224\
Data File : BF138186.D
Acq On : 12 Jun 2024 11:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 02:05:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

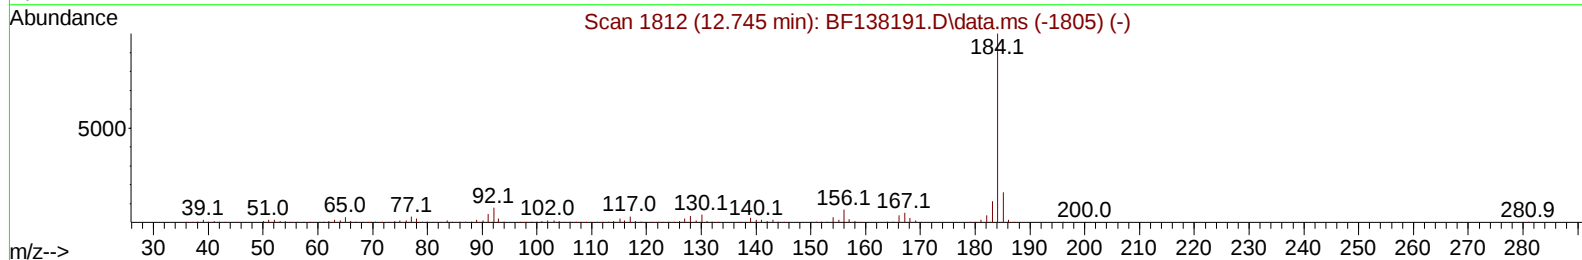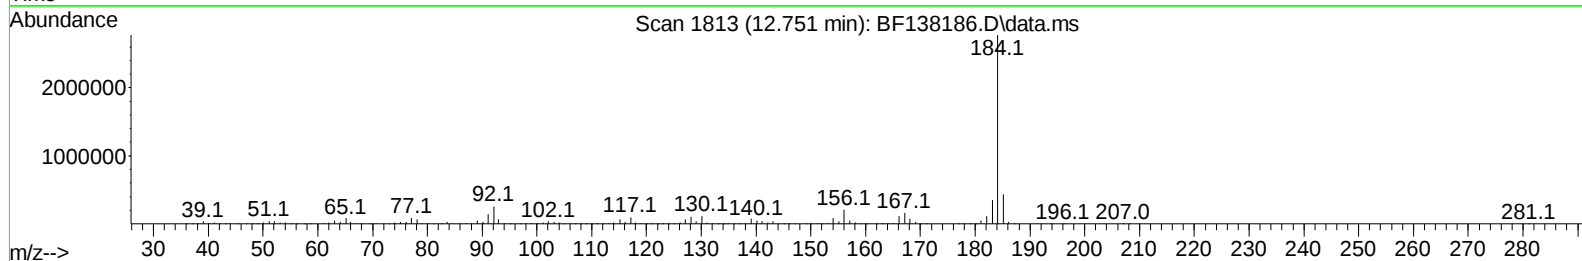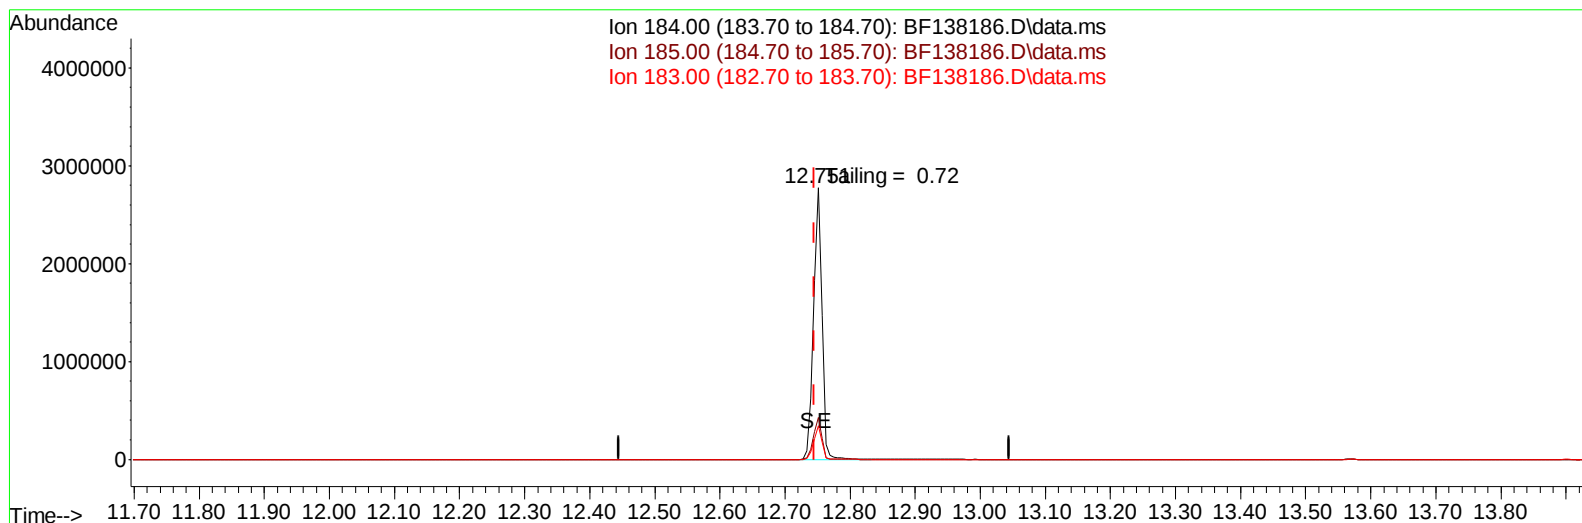

TIC: BF138186.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 1634606.01 ng

response 2514633

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.45
183.00	11.30	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2024	BNA_F	<u>BF138186.D</u>
Compound Name	Response	Retention Time
DDT	944847	13.574
DDD	7667	13.304
DDE	164	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7831	952678	0.82

Instrument :
BNA_F
ClientSampleId :
DFTPP