
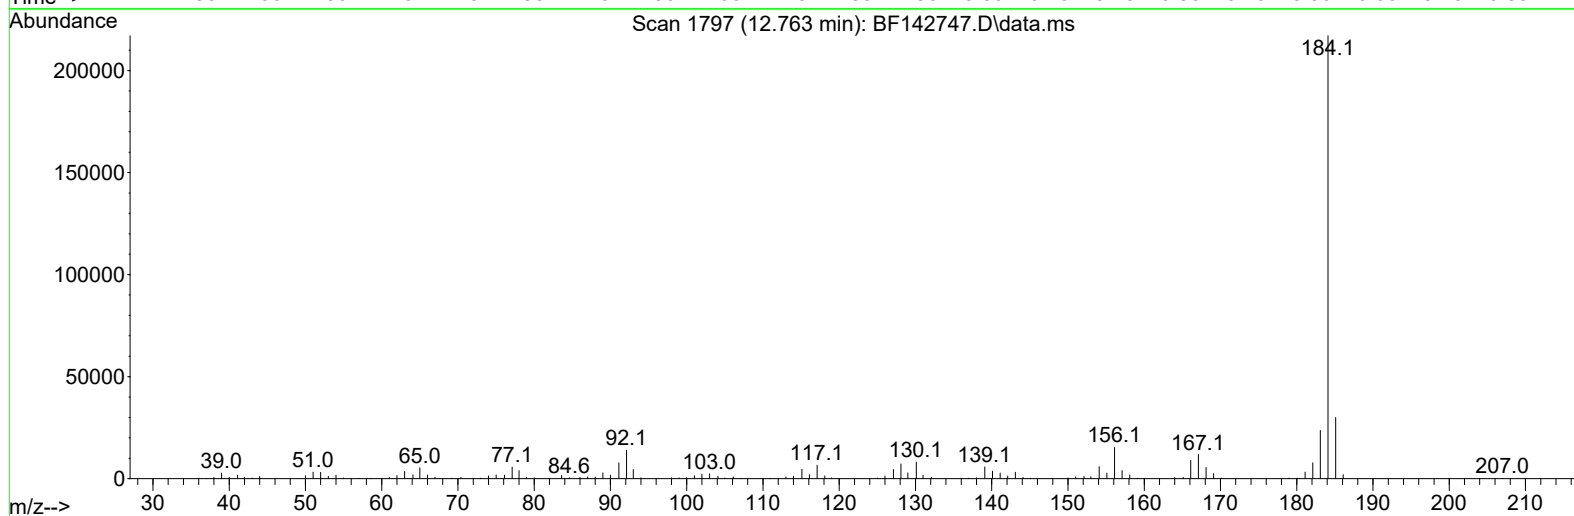


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142747.D
Acq On : 12 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 11:59:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

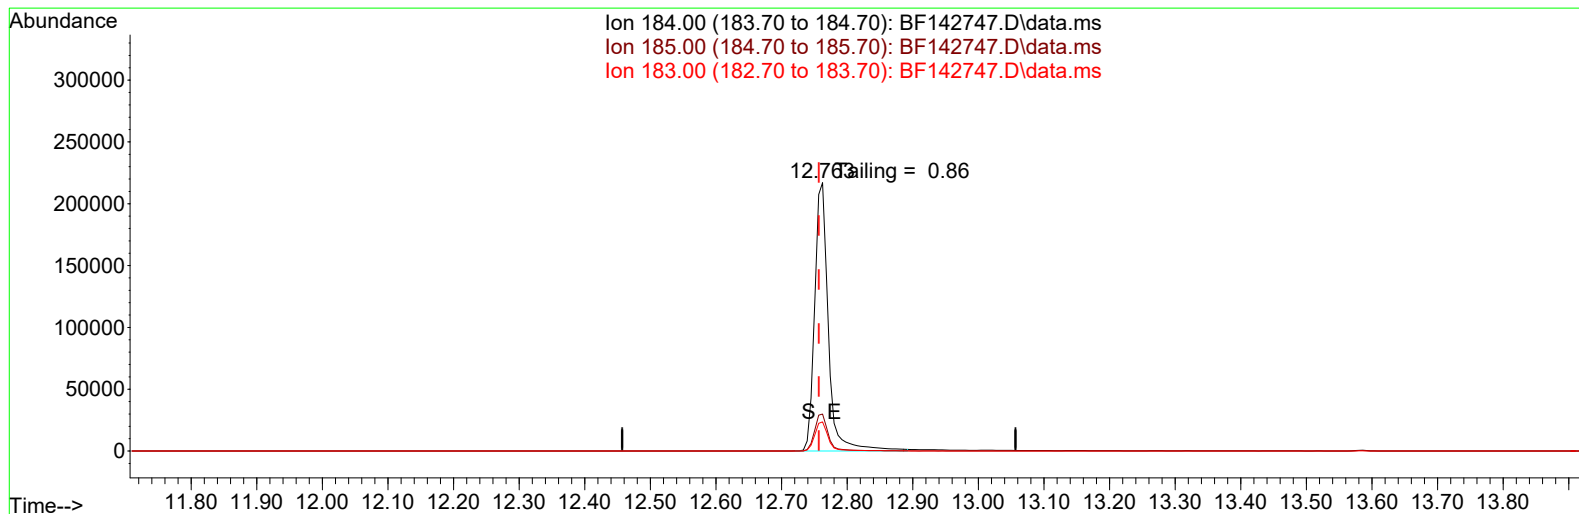

TIC: BF142747.D\data.ms

(77) Benzidine



12.763min (+ 0.006) 0.00 ng

response 319051

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.81
183.00	10.70	10.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142747.D
Acq On : 12 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 11:59:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

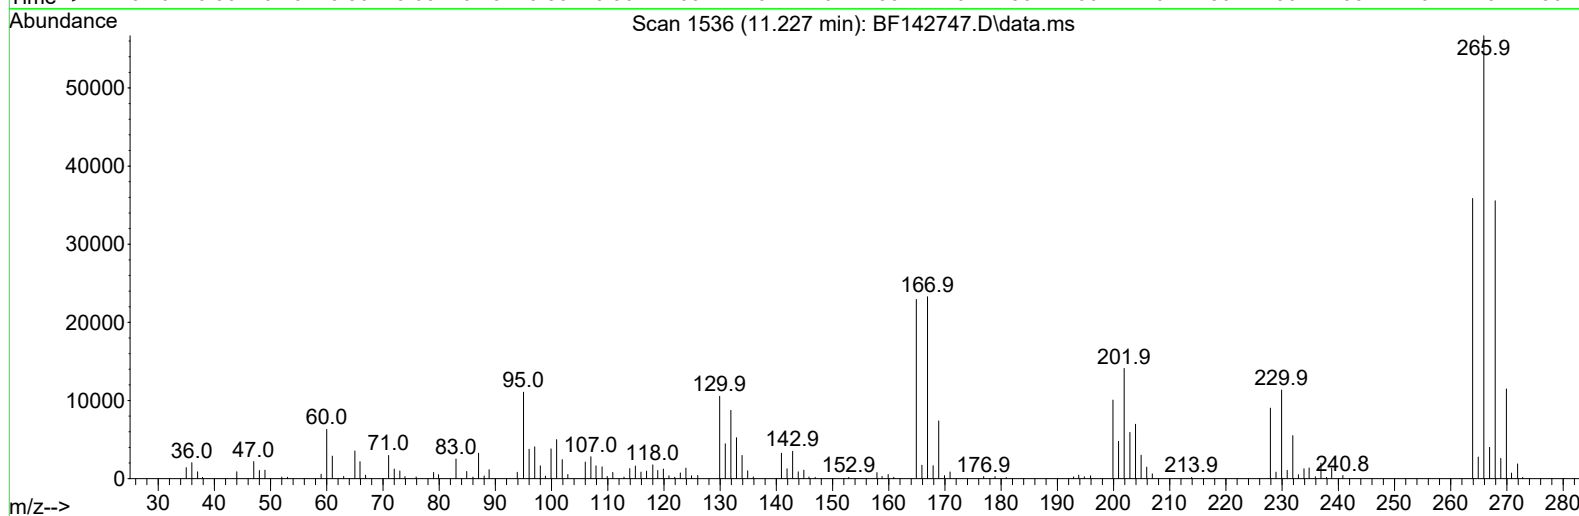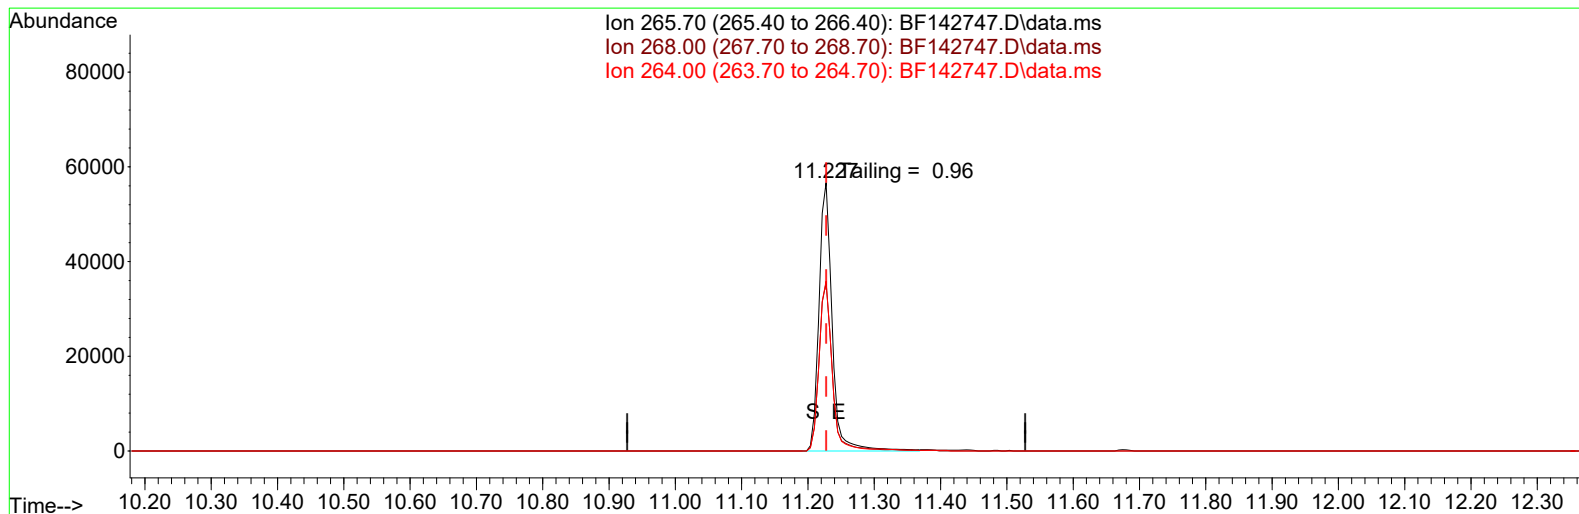

TIC: BF142747.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 48564.59 ng

response 78719

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	62.77
264.00	61.90	63.25
0.00	0.00	0.00