

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
 Data File : BF142749.D
 Acq On : 12 Jun 2025 10:56
 Operator : RC/JU
 Sample : PB168376BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168376BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	492	499	511	rBV	118605	192643	7.69%	1.354%
2	5.516	559	565	571	rBV	1348138	1890379	75.46%	13.283%
3	6.516	729	735	741	rBV	1278928	1839126	73.41%	12.923%
4	6.887	793	798	804	rBV	333987	416833	16.64%	2.929%
5	7.451	887	894	899	rBV	881547	1232777	49.21%	8.662%
6	8.175	1011	1017	1037	rBV	407246	546823	21.83%	3.842%
7	9.251	1193	1200	1205	rBV	1873114	2505133	100.00%	17.603%
8	9.928	1310	1315	1335	rVB	467551	623496	24.89%	4.381%
9	10.722	1444	1450	1469	rBV	1147466	1486526	59.34%	10.446%
10	11.422	1563	1569	1576	rBV	470555	605766	24.18%	4.257%
11	13.010	1833	1839	1844	rBV	1587702	2093699	83.58%	14.712%
12	14.063	2013	2018	2030	rVB	286942	382584	15.27%	2.688%
13	15.557	2266	2272	2292	rVB	223714	378858	15.12%	2.662%
14	17.286	2557	2566	2582	rBV3	8206	36590	1.46%	0.257%




Sum of corrected areas: 14231233

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142749.D
Acq On : 12 Jun 2025 10:56
Operator : RC/JU
Sample : PB168376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

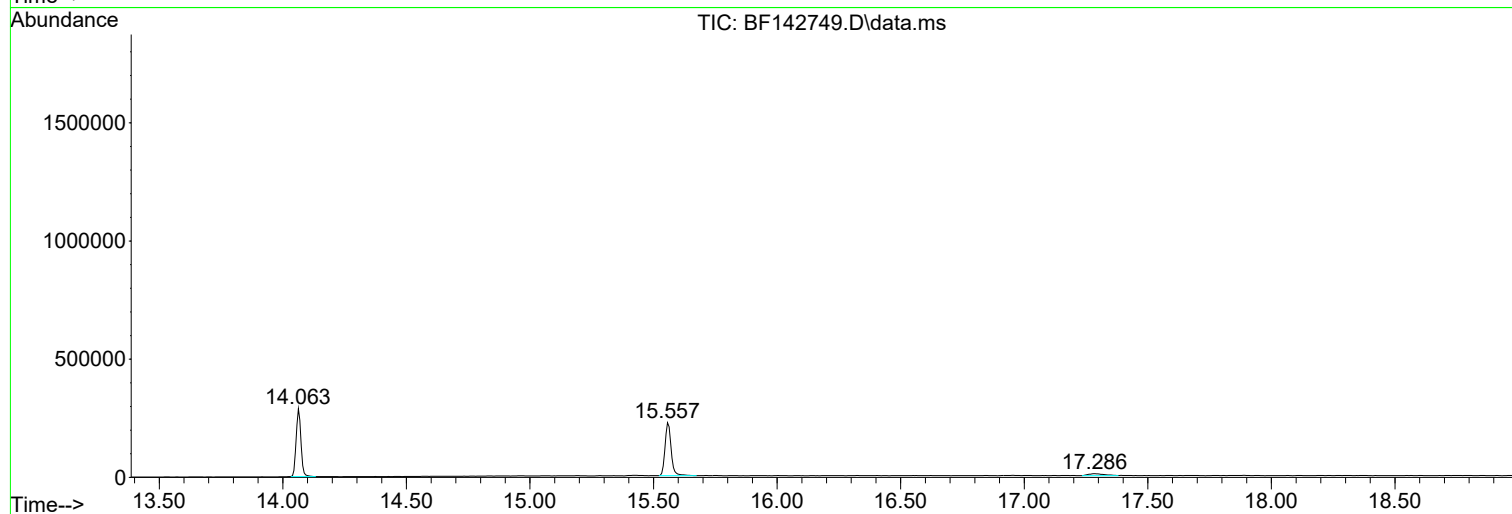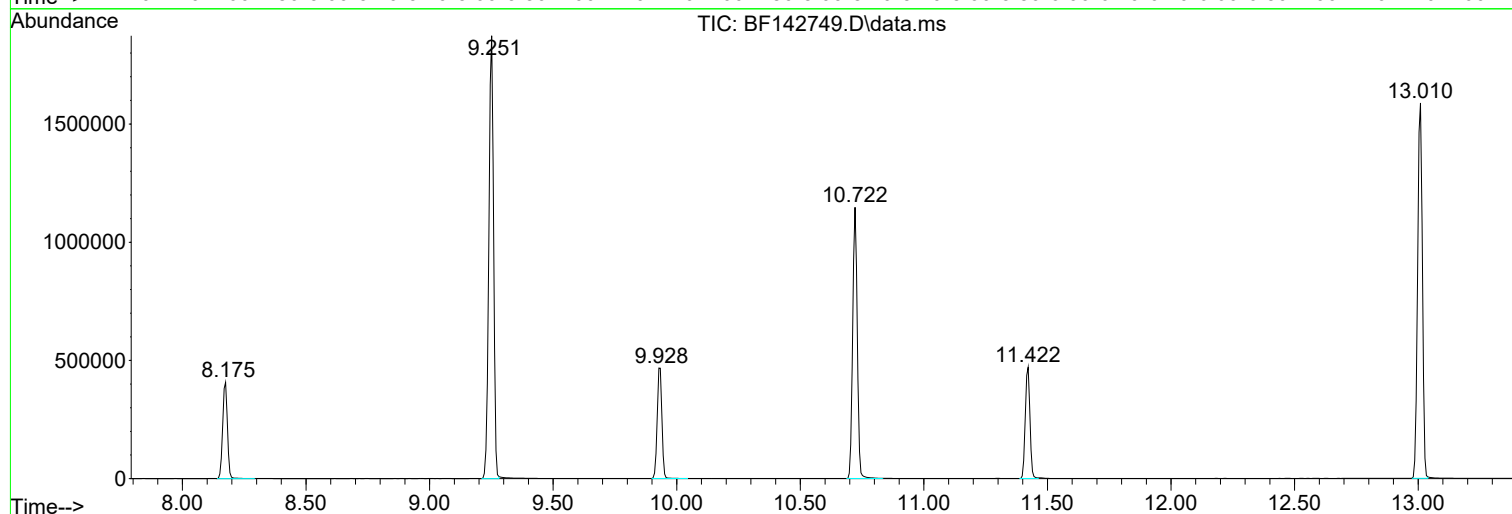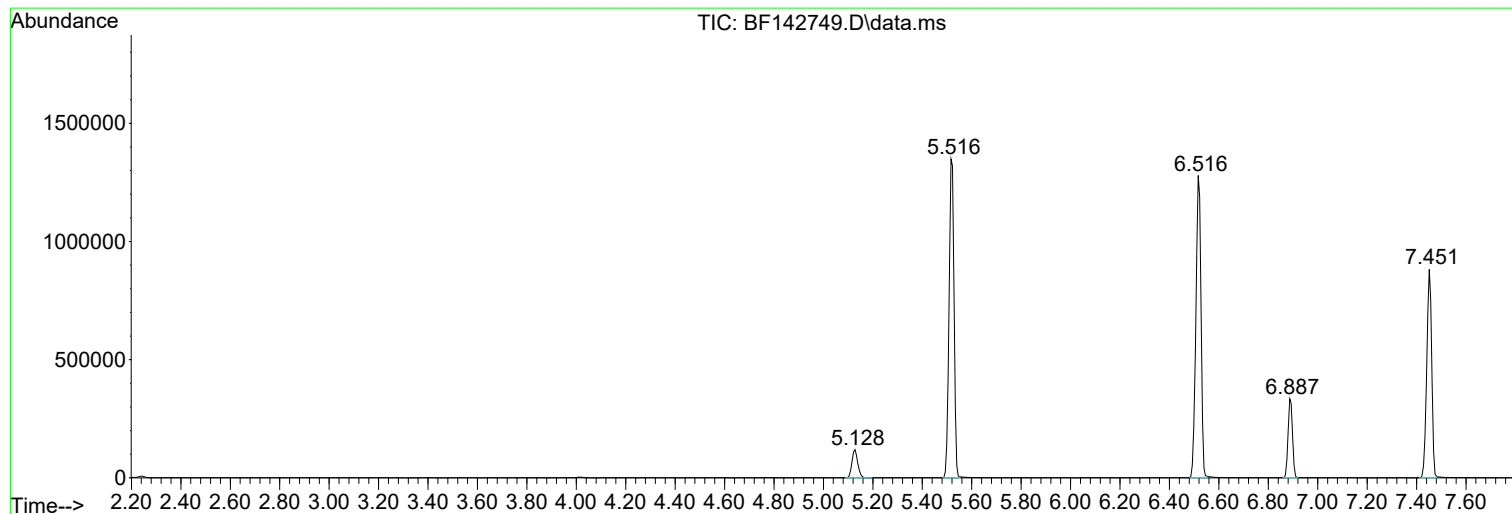

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142749.D
Acq On : 12 Jun 2025 10:56
Operator : RC/JU
Sample : PB168376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1









Instrument :
BNA_F
ClientSampleId :
PB168376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.128	9.24 ng	192643	1,4-Dichlorobenzene-d4			6.887
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	50
2	3-Hexanol, 4-methyl-		116	C7H16O	000615-29-2	28
3	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	23
4	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
5	Butane, 1-ethoxy-		102	C6H14O	000628-81-9	9

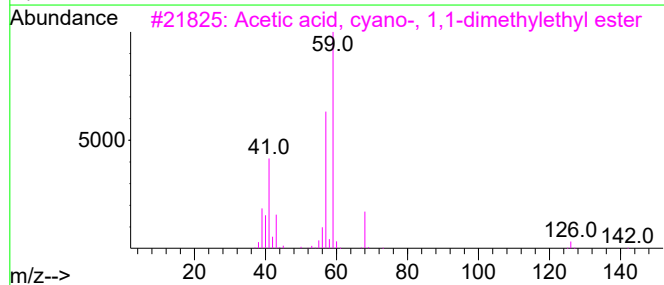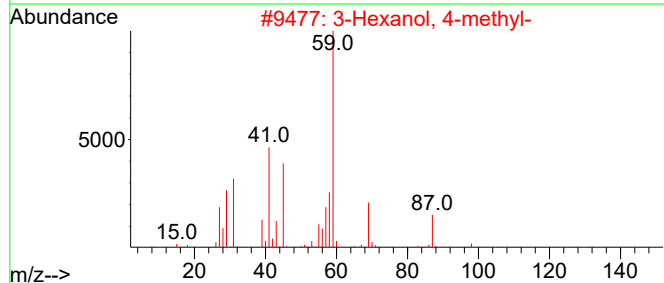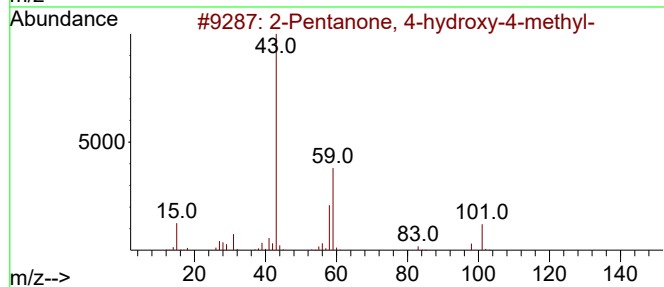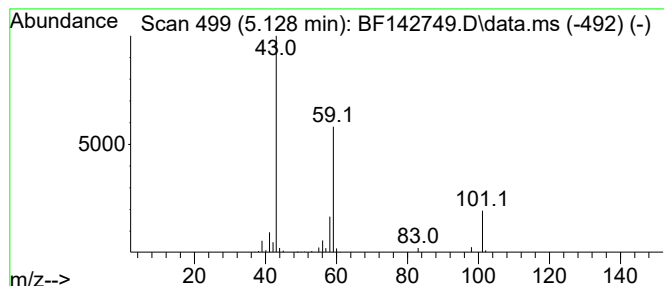

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF0611225\
Data File : BF142749.D
Acq On : 12 Jun 2025 10:56
Operator : RC/JU
Sample : PB168376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.128	9.2	ng	192643	1	6.887	416833	20.0