

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
 Data File : BF142751.D
 Acq On : 12 Jun 2025 11:54
 Operator : RC/JU
 Sample : PB168412BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168412BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	492	499	514	rVB	120224	198377	7.83%	1.388%
2	5.516	559	565	571	rBV	1383906	1940420	76.56%	13.577%
3	6.516	729	735	741	rBV	1288212	1893306	74.70%	13.247%
4	6.887	793	798	804	rBV	321597	404739	15.97%	2.832%
5	7.451	887	894	899	rBV	909899	1267898	50.03%	8.871%
6	8.175	1011	1017	1038	rBV	388664	523318	20.65%	3.662%
7	9.251	1193	1200	1205	rBV	1890683	2534398	100.00%	17.733%
8	9.928	1310	1315	1333	rVB	459867	589114	23.24%	4.122%
9	10.722	1444	1450	1471	rBV	1157673	1510498	59.60%	10.569%
10	11.422	1563	1569	1576	rBV	424613	567606	22.40%	3.971%
11	13.010	1833	1839	1844	rBV	1568608	2126218	83.89%	14.877%
12	14.063	2013	2018	2034	rBV	273458	366314	14.45%	2.563%
13	15.557	2266	2272	2291	rBV	219823	369909	14.60%	2.588%




Sum of corrected areas: 14292115

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142751.D
Acq On : 12 Jun 2025 11:54
Operator : RC/JU
Sample : PB168412BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

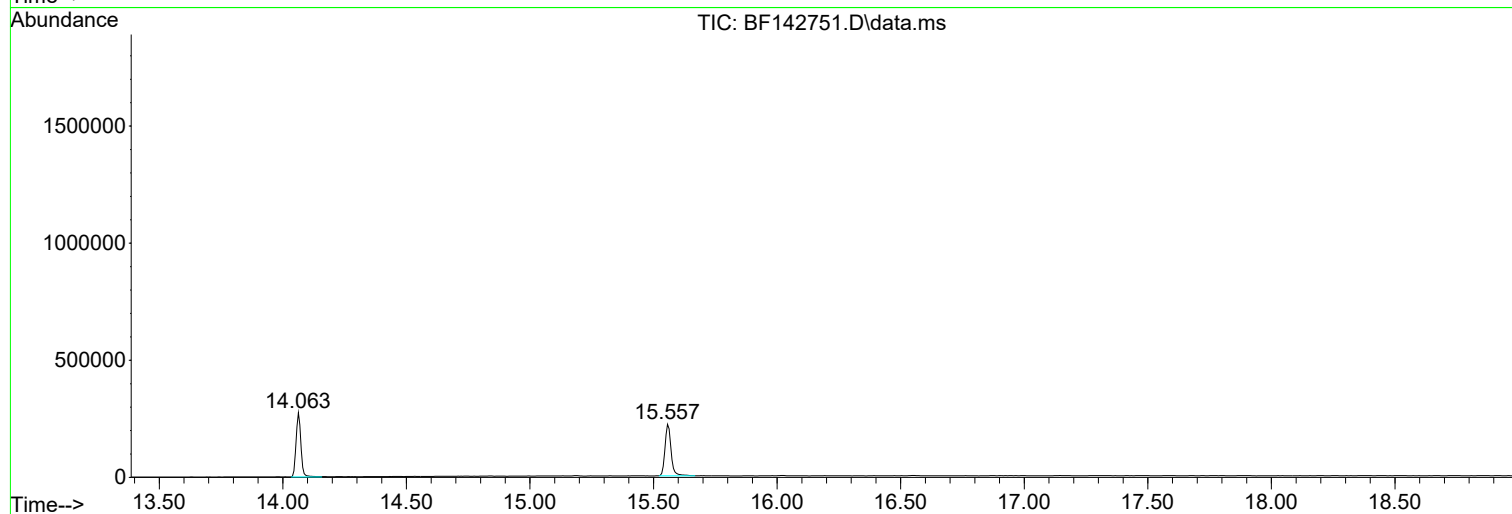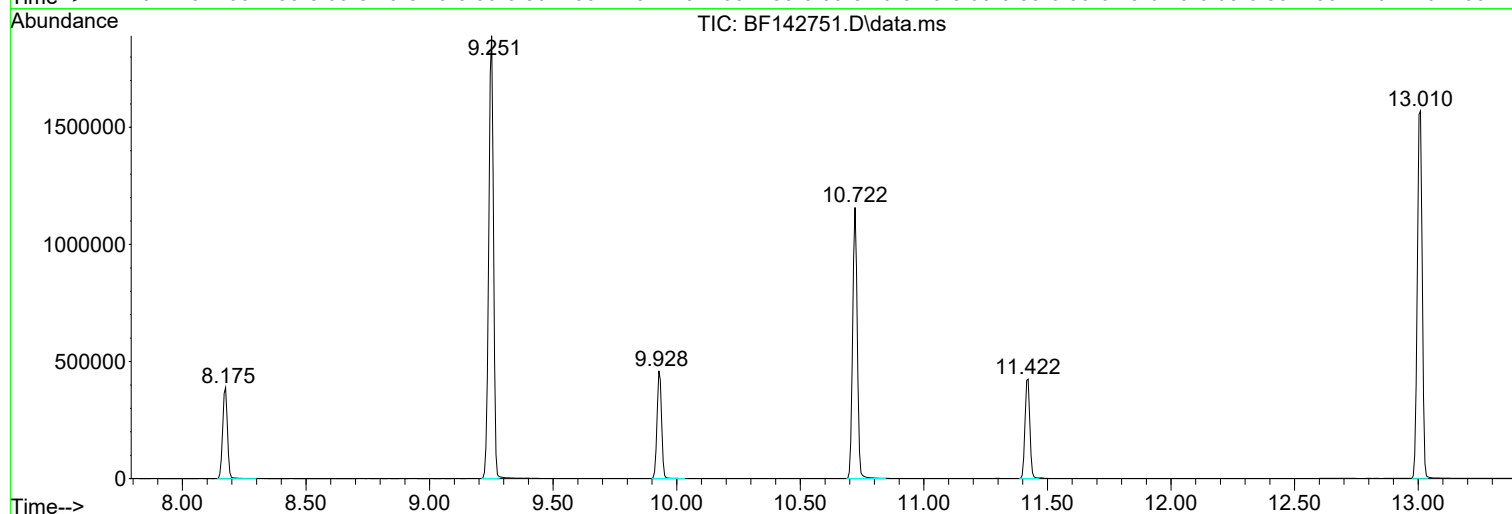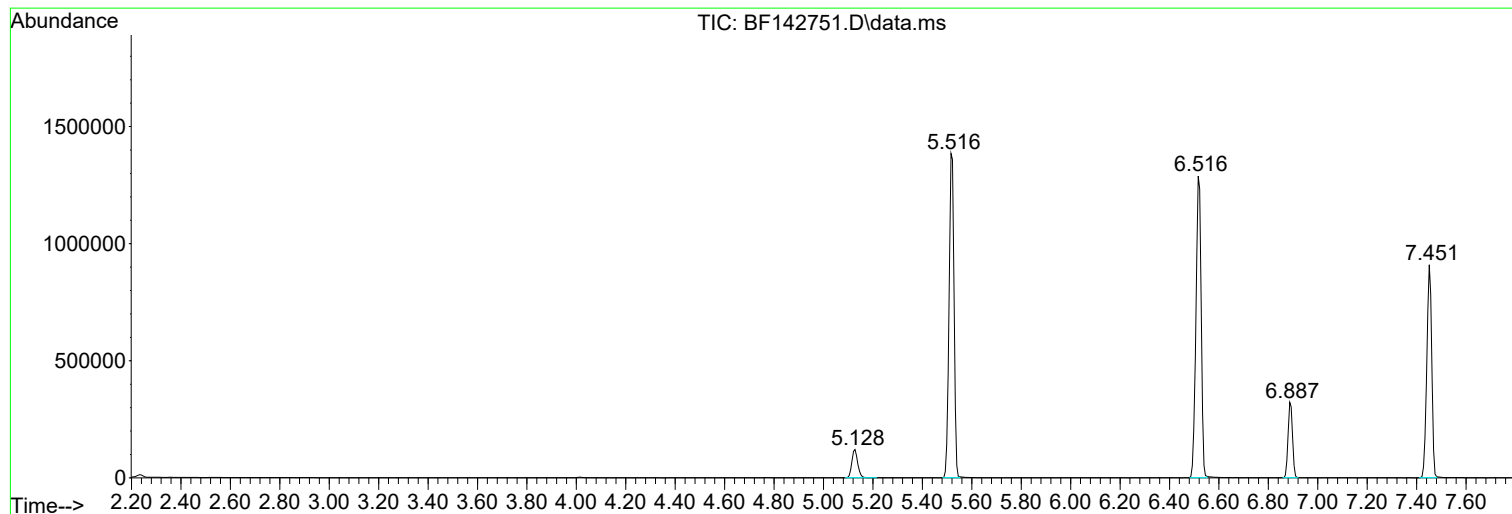

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142751.D
Acq On : 12 Jun 2025 11:54
Operator : RC/JU
Sample : PB168412BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB168412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.128	9.80 ng	198377	1,4-Dichlorobenzene-d4			6.887
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	56
2	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	25
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
4	Morpholine, 4-methyl-		101	C5H11NO	000109-02-4	9
5	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9

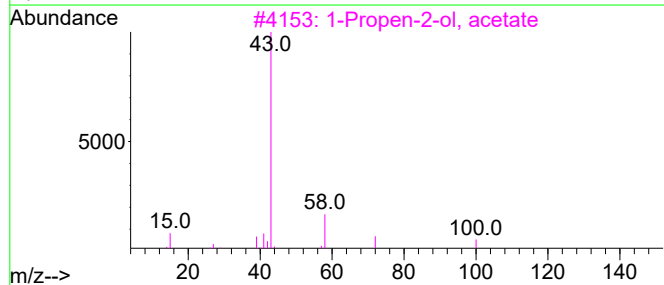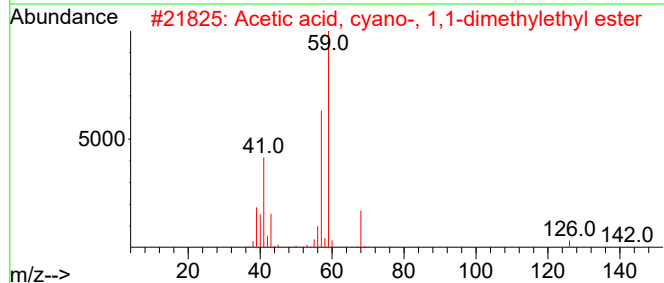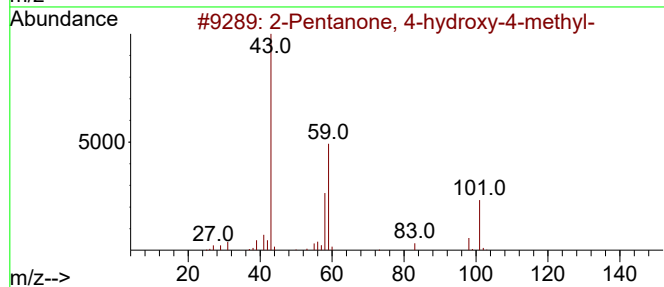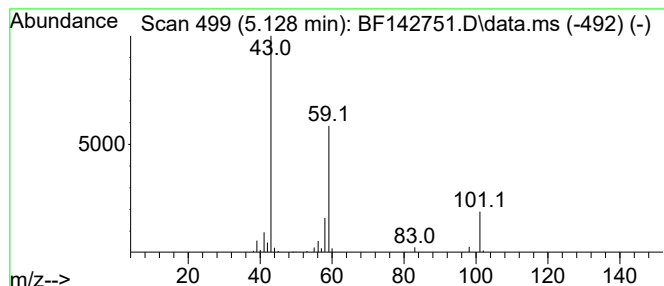

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF0611225\
Data File : BF142751.D
Acq On : 12 Jun 2025 11:54
Operator : RC/JU
Sample : PB168412BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.128	9.8	ng	198377	1	6.887	404739	20.0