

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
 Data File : BF142769.D
 Acq On : 12 Jun 2025 20:56
 Operator : RC/JU
 Sample : Q2278-01 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	293	300	307	rVB2	2338	3856	1.03%	0.152%
2	4.616	409	412	415	rBV	4323	5065	1.35%	0.200%
3	5.098	487	494	503	rBV	6627	10087	2.69%	0.399%
4	5.504	556	563	574	rBV	64359	90951	24.24%	3.594%
5	6.516	730	735	750	rBV	55196	77313	20.61%	3.055%
6	6.722	765	770	774	rBV2	3042	4047	1.08%	0.160%
7	6.892	794	799	806	rBV	198106	240556	64.12%	9.505%
8	7.451	889	894	905	rBV	32466	46883	12.50%	1.852%
9	8.175	1010	1017	1025	rBV	207985	267276	71.24%	10.560%
10	8.228	1025	1026	1040	rVB4	2217	4073	1.09%	0.161%
11	9.251	1195	1200	1209	rBV	74462	94704	25.24%	3.742%
12	9.328	1209	1213	1219	rVB3	3556	5155	1.37%	0.204%
13	9.857	1296	1303	1309	rVB3	3146	5248	1.40%	0.207%
14	9.933	1311	1316	1328	rVB	245251	301216	80.28%	11.902%
15	10.357	1381	1388	1392	rBV3	3531	6149	1.64%	0.243%
16	10.639	1431	1436	1443	rBV	6397	9403	2.51%	0.372%
17	10.722	1443	1450	1457	rBV	44633	56558	15.07%	2.235%
18	10.839	1465	1470	1475	rBV2	6464	10700	2.85%	0.423%
19	11.280	1540	1545	1549	rBV4	3865	6552	1.75%	0.259%
20	11.422	1564	1569	1577	rBV	284356	375185	100.00%	14.824%
21	11.498	1580	1582	1589	rVB3	2931	4020	1.07%	0.159%
22	11.663	1605	1610	1614	rBV5	2447	4308	1.15%	0.170%
23	11.710	1614	1618	1623	rVB3	3384	4753	1.27%	0.188%
24	11.945	1651	1658	1665	rBV3	8246	19610	5.23%	0.775%
25	12.033	1670	1673	1682	rVB7	5757	13373	3.56%	0.528%
26	12.116	1683	1687	1690	rBV	3744	4694	1.25%	0.185%
27	12.222	1702	1705	1708	rBV	2881	4613	1.23%	0.182%
28	12.404	1732	1736	1737	rBV3	3119	3913	1.04%	0.155%
29	12.474	1744	1748	1750	rBV2	7752	10105	2.69%	0.399%
30	12.504	1750	1753	1760	rVB7	6174	11411	3.04%	0.451%
31	12.639	1772	1776	1781	rBV	29700	39704	10.58%	1.569%
32	12.733	1789	1792	1794	rBV4	2771	3999	1.07%	0.158%
33	12.869	1809	1815	1820	rBV	31375	52044	13.87%	2.056%
34	13.004	1834	1838	1846	rVB	107813	146819	39.13%	5.801%
35	14.068	2014	2019	2030	rBV	240194	357574	95.31%	14.128%
36	15.568	2269	2274	2283	rVB	136680	228987	61.03%	9.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142769.D
Acq On : 12 Jun 2025 20:56
Operator : RC/JU
Sample : Q2278-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 2530904

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142769.D
Acq On : 12 Jun 2025 20:56
Operator : RC/JU
Sample : Q2278-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

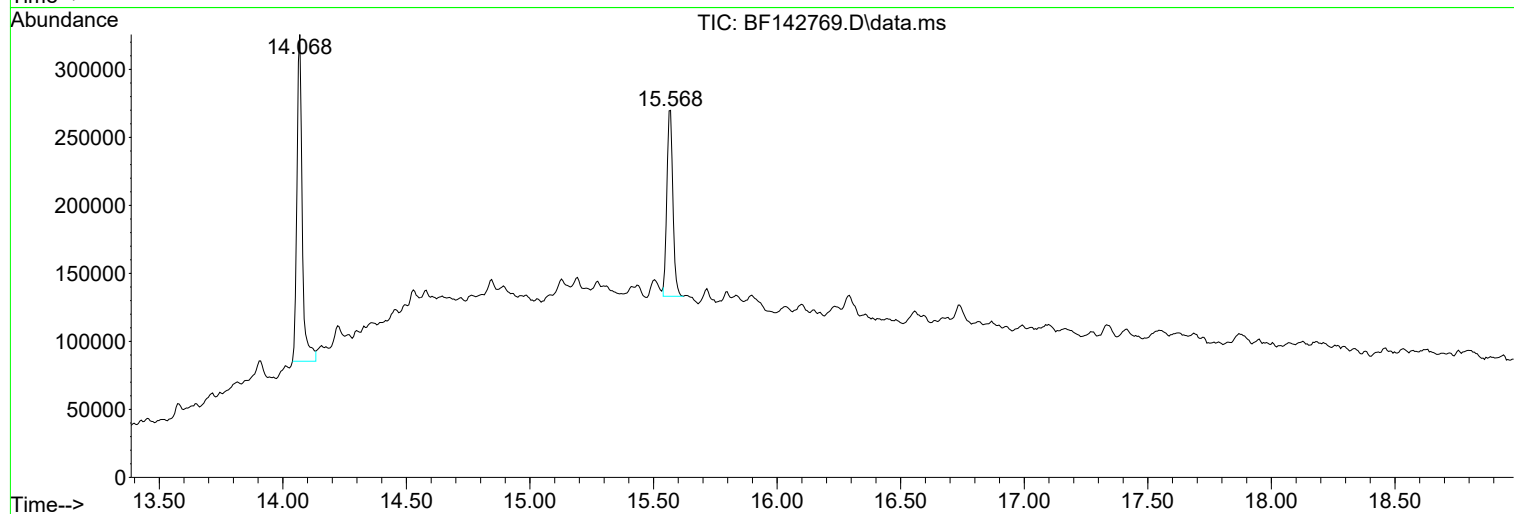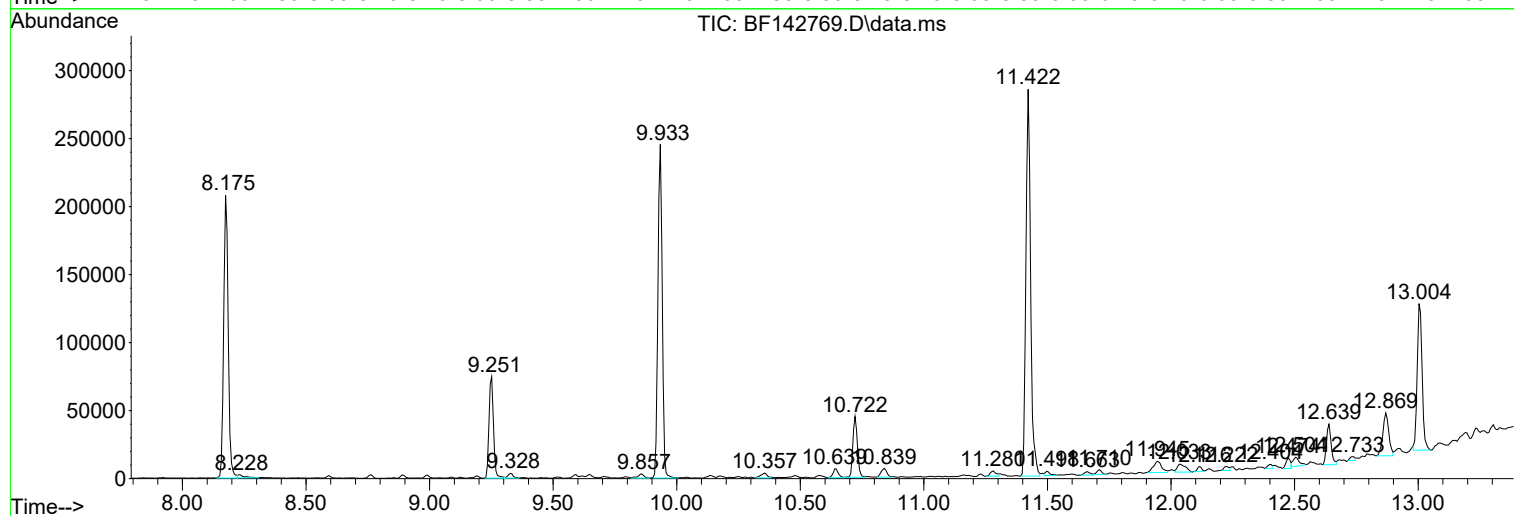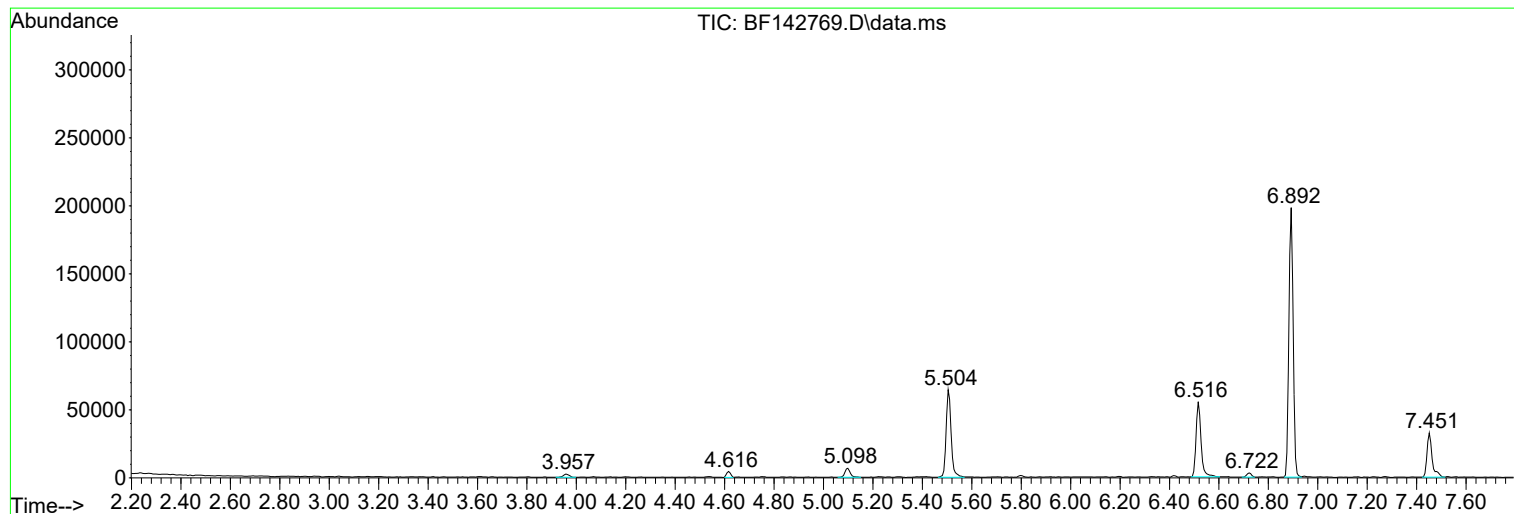

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142769.D
Acq On : 12 Jun 2025 20:56
Operator : RC/JU
Sample : Q2278-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF0611225\
Data File : BF142769.D
Acq On : 12 Jun 2025 20:56
Operator : RC/JU
Sample : Q2278-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------