
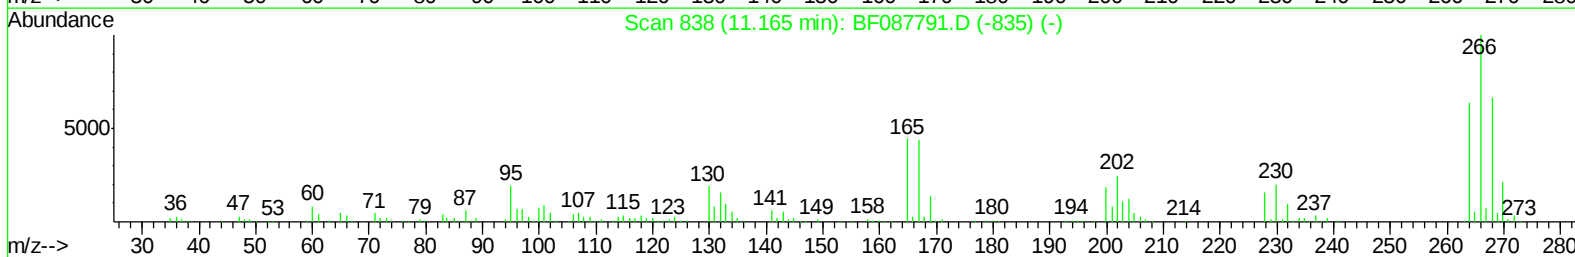
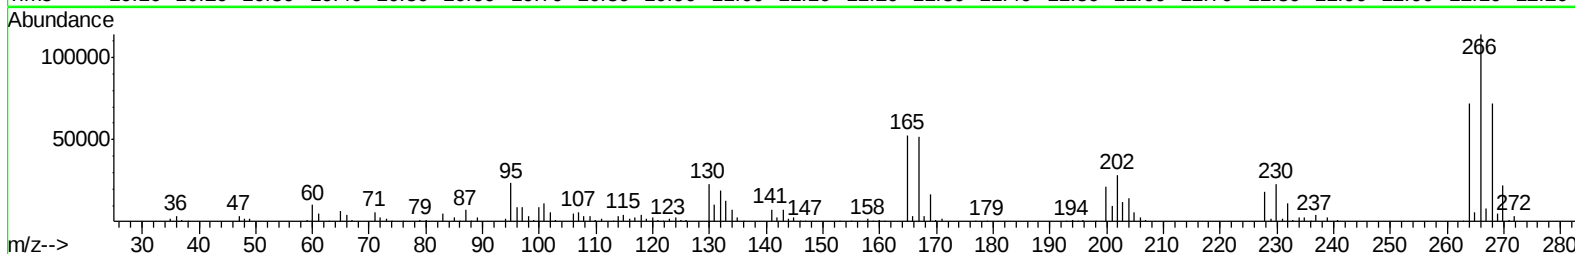


Data Path : Z:\HPCHEM1\BNA F\Data\BF061316\
Data File : BF087995.D
Acq On : 14 Jun 2016 8:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 16:06:52 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

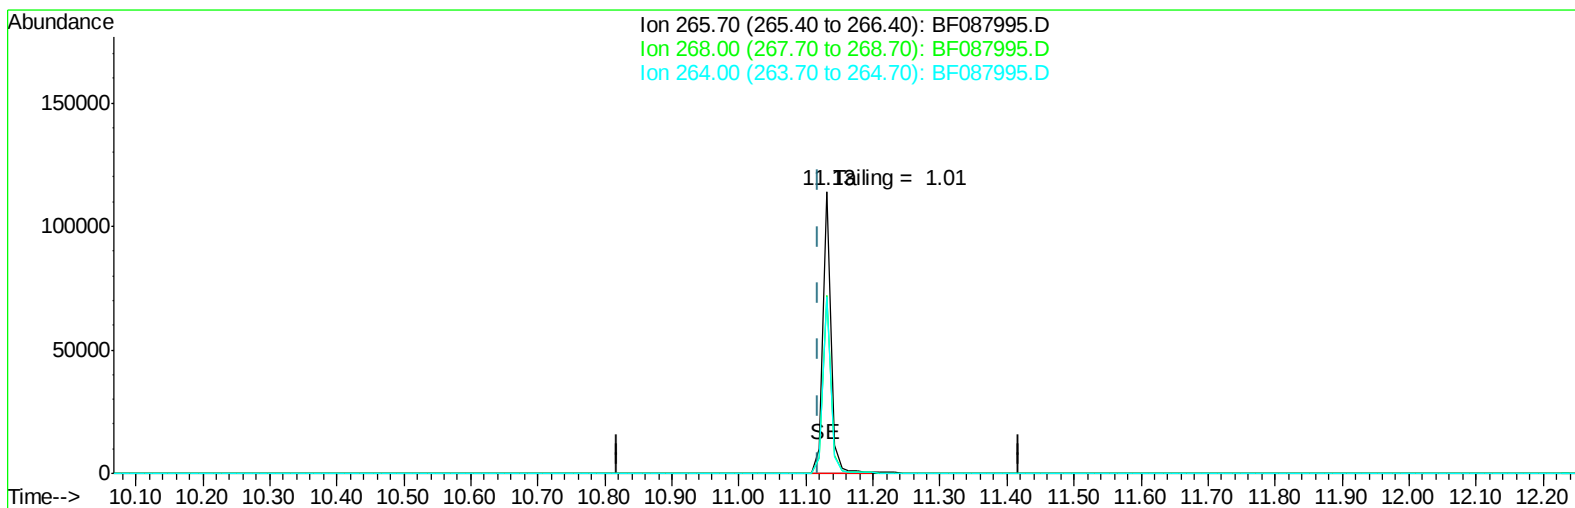

TIC: BF087995.D

(69) Pentachlorophenol (C)




11.130min (+0.011) 0.00ng

response 97078

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.25
264.00	62.00	62.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF061316\
Data File : BF087995.D
Acq On : 14 Jun 2016 8:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 16:06:52 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

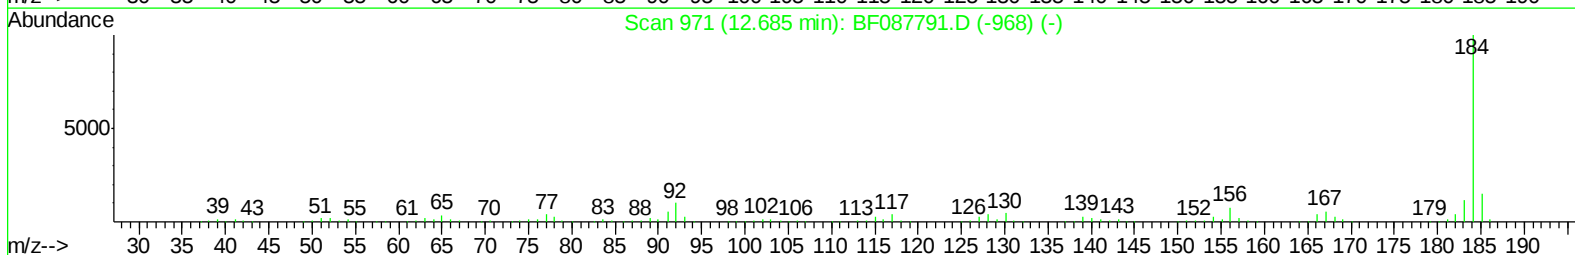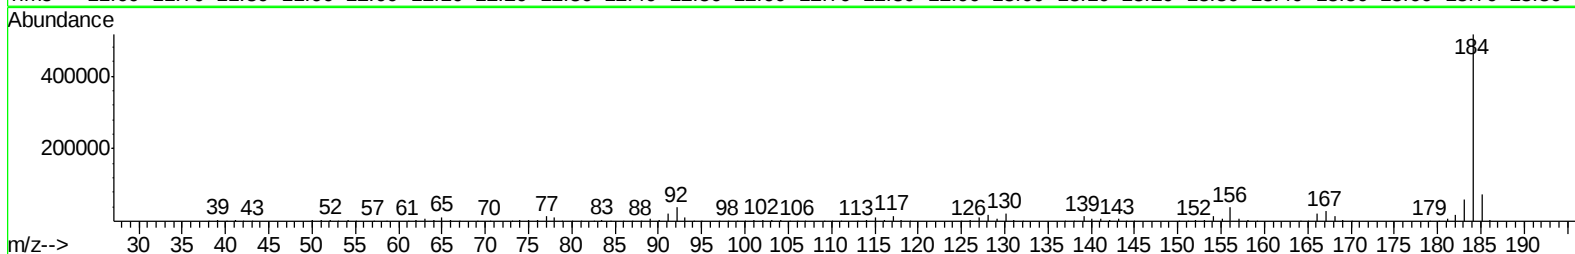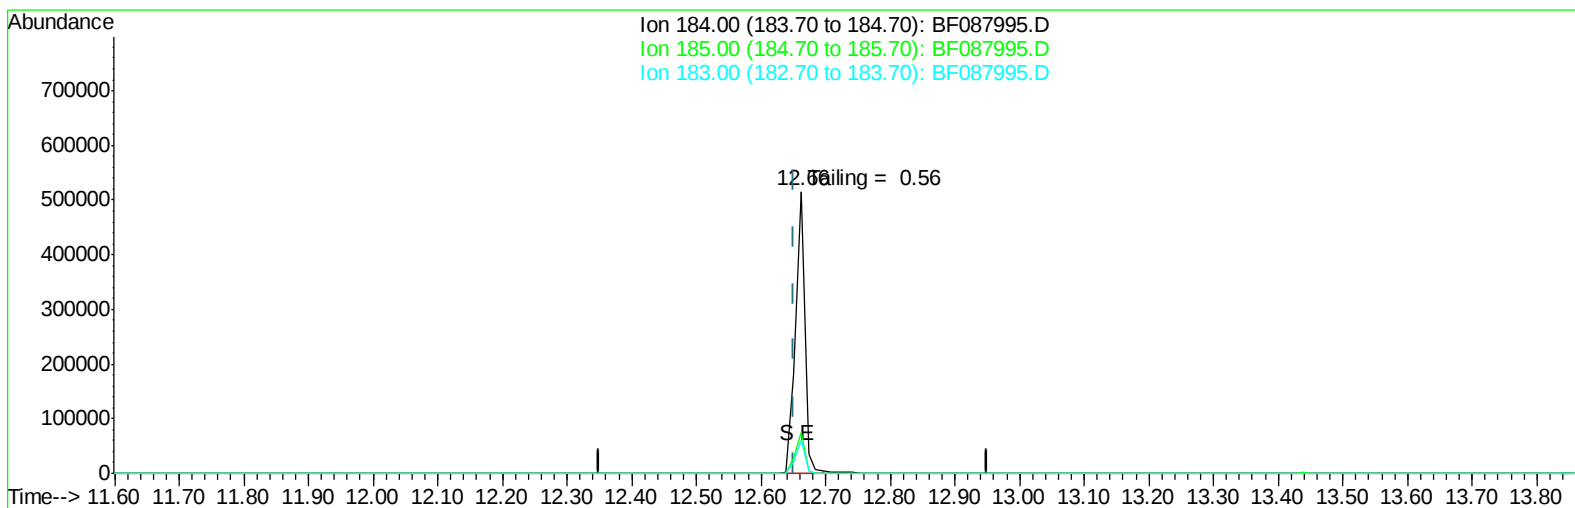

TIC: BF087995.D

(76) Benzidine

12.662min (+0.011) 9807.14ng

response 521376

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.44
183.00	11.60	11.67
0.00	0.00	0.00