


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061316\
 Data File : BF087975.D
 Acq On : 13 Jun 2016 10:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 14:10:49 2016

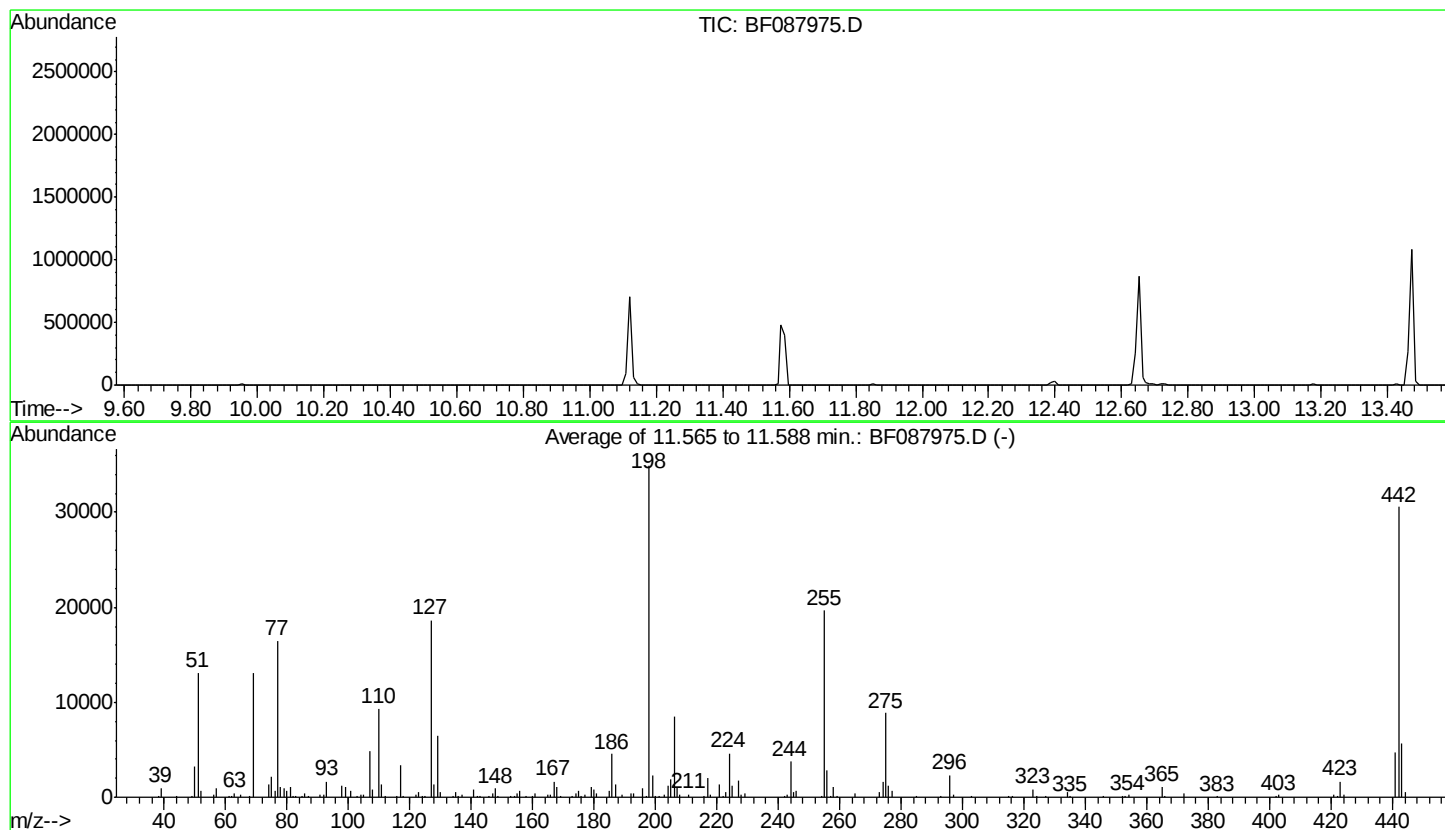

AutoFind: Scans 873, 874, 875; Background Corrected with Scan 870

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	13078	PASS
68	69	0.00	2	1.2	162	PASS
69	198	0.00	100	37.6	13141	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	18648	PASS
197	198	0.00	2	0.4	153	PASS
198	198	100	100	100.0	34921	PASS
199	198	5	9	6.7	2323	PASS
275	198	10	60	25.4	8863	PASS
365	198	1	100	3.2	1132	PASS
441	442	0.01	24	15.4	4712	PASS
442	198	50	100	87.5	30558	PASS
443	442	15	24	18.7	5710	PASS