


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061316\
 Data File : BF087995.D
 Acq On : 14 Jun 2016 8:17
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 14:10:49 2016

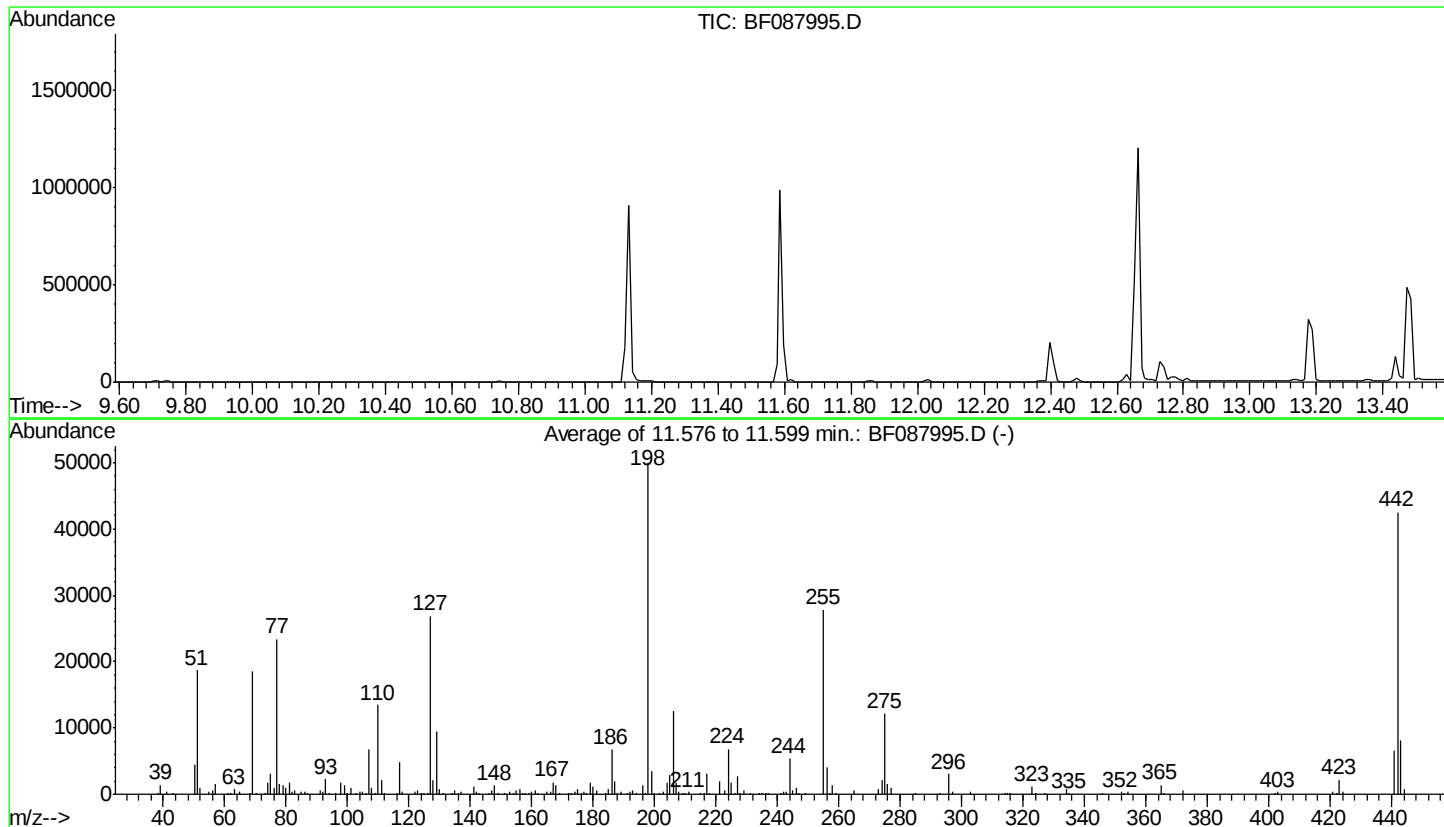

AutoFind: Scans 874, 875, 876; Background Corrected with Scan 871

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	18694	PASS
68	69	0.00	2	1.4	265	PASS
69	198	0.00	100	37.1	18530	PASS
70	69	0.00	2	0.7	127	PASS
127	198	10	80	53.9	26933	PASS
197	198	0.00	2	0.5	272	PASS
198	198	100	100	100.0	50004	PASS
199	198	5	9	6.8	3392	PASS
275	198	10	60	24.3	12158	PASS
365	198	1	100	2.8	1418	PASS
441	442	0.01	24	15.5	6579	PASS
442	198	50	100	84.9	42478	PASS
443	442	15	24	19.0	8051	PASS