

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
 Data File : BF095913.D
 Acq On : 14 Jun 2017 1:39
 Operator : SJ/MA
 Sample : I3624-04 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NB-RO6822-060917

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.540	499	502	511	rBV2	5790	14056	2.31%	0.279%
2	5.275	624	627	655	rBV	56092	207432	34.09%	4.115%
3	6.951	909	912	921	rBV3	58899	161199	26.49%	3.198%
4	7.022	921	924	945	rVB	137750	342777	56.33%	6.800%
5	7.351	975	980	996	rBV	341318	463419	76.15%	9.193%
6	7.587	1016	1020	1036	rBV	143888	216799	35.62%	4.301%
7	8.281	1135	1138	1157	rBV	51588	130165	21.39%	2.582%
8	9.380	1321	1325	1343	rBV	448514	608566	100.00%	12.072%
9	11.157	1623	1627	1650	rBV	236957	300061	49.31%	5.952%
10	11.869	1744	1748	1754	rBV	9013	13499	2.22%	0.268%
11	12.204	1800	1805	1817	rBV2	470932	600375	98.65%	11.909%
12	13.510	2024	2027	2042	rBB2	63573	99770	16.39%	1.979%
13	13.827	2077	2081	2090	rBB	3764	6357	1.04%	0.126%
14	14.598	2208	2212	2225	rVB	383523	512452	84.21%	10.165%
15	15.562	2372	2376	2382	rVB3	3842	7574	1.24%	0.150%
16	16.221	2481	2488	2491	rBV2	4521	7386	1.21%	0.147%
17	16.421	2517	2522	2528	rBV	34637	43794	7.20%	0.869%
18	16.727	2570	2574	2579	rBV	46741	61976	10.18%	1.229%
19	16.968	2611	2615	2620	rBV	220199	231214	37.99%	4.587%
20	17.162	2646	2648	2651	rBV4	6258	7488	1.23%	0.149%
21	17.698	2735	2739	2742	rBV5	5847	9542	1.57%	0.189%
22	18.127	2810	2812	2816	rBV4	5302	7590	1.25%	0.151%
23	18.174	2818	2820	2825	rVB6	14165	15063	2.48%	0.299%
24	18.239	2828	2831	2836	rBV7	13732	23386	3.84%	0.464%
25	18.321	2839	2845	2854	rBV	428041	579037	95.15%	11.486%
26	19.992	3125	3129	3137	rVB	296648	370195	60.83%	7.343%


Sum of corrected areas: 5041172

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
Data File : BF095913.D
Acq On : 14 Jun 2017 1:39
Operator : SJ/MA
Sample : I3624-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-RO6822-060917

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

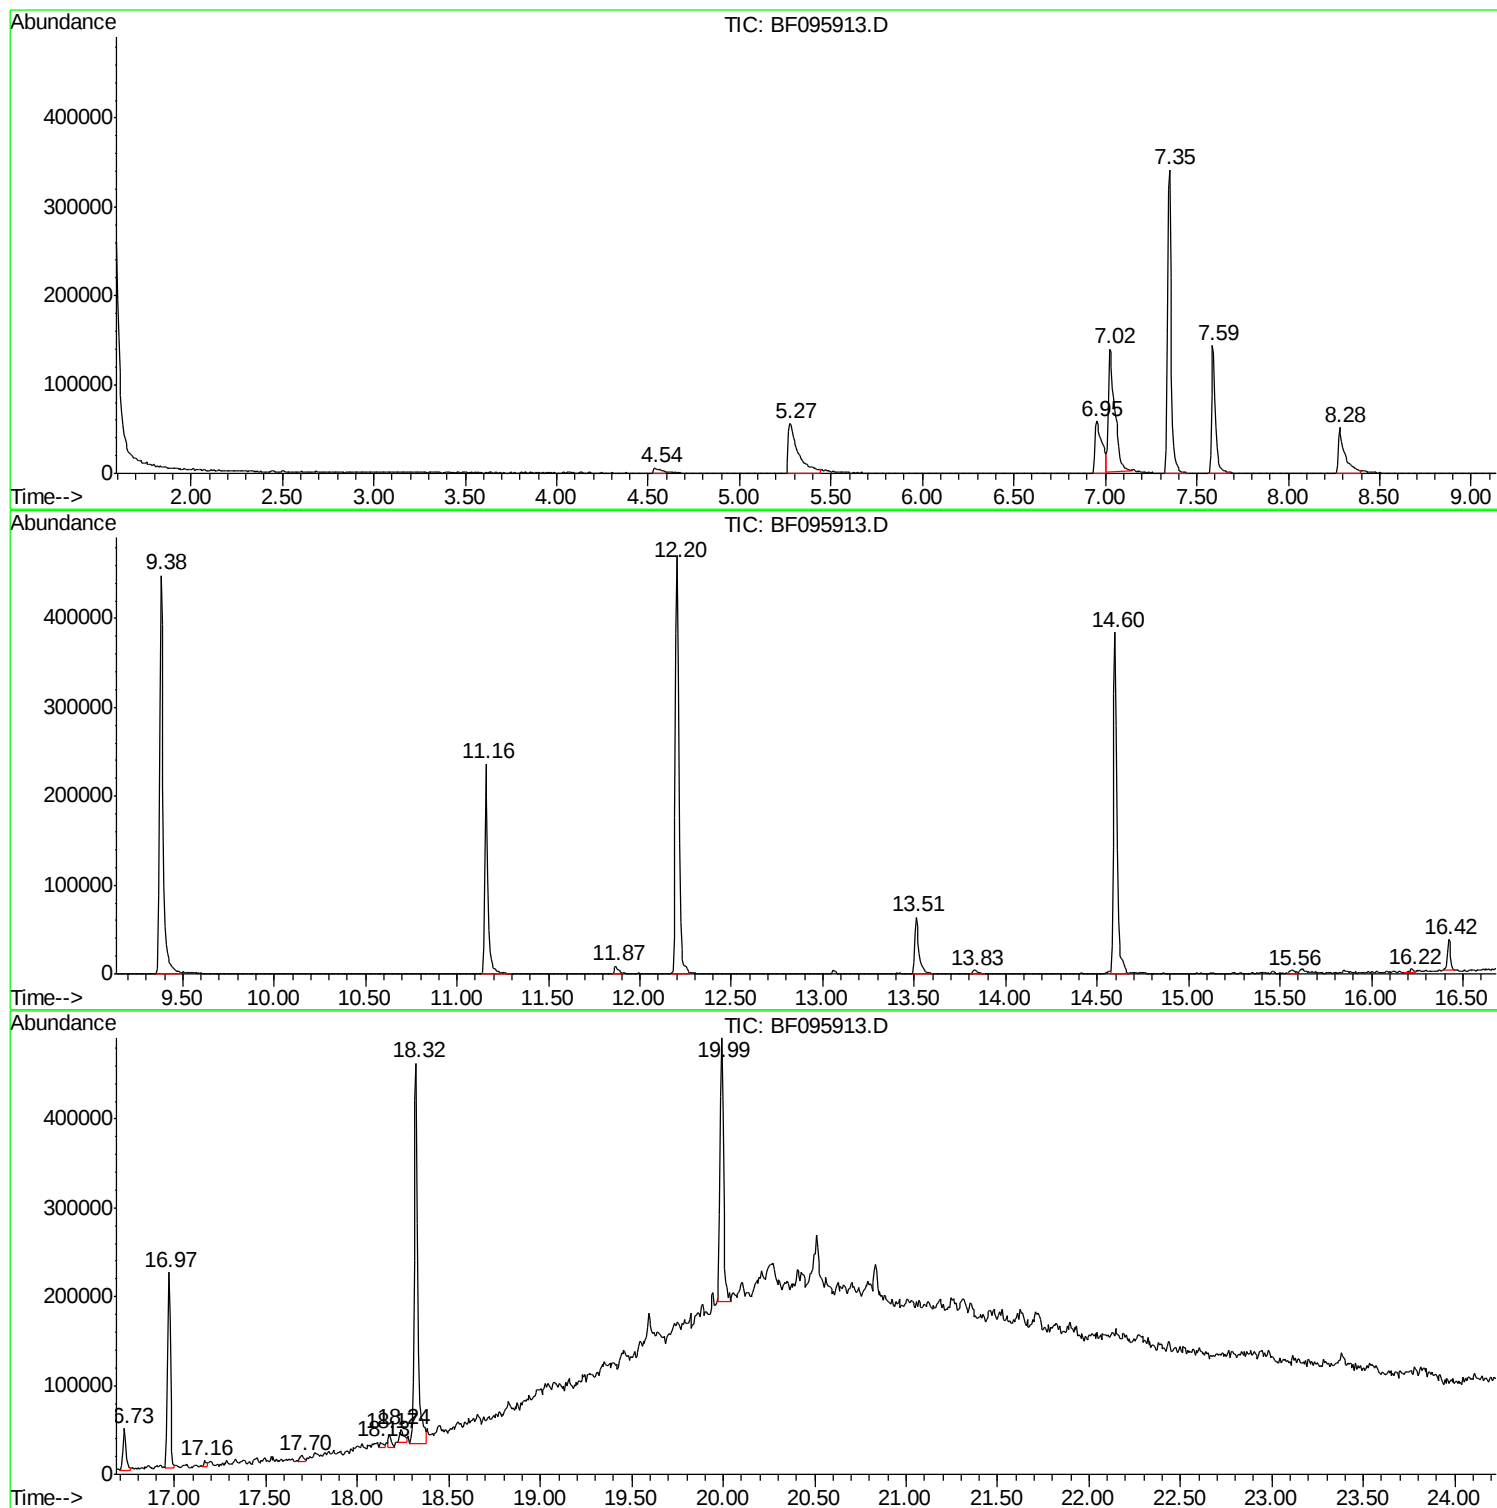

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
Data File : BF095913.D
Acq On : 14 Jun 2017 1:39
Operator : SJ/MA
Sample : I3624-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-RO6822-060917










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.02 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.02	14.79 ng	342777	1,4-Dichlorobenzene-d4	7.35

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		N-(1,2,3,4-Tetrahydro-isoquinoli...	302	C16H18N2O2S	1000274-62-8	10
3		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
4		1-Aminoindan	133	C9H11N	034698-41-4	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

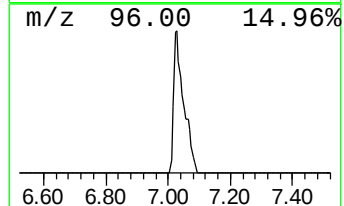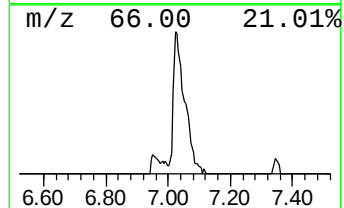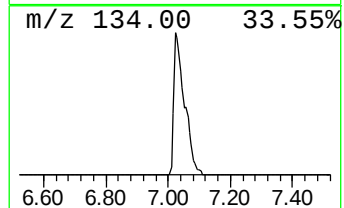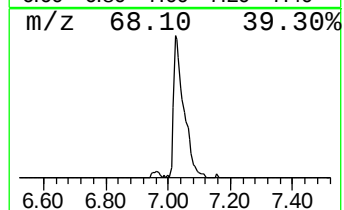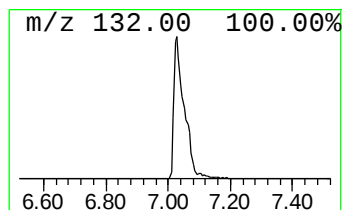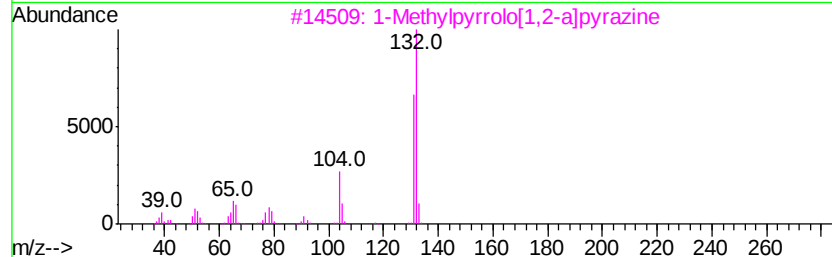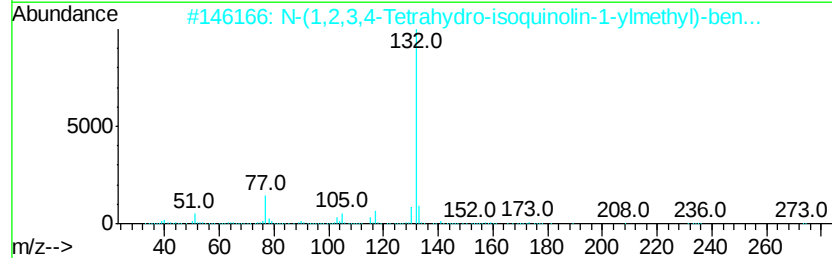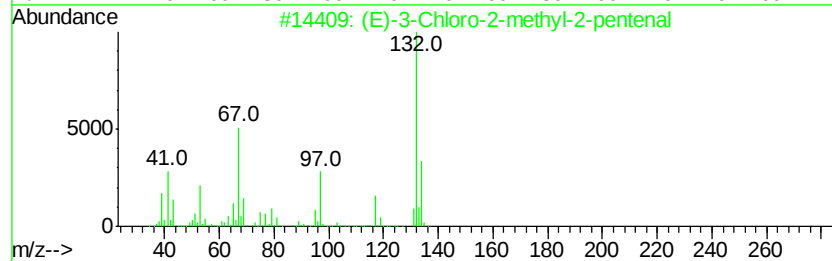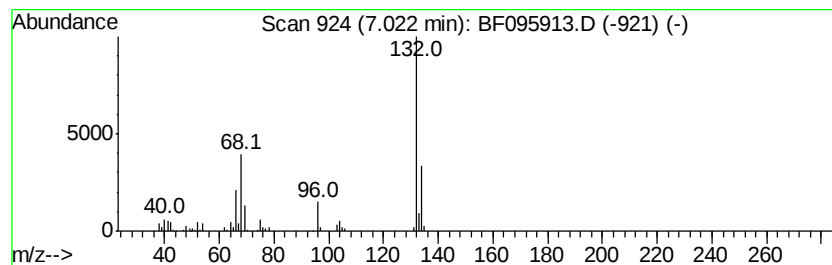

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
Data File : BF095913.D
Acq On : 14 Jun 2017 1:39
Operator : SJ/MA
Sample : I3624-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-RO6822-060917

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.02	7.02	14.8	ng	342777	1	7.35	463419	20.0